

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031716\
 Data File : BM004665.D
 Acq On : 17 Mar 2016 14:19
 Operator : UM/SJ
 Sample : H1783-04
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 18 05:07:14 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 18 05:06:10 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	33298	20.00	ng/ul	0.03
18) Naphthalene-d8	10.66	136	288346	20.00	ng/ul	0.02
36) Acenaphthene-d10	14.47	164	153104	20.00	ng/ul	0.00
62) Phenanthrene-d10	17.22	188	338284	20.00	ng/ul	0.00
78) Chrysene-d12	21.40	240	366990	20.00	ng/ul	0.00
86) Perylene-d12	23.70	264	355472	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.34	96	2086	2.16	ng/uL	0.00
5) Phenol-d5	7.00	99	41377	15.12	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.20	67	110400	71.19	ng/ul	0.02
9) 2-Chlorophenol-d4	7.39	132	124017	56.30	ng/ul	0.01
13) 4-Methylphenol-d8	8.55	113	77450	35.12	ng/ul	0.00
19) Nitrobenzene-d5	9.01	128	73645	36.72	ng/ul	0.01
22) 2-Nitrophenol-d4	9.72	143	79021	36.48	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.26	165	131752	31.01	ng/ul	0.00
29) 4-Chloroaniline-d4	10.79	131	1066	0.21	ng/ul	0.02
44) Dimethylphthalate-d6	13.89	166	430493	35.97	ng/ul	0.00
47) Acenaphthylene-d8	14.17	160	537028	36.60	ng/ul	0.00
52) 4-Nitrophenol-d4	14.66	143	15868	6.86	ng/ul	0.00
58) Fluorene-d10	15.47	176	373965	35.85	ng/ul	0.00
63) 4,6-Dinitro-2-methylphenol	15.58	200	59376	33.40	ng/ul	0.00
71) Anthracene-d10	17.32	188	579962	37.24	ng/ul	0.00
79) Pyrene-d10	19.61	212	651429	38.89	ng/ul	0.00
90) Benzo(a)pyrene-d12	23.56	264	668320	42.09	ng/ul	0.00

Target Compounds


						Ovalue
2) 1,4-Dioxane	3.37	88	1562	1.39	ng/uL#	86
10) 2-Chlorophenol	7.42	128	4795	2.06	ng/ul#	80
11) 2-Methylphenol	8.24	108	30811	13.93	ng/ul	92
20) Nitrobenzene	9.06	77	594976	120.24	ng/ul	98
23) 2-Nitrophenol	9.76	139	27308	11.38	ng/ul	93
32) Caprolactam	11.45	113	36833	25.12	ng/ul#	1
37) 1,2,4,5-Tetrachlorobenzene	12.66	216	142896	29.21	ng/ul	98
42) 2-Chloronaphthalene	13.48	162	9735	1.01	ng/ul#	35
46) 2,6-Dinitrotoluene	13.89	165	3087	1.43	ng/ul#	39
53) 4-Nitrophenol	14.67	109	3219	1.72	ng/ul	86
73) 1,2,3,4-Tetrachlorobenzene	13.27	216	396509	85.19	ng/uL	99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031716\
Data File : BM004665.D
Acq On : 17 Mar 2016 14:19
Operator : UM/SJ
Sample : H1783-04
Misc :
ALS Vial : 9 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 18 05:07:14 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM02.2-EPA-BM031516.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 18 05:06:10 2016
Response via : Initial Calibration

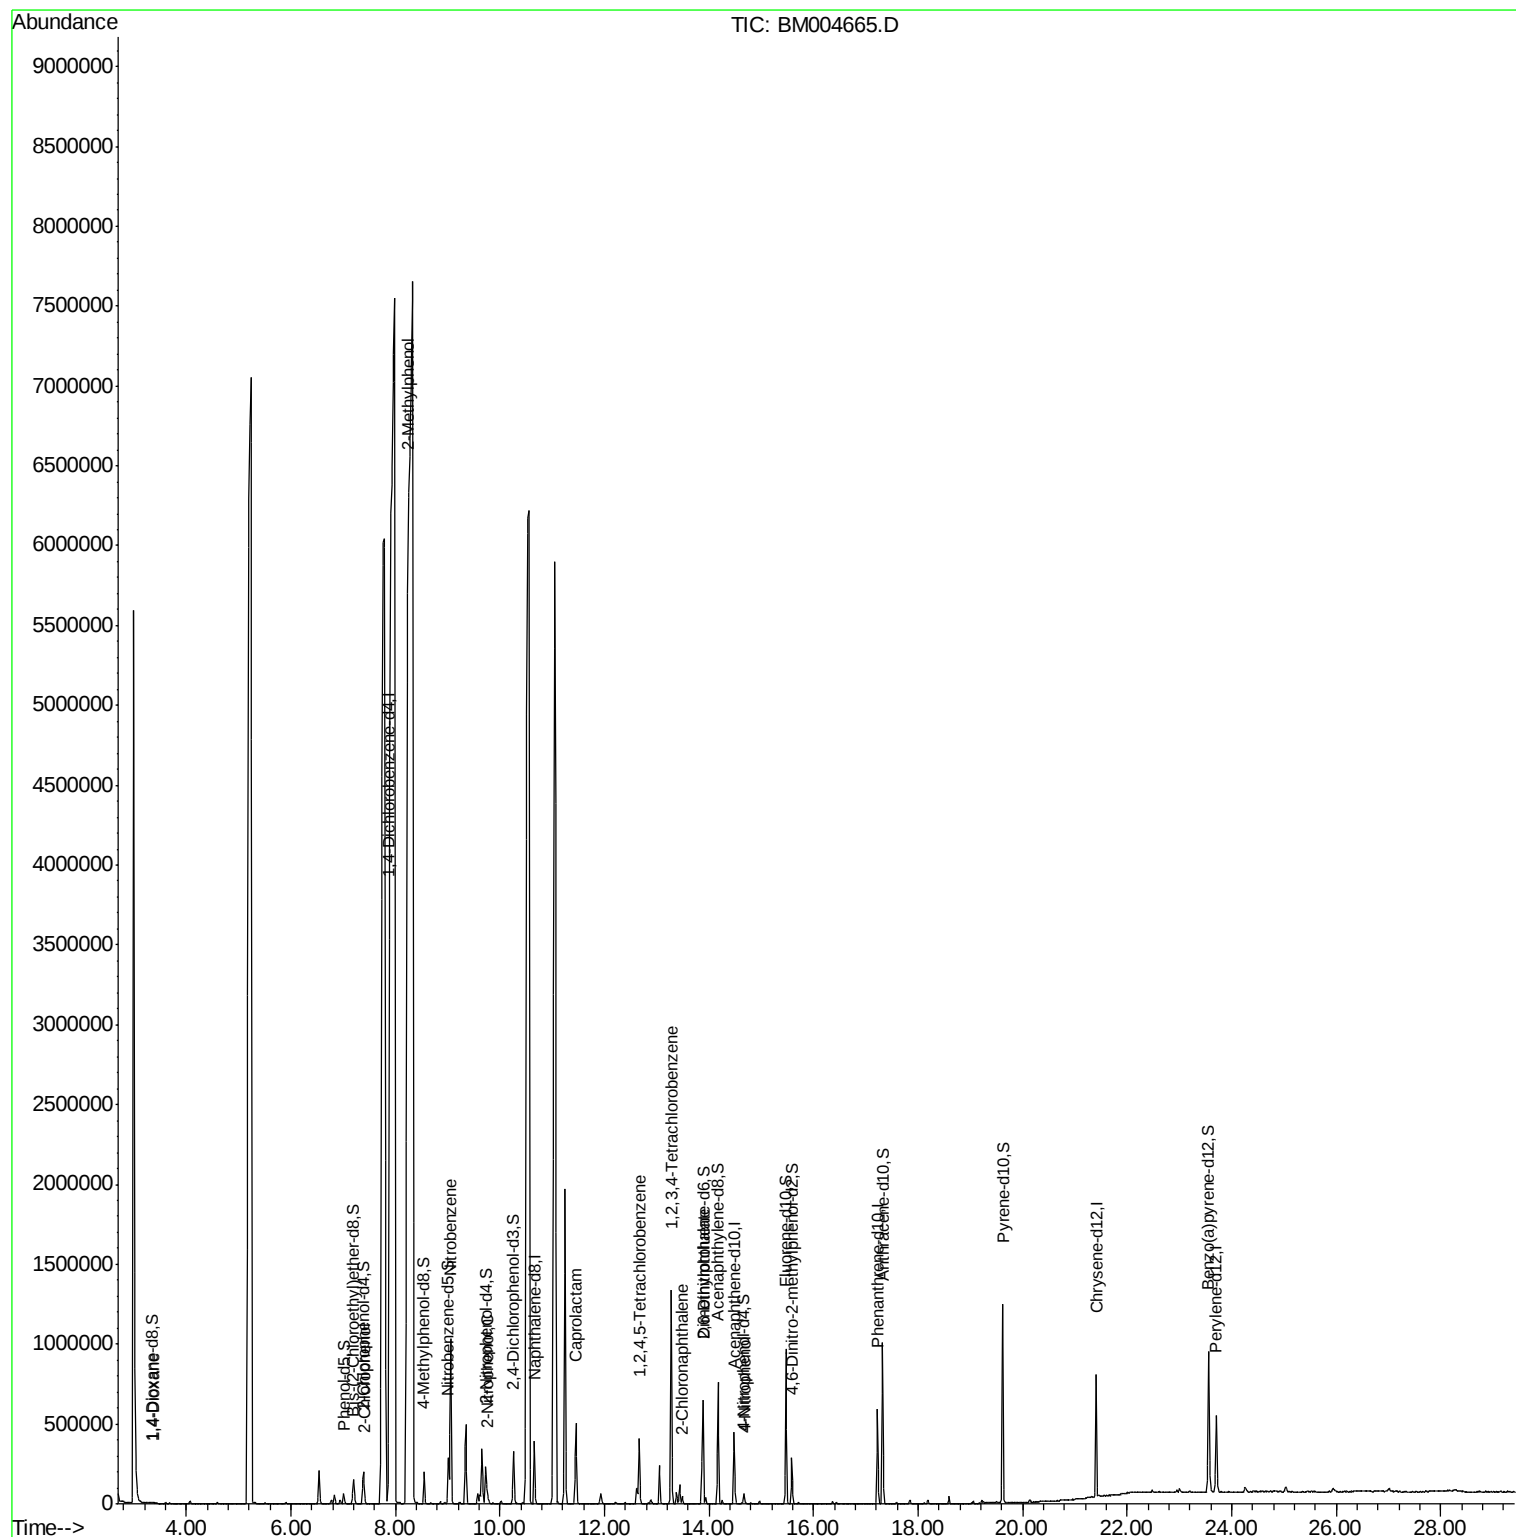



#2

1,4-Dioxane

Concen: 1.39 ng/uL

RT: 3.37 min Scan# 116

Delta R.T. -0.00 min

Lab File: BM004665.D

Acq: 17 Mar 2016 14:19

Instrument :

BNA_M

ClientSampleId :


Tot Ion: 88 Resp: 1562

Ion Ratio Lower Upper

88 100

43 17.2 21.0 31.6#

58 50.7 47.8 71.8



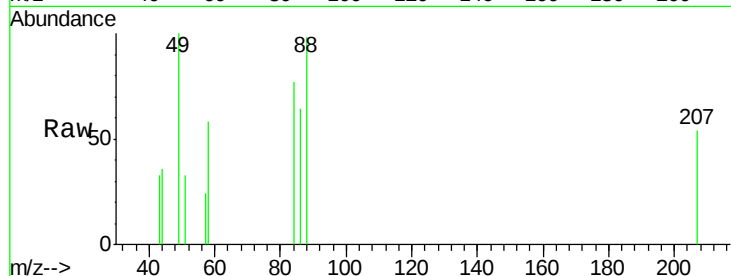


Abundance Ion 88.00 (87.70 to 88.70): BM004663.D (-112) (-)

Ion 43.00 (42.70 to 43.70): BM004663.D (-112) (-)

Ion 58.00 (57.70 to 58.70): BM004663.D (-112) (-)

Time-->

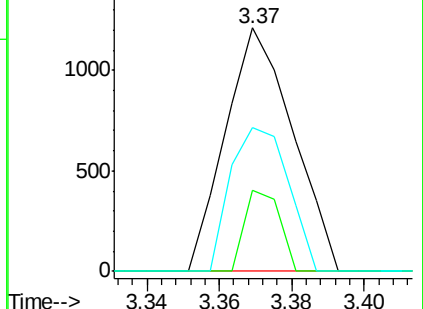

#10

2-Chlorophenol

Concen: 2.06 ng/uL

RT: 7.42 min Scan# 804

Delta R.T. 0.01 min

Lab File: BM004665.D

Acq: 17 Mar 2016 14:19


Tgt Ion: 128 Resp: 4795

Ion Ratio Lower Upper

128 100

64 59.7 31.9 47.9#

130 34.2 25.6 38.4






Abundance Ion 128.00 (127.70 to 128.70): BM004663.D (-796) (-)

Ion 64.00 (63.70 to 64.70): BM004663.D (-796) (-)

Ion 130.00 (129.70 to 130.70): BM004663.D (-796) (-)

Time-->

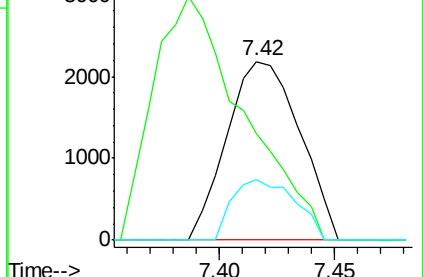



#11

2-Methylphenol

Concen: 13.93 ng/ul

RT: 8.24 min Scan# 944

Delta R.T. -0.04 min

Lab File: BM004665.D

Acq: 17 Mar 2016 14:19

Instrument :

BNA_M


ClientSampleId :

Tot Ion:108 Resp: 30811

Ion Ratio Lower Upper




108 100

107 97.9 72.4 108.6



Abundance Ion 108.00 (107.70 to 108.70): E

Ion 107.00 (106.70 to 107.70): E

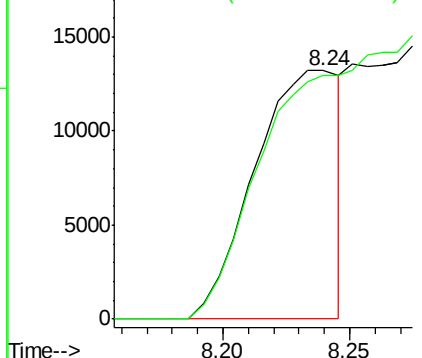

#20

Nitrobenzene

Concen: 120.24 ng/ul

RT: 9.06 min Scan# 1083

Delta R.T. 0.02 min

Lab File: BM004665.D

Acq: 17 Mar 2016 14:19


Tgt Ion: 77 Resp: 594976

Ion Ratio Lower Upper

77 100

123 47.4 39.0 58.4



65 13.1 10.4 15.6




Abundance Ion 77.00 (76.70 to 77.70): BM0

Ion 123.00 (122.70 to 123.70): E

Ion 65.00 (64.70 to 65.70): BM0

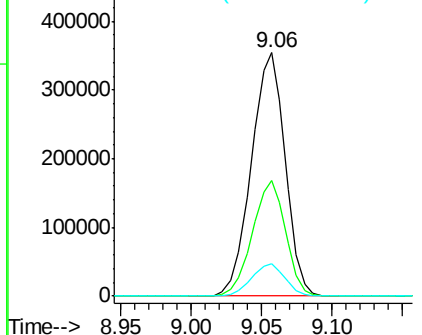



#23

2-Nitrophenol

Concen: 11.38 ng/ul

RT: 9.76 min Scan# 1202

Delta R.T. 0.01 min

Lab File: BM004665.D

Acq: 17 Mar 2016 14:19

Instrument :

BNA_M

ClientSampleId :


Tot Ion:139 Resp: 27308

Ion Ratio Lower Upper

139 100

65 51.4 36.3 54.5




109 31.3 26.4 39.6

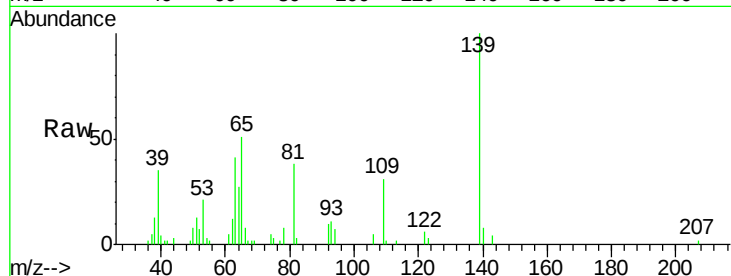

Abundance Ion 139.00 (138.70 to 139.70): E

Ion 65.00 (64.70 to 65.70): BM0

Ion 109.00 (108.70 to 109.70): E

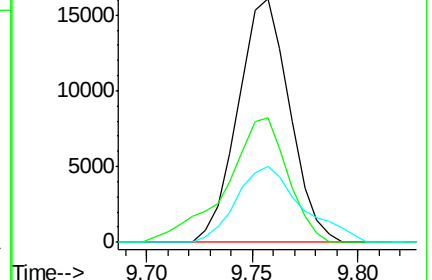

#32

Caprolactam

Concen: 25.12 ng/ul

RT: 11.45 min Scan# 1490

Delta R.T. -0.09 min

Lab File: BM004665.D

Acq: 17 Mar 2016 14:19


Tgt Ion:113 Resp: 36833

Ion Ratio Lower Upper

113 100

55 0.0 101.9 152.9#



56 0.0 81.2 121.8#




Abundance Ion 113.00 (112.70 to 113.70): E

Ion 55.00 (54.70 to 55.70): BM0

Ion 56.00 (55.70 to 56.70): BM0

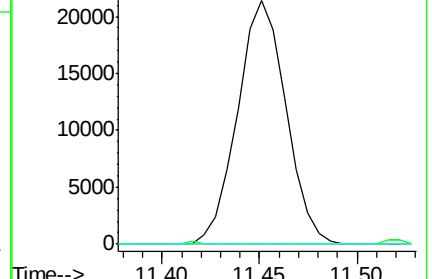


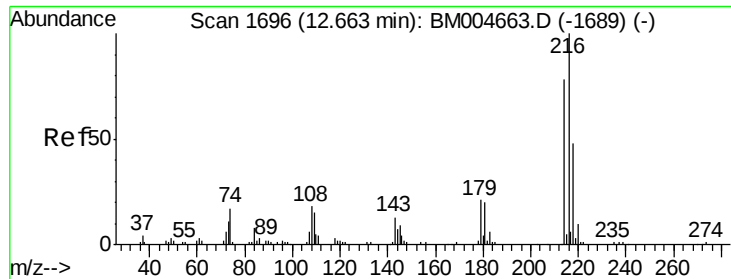




#37
 1,2,4,5-Tetrachlorobenzene
 Concen: 29.21 ng/ul
 RT: 12.66 min Scan# 1696
 Delta R.T. -0.00 min
 Lab File: BM004665.D
 Acq: 17 Mar 2016 14:19

Instrument :
 BNA_M
 ClientSampleId :

Tot Ion:	216	Resp:	142896
Ion	Ratio	Lower	Upper
216	100		
214	80.2	62.5	93.7
179	21.0	18.2	27.2
108	18.2	14.2	21.2

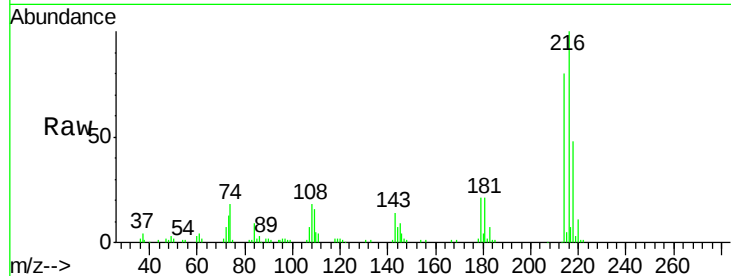


Abundance Ion 216.00 (215.70 to 216.70): E
 Ion 214.00 (213.70 to 214.70): E
 Ion 179.00 (178.70 to 179.70): E
 Ion 108.00 (107.70 to 108.70): E

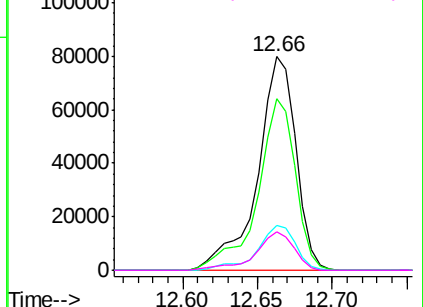




#42
 2-Chloronaphthalene
 Concen: 1.01 ng/ul
 RT: 13.48 min Scan# 1835
 Delta R.T. 0.13 min
 Lab File: BM004665.D
 Acq: 17 Mar 2016 14:19

Tgt Ion:	162	Resp:	9735
Ion	Ratio	Lower	Upper
162	100		
164	67.4	25.9	38.9#
127	0.0	34.1	51.1#

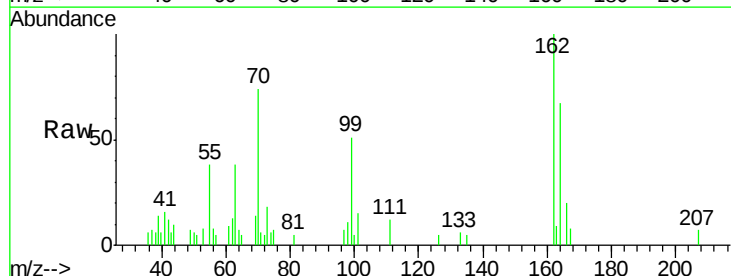

Abundance Ion 162.00 (161.70 to 162.70): E
 Ion 164.00 (163.70 to 164.70): E
 Ion 127.00 (126.70 to 127.70): E



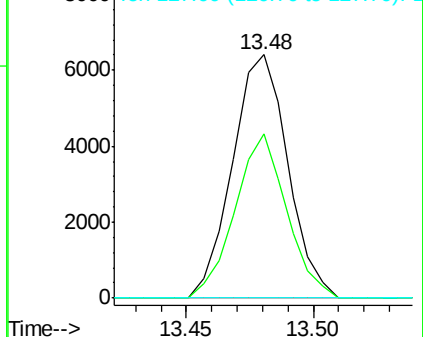



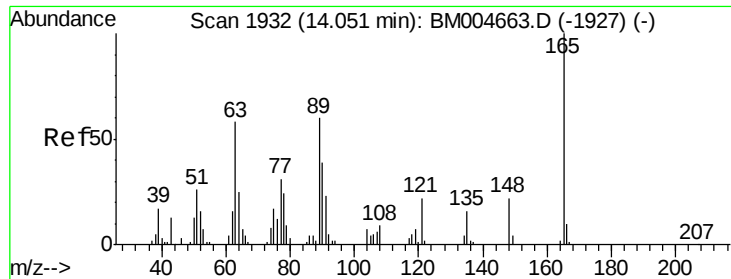

#46
 2,6-Dinitrotoluene
 Concen: 1.43 ng/ul
 RT: 13.89 min Scan# 1904
 Delta R.T. -0.16 min
 Lab File: BM004665.D
 Acq: 17 Mar 2016 14:19




Instrument :
 BNA_M
 ClientSampled :


Tot Ion:165 Resp: 3087
 Ion Ratio Lower Upper
 165 100
 89 0.0 42.4 63.6#
 121 33.1 16.6 24.8#

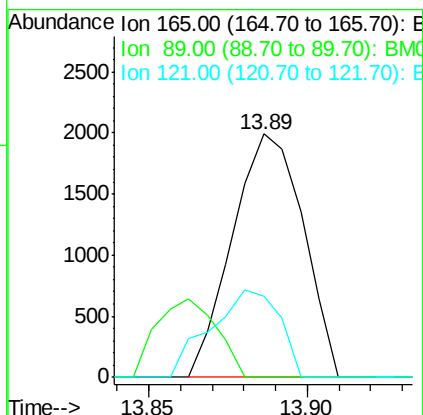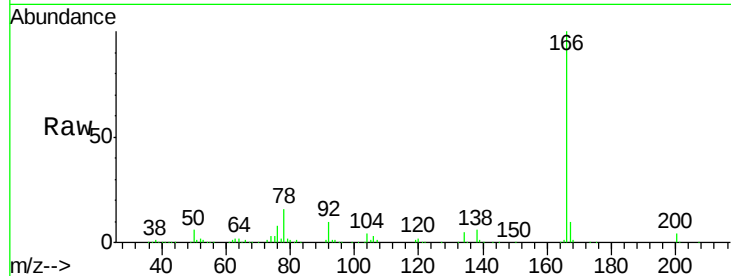

#53
 4-Nitrophenol
 Concen: 1.72 ng/ul
 RT: 14.67 min Scan# 2038
 Delta R.T. -0.01 min
 Lab File: BM004665.D
 Acq: 17 Mar 2016 14:19

Tgt Ion:109 Resp: 3219
 Ion Ratio Lower Upper
 109 100
 139 115.2 103.7 155.5
 65 129.6 89.4 134.2

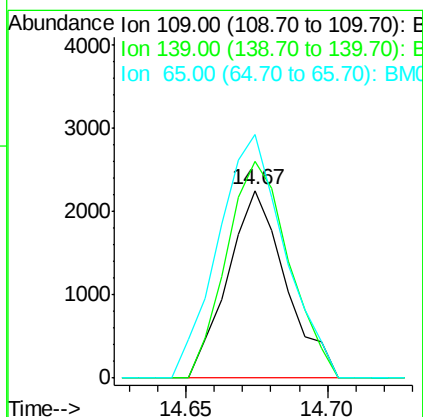

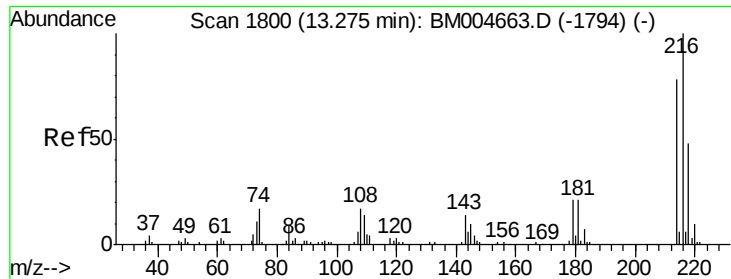

#73

1,2,3,4-Tetrachlorobenzene

Concen: 85.19 ng/uL

RT: 13.27 min Scan# 1800

Delta R.T. -0.00 min

Lab File: BM004665.D

Acq: 17 Mar 2016 14:19

Instrument :

BNA_M

ClientSampleId :


Tot Ion:216 Resp: 396509

Ion Ratio Lower Upper

216 100

214 77.6 62.5 93.7

218 47.3 38.4 57.6



Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

