

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031717\
 Data File : BM009278.D
 Acq On : 17 Mar 2017 17:37
 Operator : SJ/MA
 Sample : I2218-20
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CB300

Quant Time: Mar 18 00:40:26 2017
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM031717-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Sat Mar 18 00:39:50 2017
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	98102	20.00	ng/ul	0.00
2) Naphthalene-d8	10.67	136	439697	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.52	164	317460	20.00	ng/ul	0.00
12) Phenanthrene-d10	17.26	188	836253	20.00	ng/ul	0.00
18) Chrysene-d12	21.43	240	1315396	20.00	ng/ul	0.00
23) Perylene-d12	23.77	264	1362960	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	10.29	165	4577	0.64	ng/uL	0.00
7) Acenaphthylene-d8	14.21	160	606553	22.54	ng/ul	0.00
10) Fluorene-d10	15.50	176	567925	24.07	ng/ul	0.00
15) Anthracene-d10	17.36	188	966227	24.32	ng/ul	0.00
19) Pyrene-d10	19.65	212	1271159	24.10	ng/ul	0.00
26) Benzo(a)pyrene-d12	23.61	264	1014882	16.38	ng/ul	0.00
Target Compounds				Qvalue		
14) Phenanthrene	17.30	178	66976	1.42	ng/ul	98
16) Anthracene	17.30	178	66976	1.37	ng/ul	97
17) Fluoranthene	19.32	202	146992	2.46	ng/ul	97
20) Pyrene	19.68	202	139798	2.06	ng/ul#	92
21) Benzo(a)anthracene	21.47	228	88300	1.18	ng/ul	95
22) Chrysene	21.47	228	88300	1.25	ng/ul	99
24) Benzo(b)fluoranthene	23.06	252	106089	1.32	ng/ul#	78


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA M\DATA\BM031717\
Data File : BM009278.D
Acq On : 17 Mar 2017 17:37
Operator : SJ/MA
Sample : I2218-20
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CB300

Quant Time: Mar 18 00:40:26 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM031717-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Sat Mar 18 00:39:50 2017
Response via : Initial Calibration

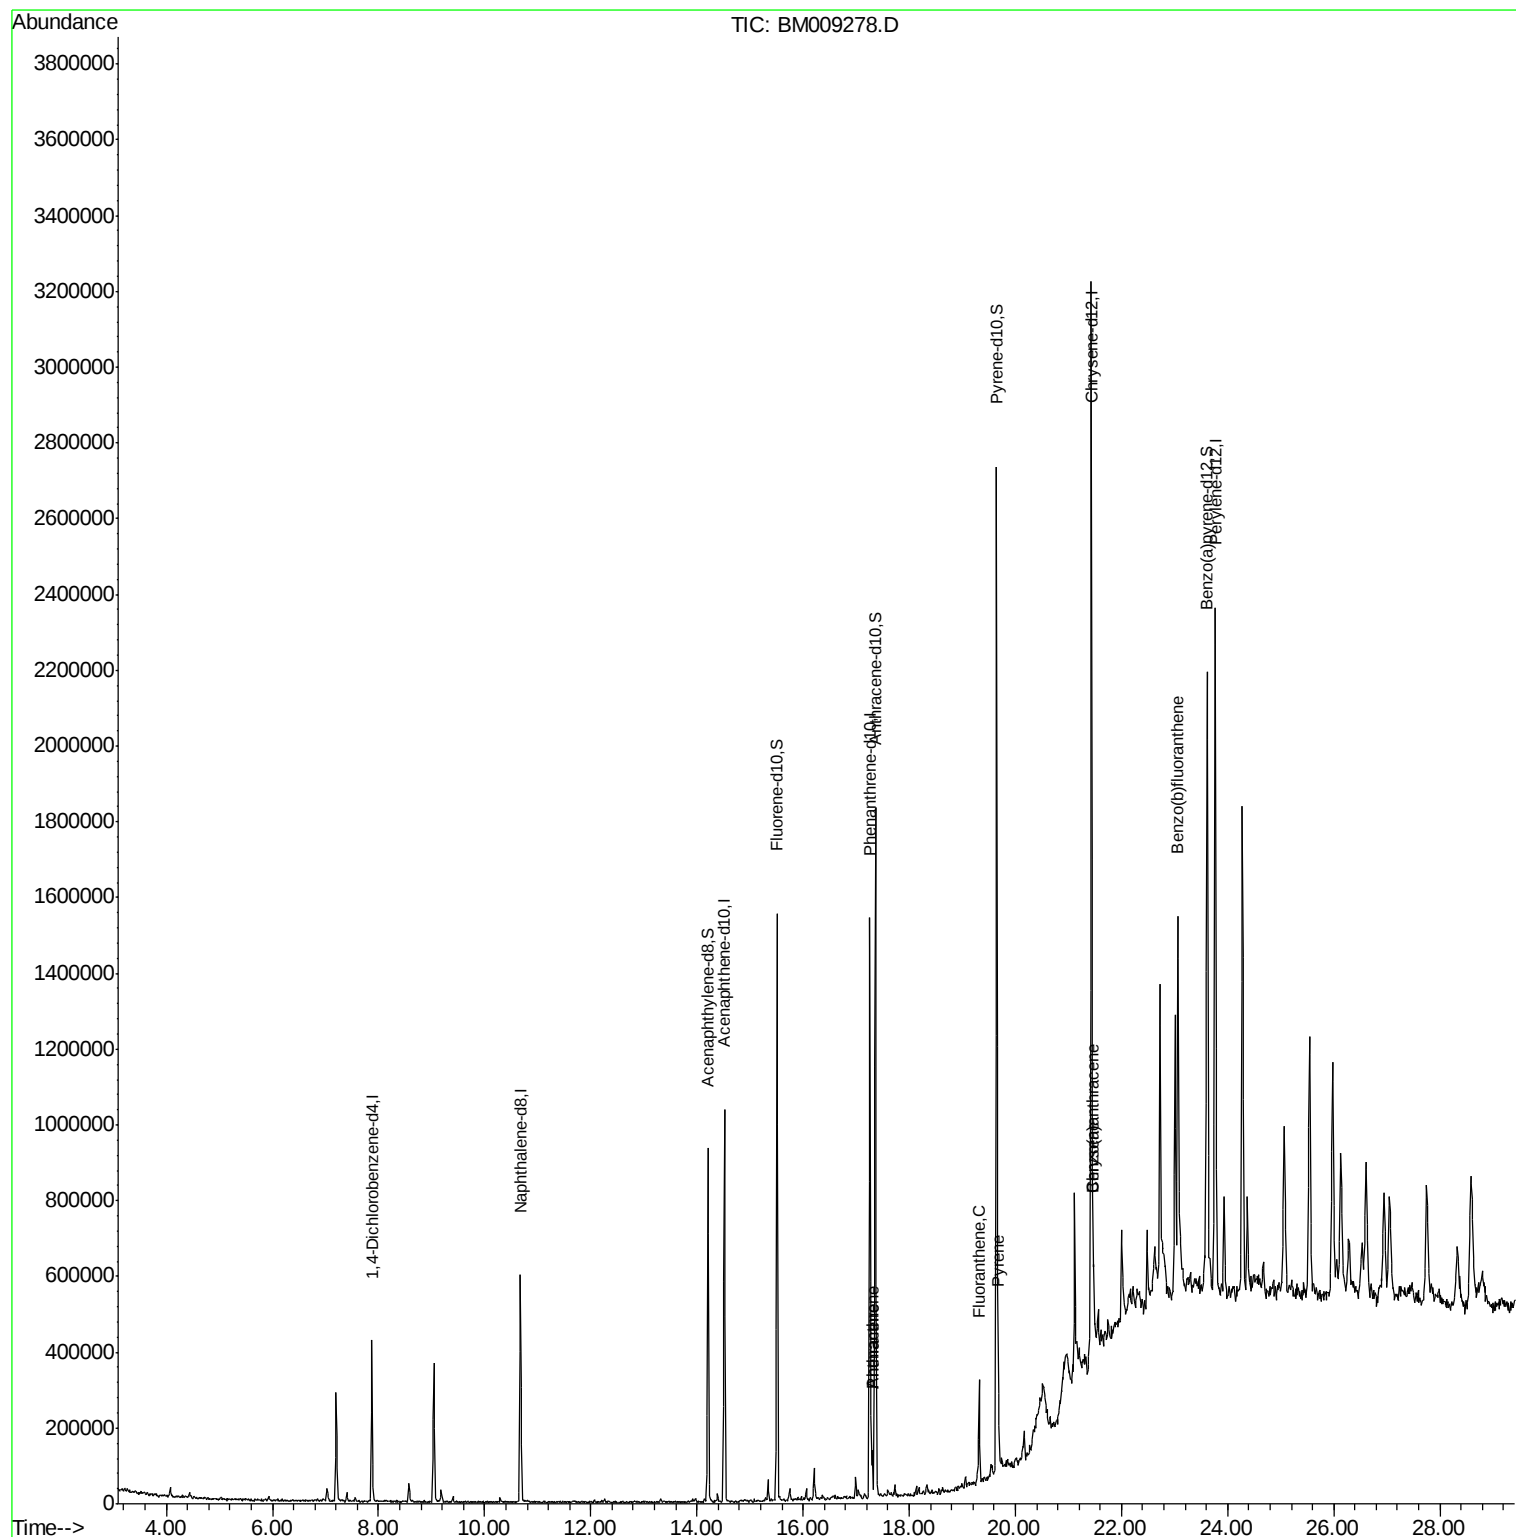

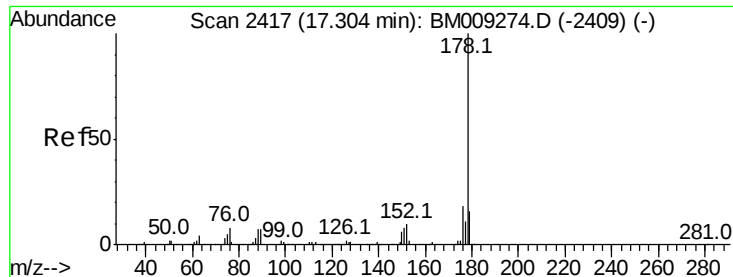

#14

Phenanthrene

Concen: 1.42 ng/ul

RT: 17.30 min Scan# 2417

Delta R.T. 0.00 min

Lab File: BM009278.D

Acq: 17 Mar 2017 17:37

Instrument :

BNA_M

ClientSampleId :

CB300


Tot Ion:178 Resp: 66976

Ion Ratio Lower Upper

178 100

179 13.8 12.2 18.4




176 20.4 16.4 24.6

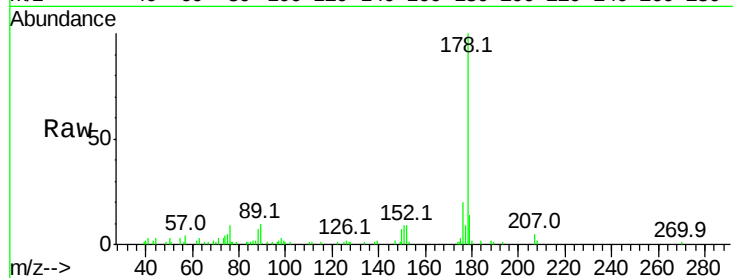

Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

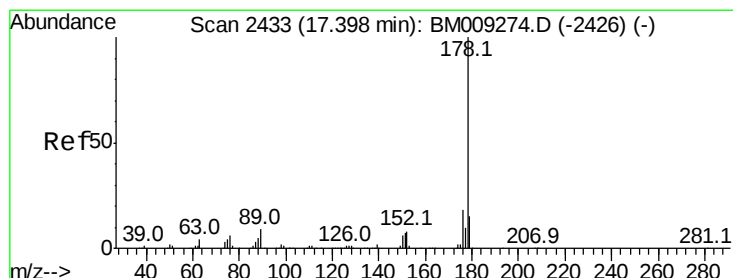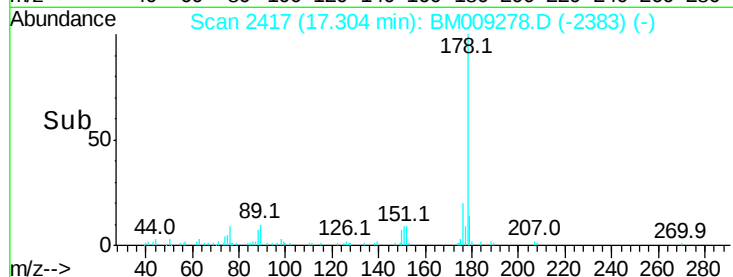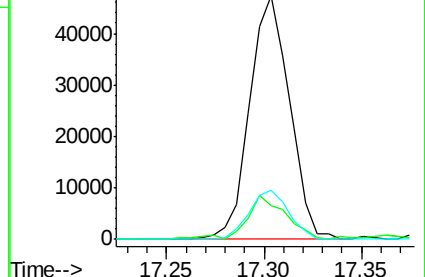

#16

Anthracene

Concen: 1.37 ng/ul

RT: 17.30 min Scan# 2417

Delta R.T. -0.09 min

Lab File: BM009278.D

Acq: 17 Mar 2017 17:37


Tgt Ion:178 Resp: 66976

Ion Ratio Lower Upper

178 100

179 13.8 12.7 19.1



176 20.4 15.8 23.8

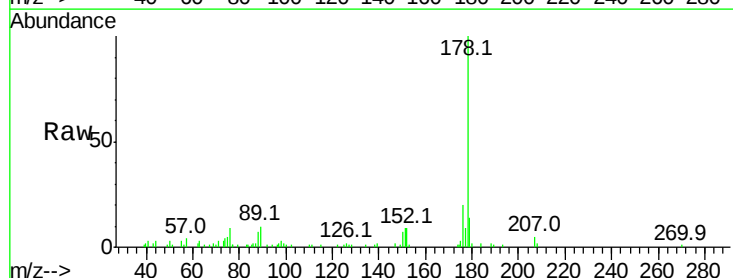


Abundance Ion 178.00 (177.70 to 178.70): E

Ion 179.00 (178.70 to 179.70): E

Ion 176.00 (175.70 to 176.70): E

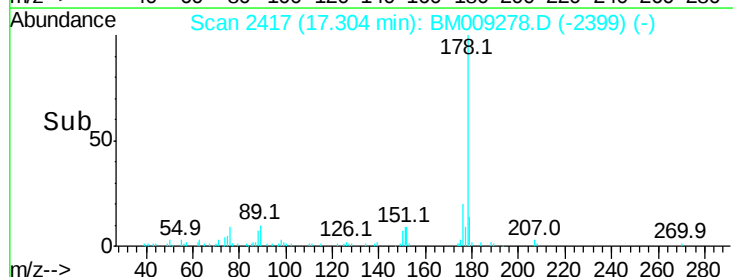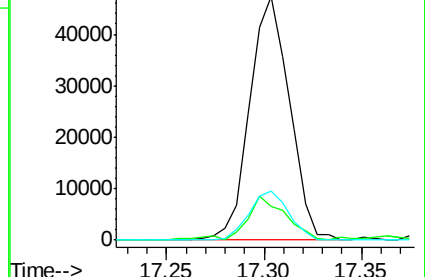

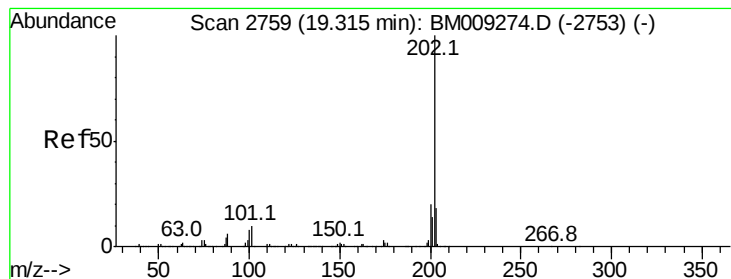

#17

Fluoranthene

Concen: 2.46 ng/ul

RT: 19.32 min Scan# 2759

Delta R.T. 0.00 min

Lab File: BM009278.D

Acq: 17 Mar 2017 17:37

Instrument :

BNA_M

ClientSampleId :

CB300


Tot Ion:202 Resp: 146992

Ion Ratio Lower Upper

202 100

101 11.3 9.8 14.8




100 8.1 7.5 11.3

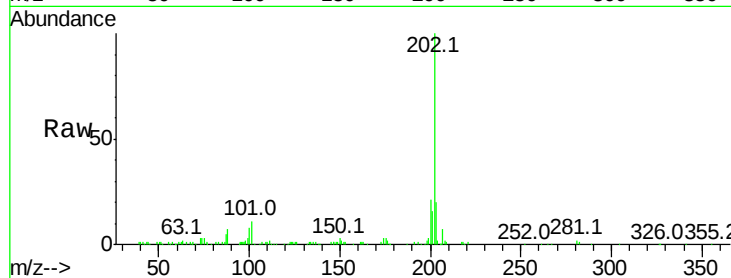

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

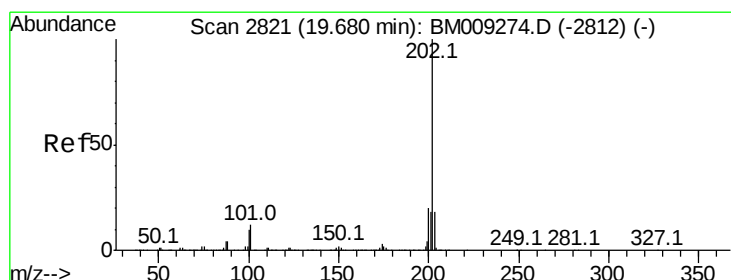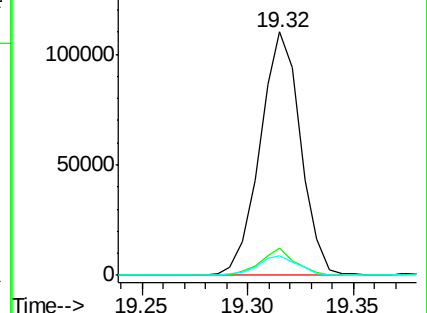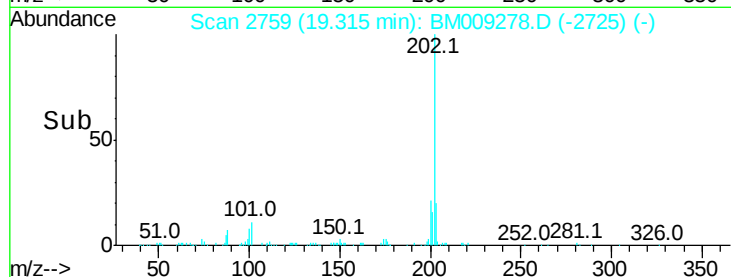

#20

Pyrene

Concen: 2.06 ng/ul

RT: 19.68 min Scan# 2821

Delta R.T. 0.00 min

Lab File: BM009278.D

Acq: 17 Mar 2017 17:37


Tgt Ion:202 Resp: 139798

Ion Ratio Lower Upper

202 100

101 11.0 11.2 16.8#



100 8.9 9.8 14.6#

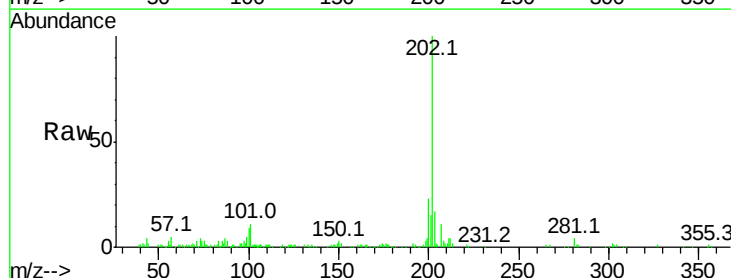


Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

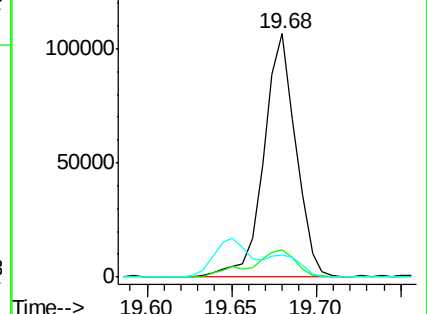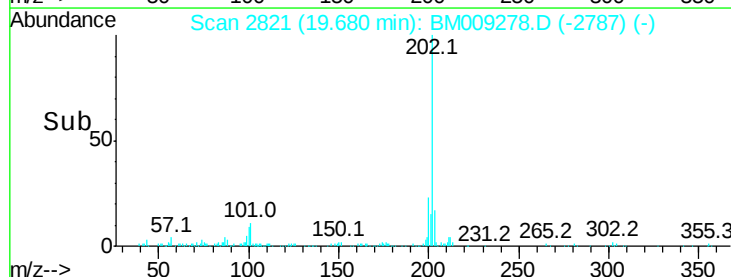

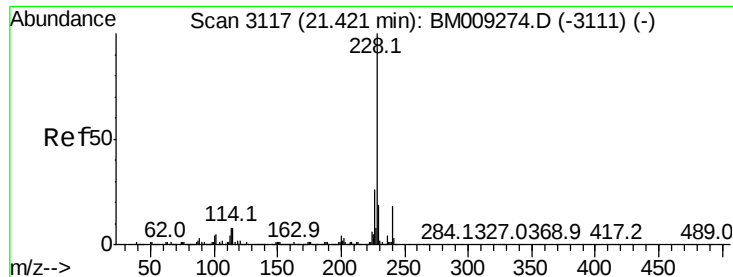

#21

Benzo(a)anthracene

Concen: 1.18 ng/ul

RT: 21.47 min Scan# 3126

Delta R.T. 0.05 min

Lab File: BM009278.D

Acq: 17 Mar 2017 17:37

Instrument :

BNA_M

ClientSampleId :

CB300





Tot Ion:228 Resp: 88300

Ion Ratio Lower Upper

228 100

229 20.7 15.9 23.9

226 31.8 22.1 33.1

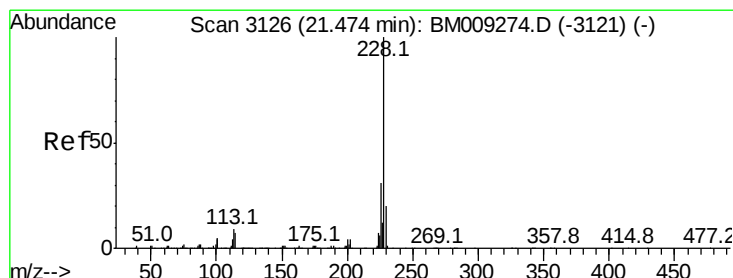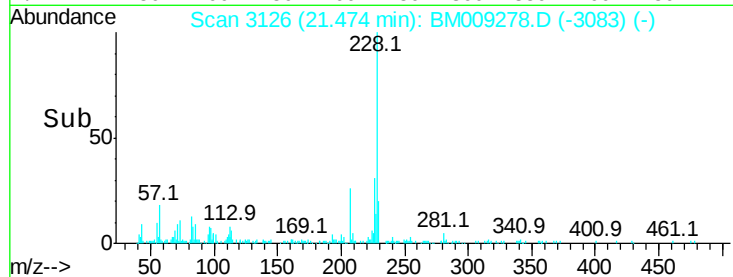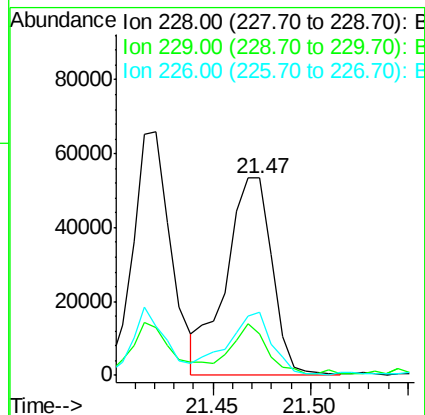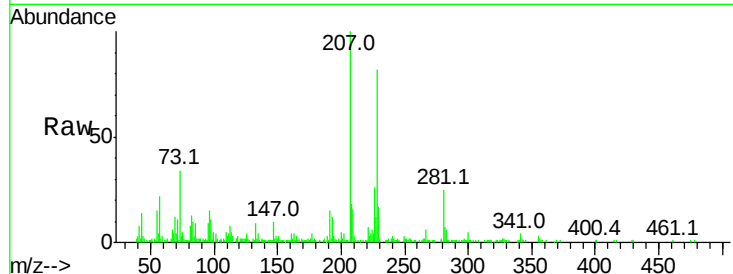

#22

Chrysene

Concen: 1.25 ng/ul

RT: 21.47 min Scan# 3126

Delta R.T. 0.00 min

Lab File: BM009278.D

Acq: 17 Mar 2017 17:37




Tgt Ion:228 Resp: 88300


Ion Ratio Lower Upper

228 100

226 31.8 25.0 37.6

229 20.7 16.6 25.0

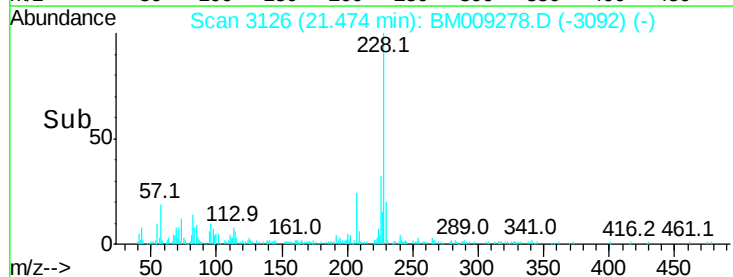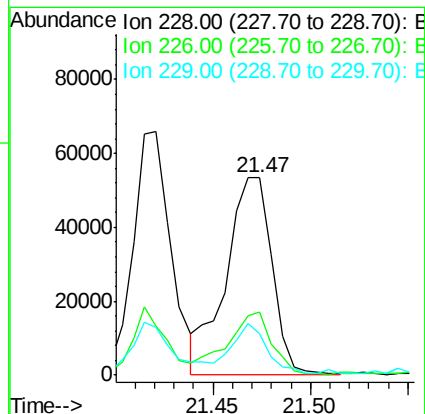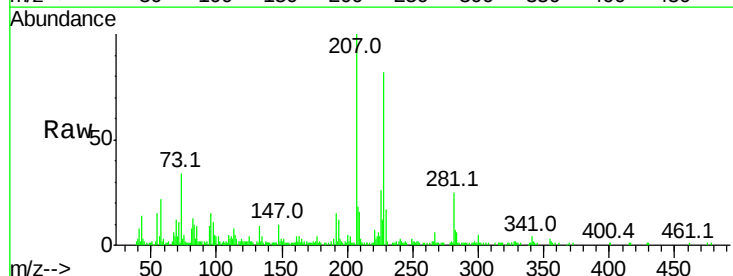

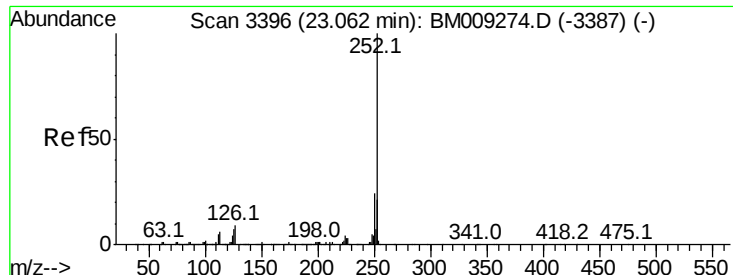

#24

Benzo(b)fluoranthene

Concen: 1.32 ng/ul

RT: 23.06 min Scan# 3395

Delta R.T. -0.01 min

Lab File: BM009278.D

Acq: 17 Mar 2017 17:37

Instrument :

BNA_M

ClientSampleId :

CB300


Tot Ion:252 Resp: 106089

Ion Ratio Lower Upper

252 100

253 25.9 17.8 26.6

125 30.5 9.4 14.0#

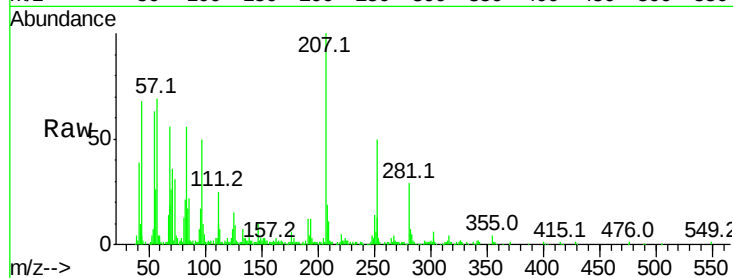

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

