

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031720\
 Data File : BM025617.D
 Acq On : 17 Mar 2020 19:08
 Operator : CG/JU
 Sample : L1516-09RX
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :

Quant Time: Mar 18 01:16:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 17 17:05:05 2020
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2818	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	11309	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.22	164	7626	0.40	ng/ul	0.00
10) Phenanthrene-d10	0.00	188	0	0.00	ng/ul	-16.97
16) Chrysene-d12	21.16	240	18880	0.40	ng/ul	0.00
20) Perylene-d12	23.31	264	20948	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.95	152	4462	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.00	212	11709	0.00	ng/ul	0.00
Target Compounds						
					Ovalue	
17) Pyrene	19.39	202	1769	0.021	ng/ul#	81
23) Benzo(a)pyrene	23.18	252	4009	0.058	ng/ul#	63


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031720\
Data File : BM025617.D
Acq On : 17 Mar 2020 19:08
Operator : CG/JU
Sample : L1516-09RX
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :

Quant Time: Mar 18 01:16:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 17 17:05:05 2020
Response via : Initial Calibration

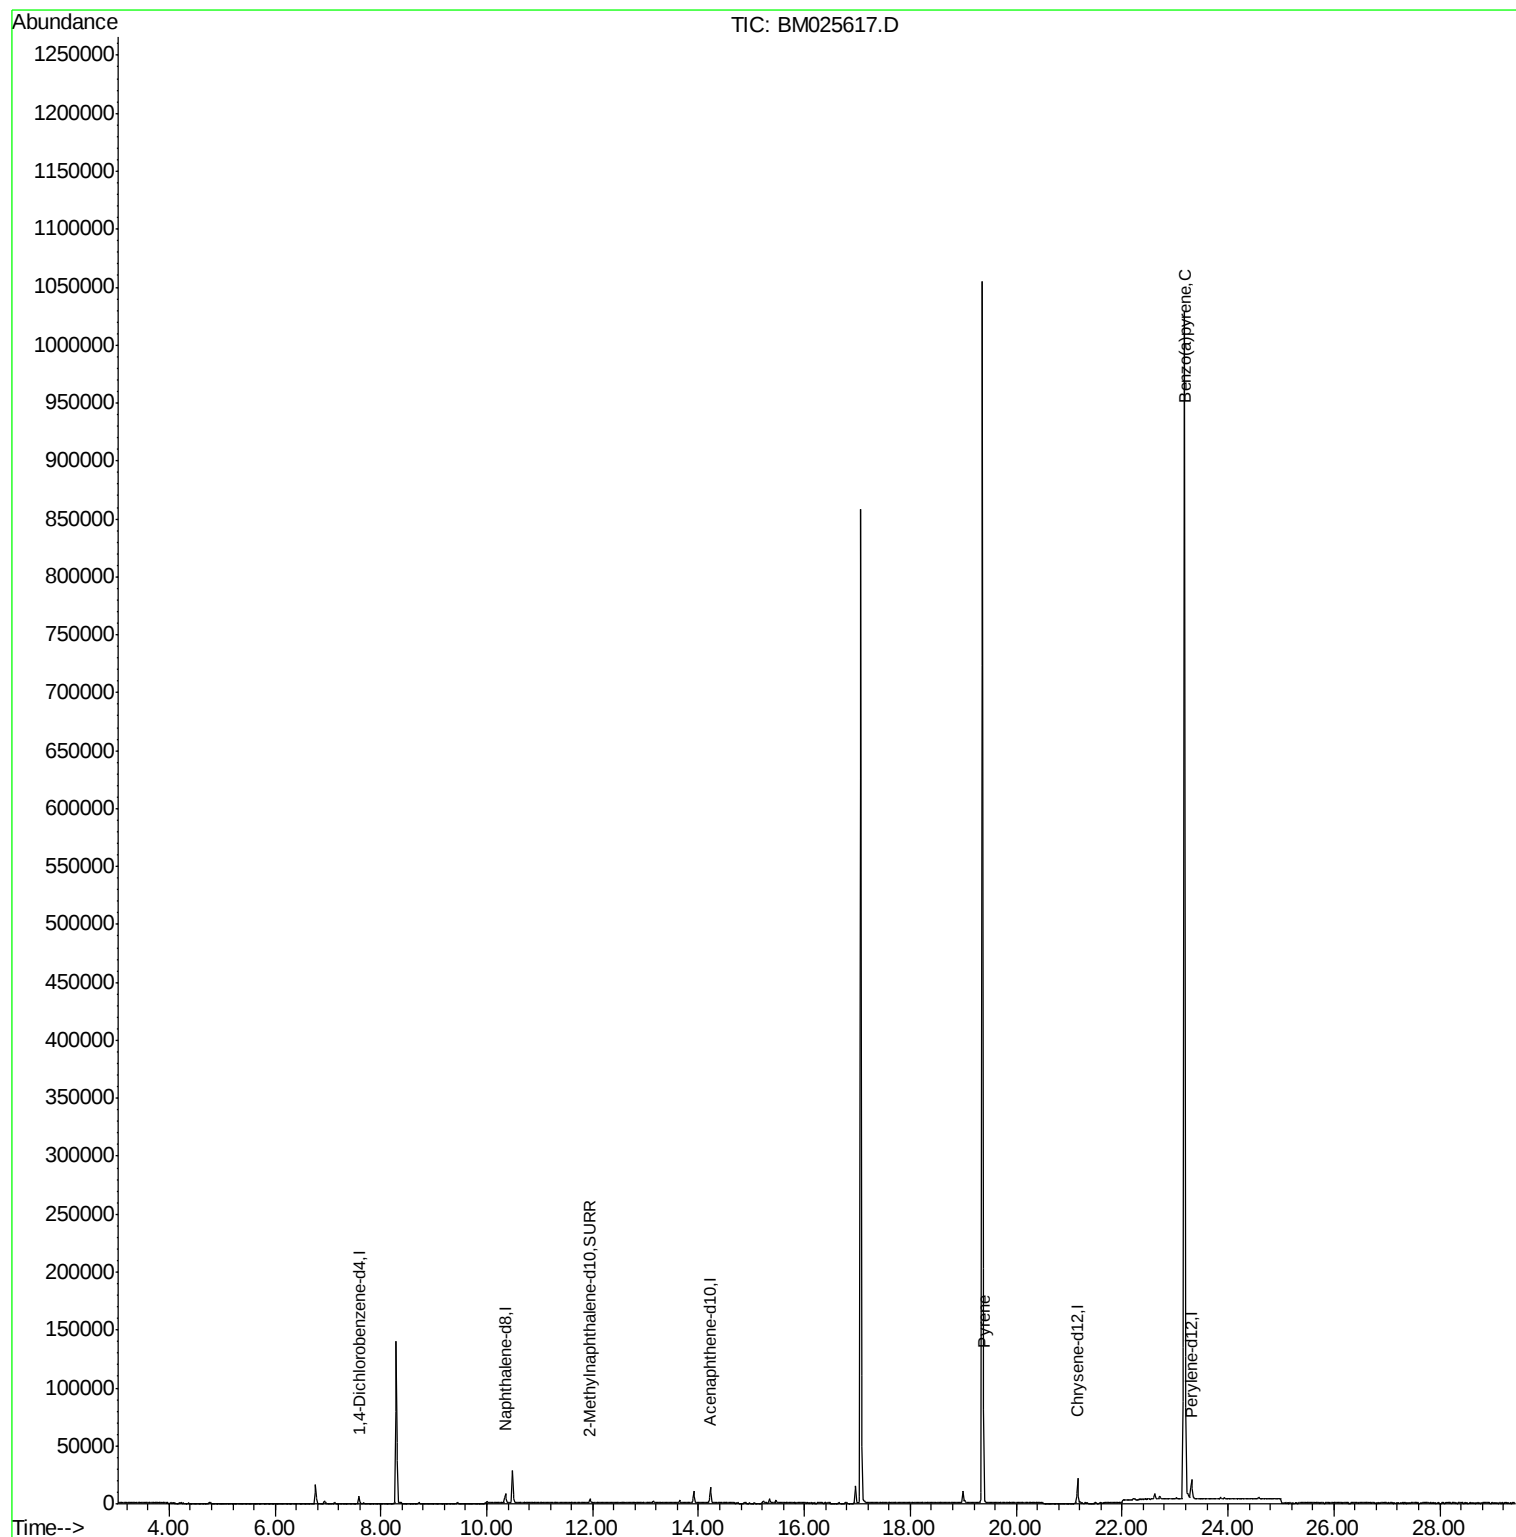

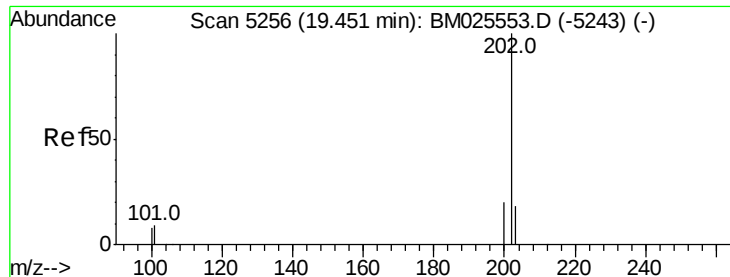

#17

Pvrene

Concen: 0.021 ng/ul

RT: 19.39 min Scan# 5240

Delta R.T. -0.00 min

Lab File: BM025617.D

Acq: 17 Mar 2020 19:08

Instrument :

BNA_M

ClientSampleId :


Tot Ion:202 Resp: 1769

Ion Ratio Lower Upper

202 100

101 14.5 7.1 10.7#




100 16.0 6.0 9.0#

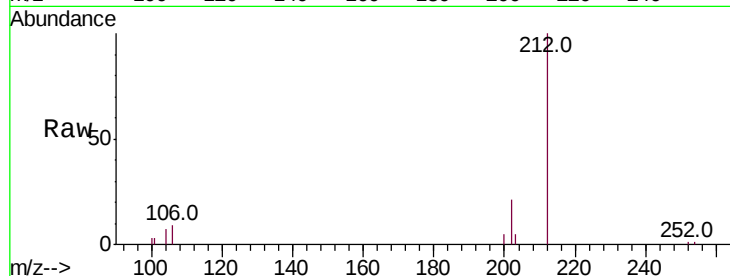

Abundance Ion 202.00 (201.70 to 202.70): E

Ion 101.00 (100.70 to 101.70): E

Ion 100.00 (99.70 to 100.70): B

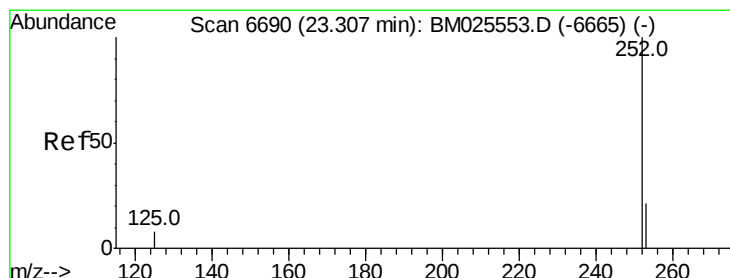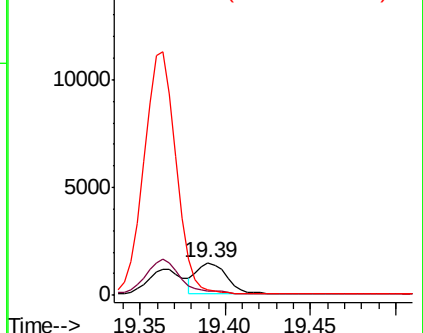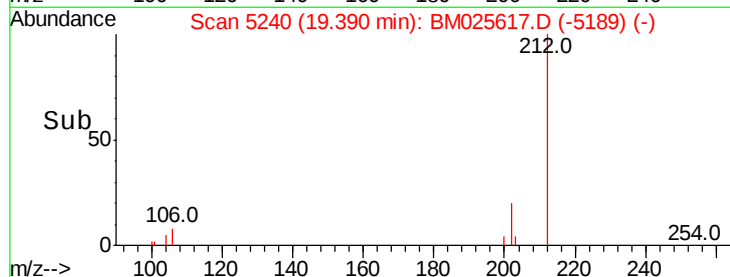

#23

Benzo(a)pyrene

Concen: 0.058 ng/ul

RT: 23.18 min Scan# 6637

Delta R.T. -0.04 min

Lab File: BM025617.D

Acq: 17 Mar 2020 19:08


Tgt Ion:252 Resp: 4009

Ion Ratio Lower Upper

252 100

253 43.3 21.3 31.9#

125 29.4 8.5 12.7#

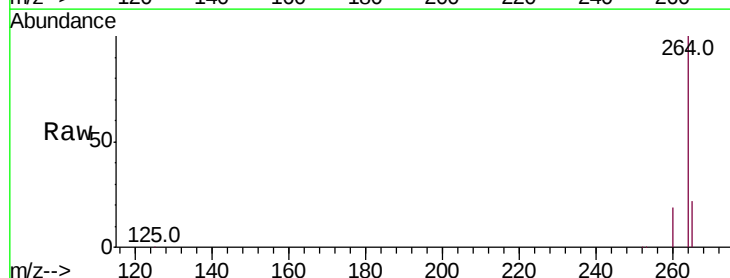

Abundance Ion 252.00 (251.70 to 252.70): E

Ion 253.00 (252.70 to 253.70): E

Ion 125.00 (124.70 to 125.70): E

