




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031720\
Data File : BM025613.D
Acq On : 17 Mar 2020 16:44
Operator : CG/JU
Sample : PB127627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
3/18/2020 9:01:51 AM

Quant Time: Mar 17 17:29:32 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 17 17:05:05 2020
Response via : Initial Calibration

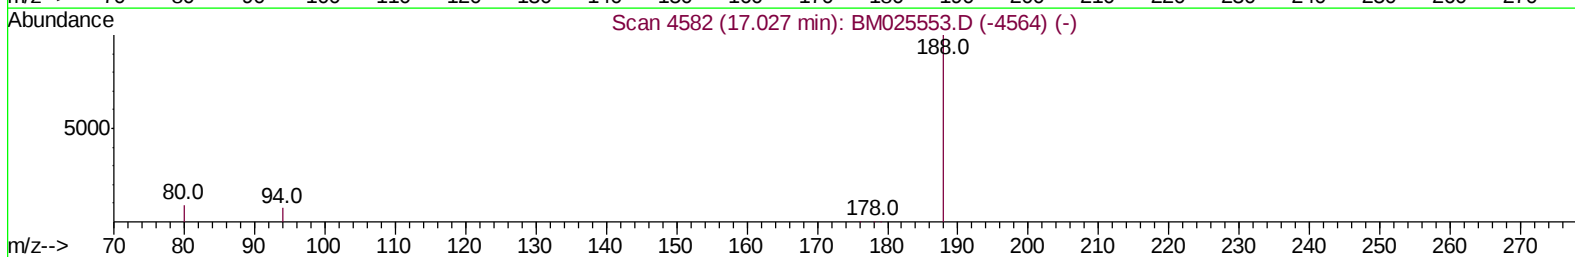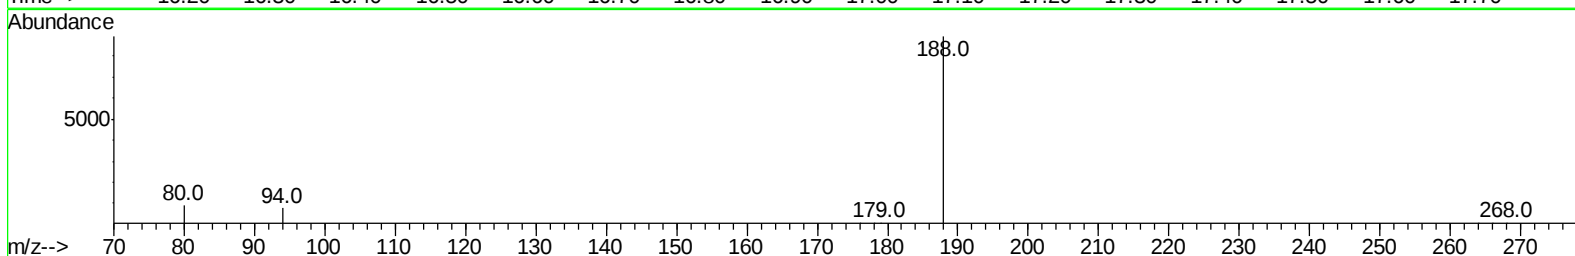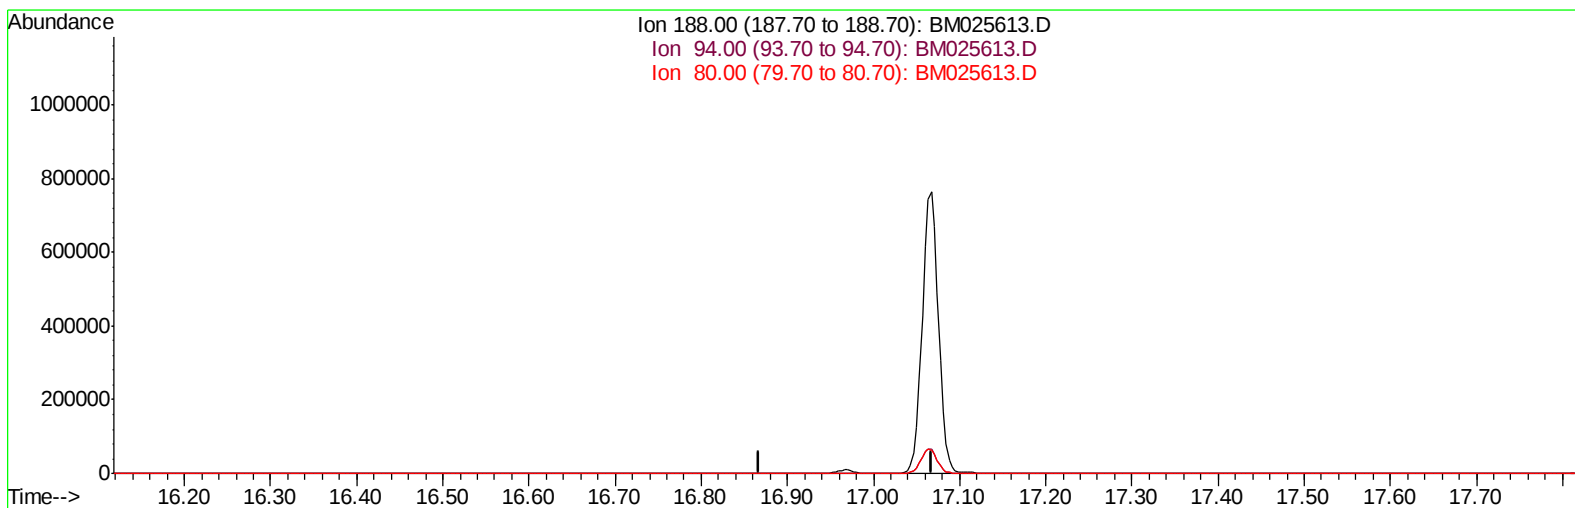

TIC: BM025613.D

(10) Phenanthrene-d10 (I)

16.968min (-16.968) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00




Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031720\
 Data File : BM025613.D
 Acq On : 17 Mar 2020 16:44
 Operator : CG/JU
 Sample : PB127627BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK27

Manual Integrations
 APPROVED

mohammad
 3/18/2020 9:01:51 AM

Quant Time: Mar 17 17:29:32 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 17 17:05:05 2020
 Response via : Initial Calibration

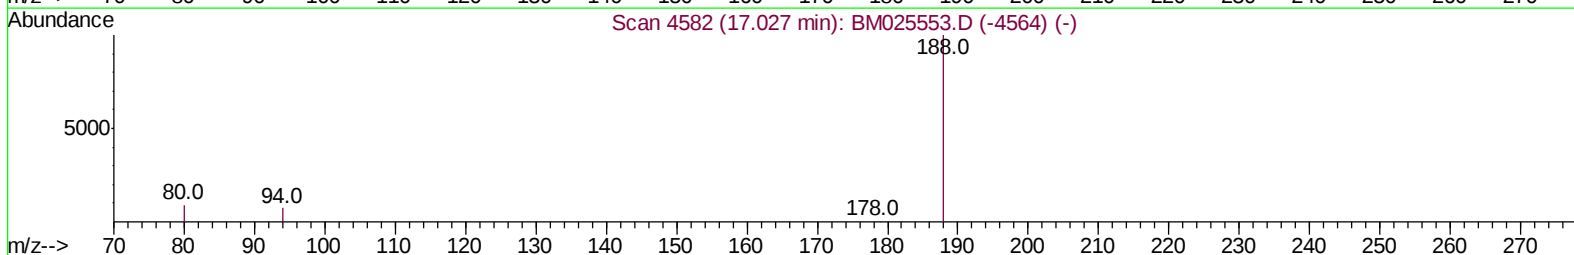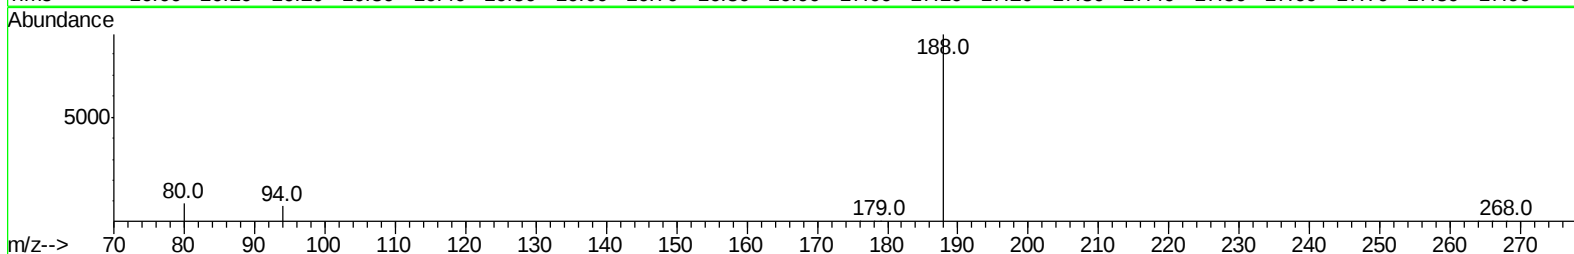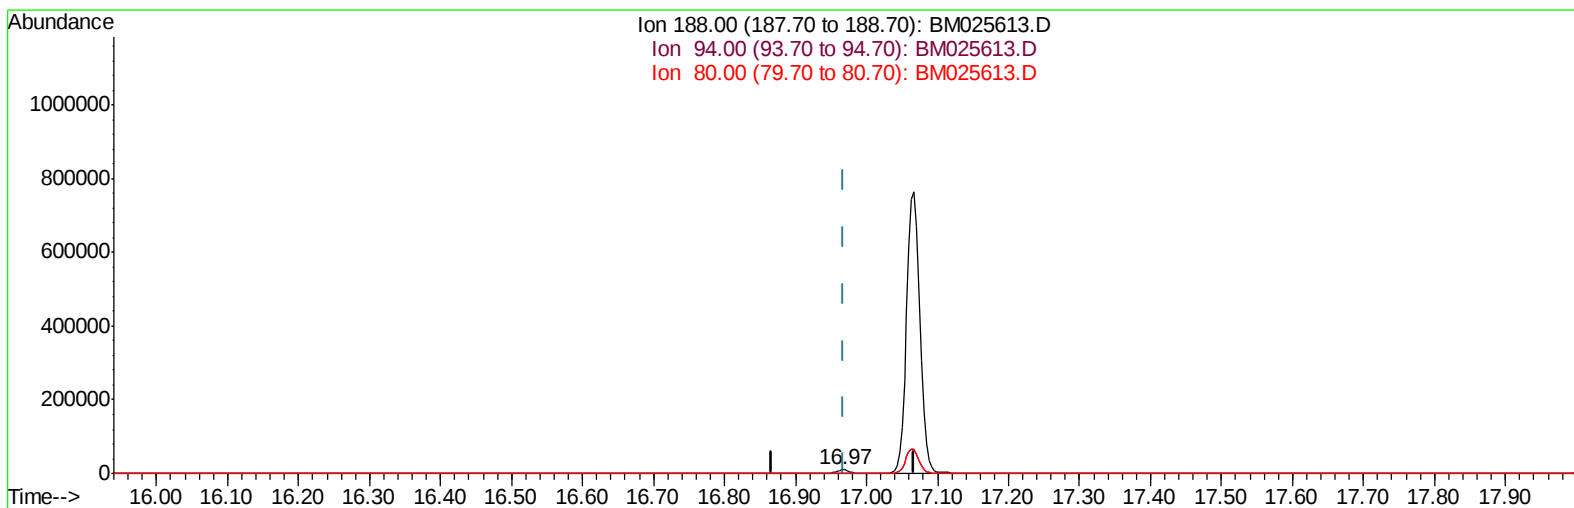

TIC: BM025613.D

(10) Phenanthrene-d10 (I)

16.966min (-0.002) 0.40ng/ul m

response 11911

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	8.45
80.00	8.70	10.03
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031720\
 Data File : BM025613.D
 Acq On : 17 Mar 2020 16:44
 Operator : CG/JU
 Sample : PB127627BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK27

Manual Integrations
 APPROVED

mohammad
 3/18/2020 9:01:51 AM

Quant Time: Mar 17 17:30:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 17 17:05:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2015	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	7770	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.23	164	5286	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.97	188	11911m	0.40	ng/ul	0.00
16) Chrysene-d12	21.16	240	12533	0.40	ng/ul	0.00
20) Perylene-d12	23.31	264	13116	0.40	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Methylnaphthalene-d10	11.95	152	4676	0.33	ng/ul	0.00
14) Fluoranthene-d10	19.00	212	11926	0.36	ng/ul	0.00

Target Compounds	Ovalue

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA M\Data\BM031720\
Data File : BM025613.D
Acq On : 17 Mar 2020 16:44
Operator : CG/JU
Sample : PB127627BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK27

Manual Integrations
APPROVED

mohammad
3/18/2020 9:01:51 AM

Quant Time: Mar 17 17:30:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 17 17:05:05 2020
Response via : Initial Calibration

