




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031720\
Data File : BM025617.D
Acq On : 17 Mar 2020 19:08
Operator : CG/JU
Sample : L1516-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD27

Manual Integrations
APPROVED

mohammad
3/18/2020 9:02:02 AM

Quant Time: Mar 18 01:16:16 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 17 17:05:05 2020
Response via : Initial Calibration

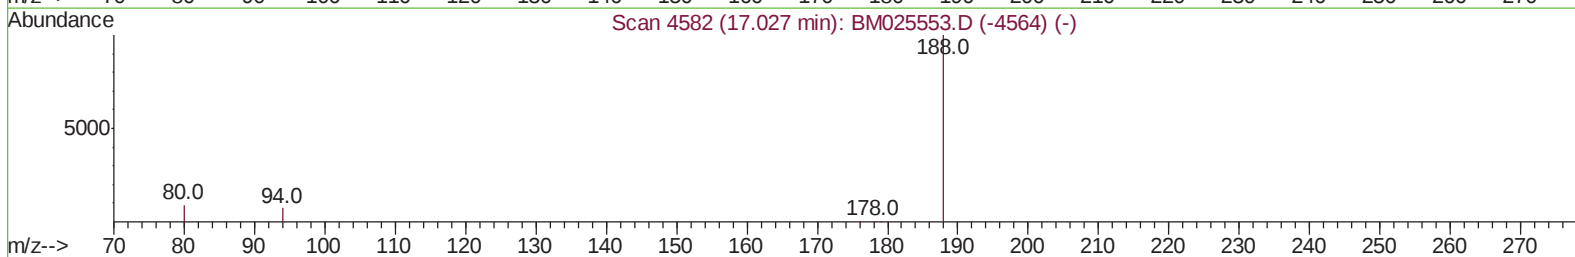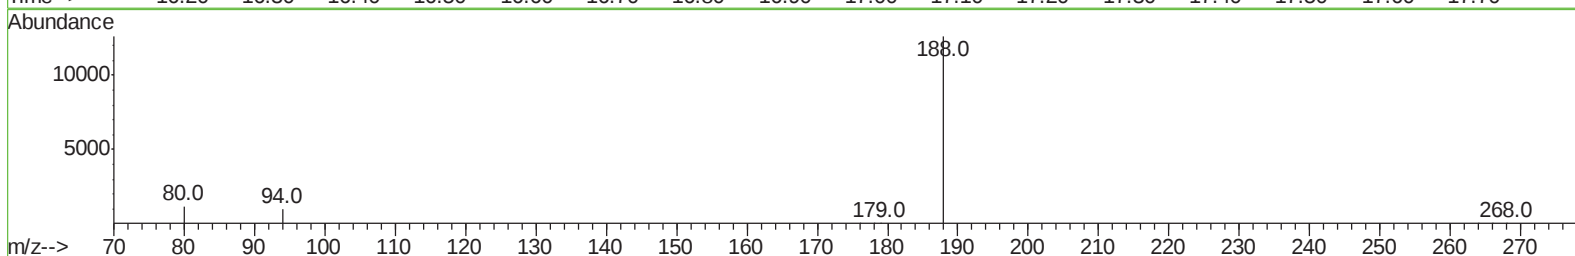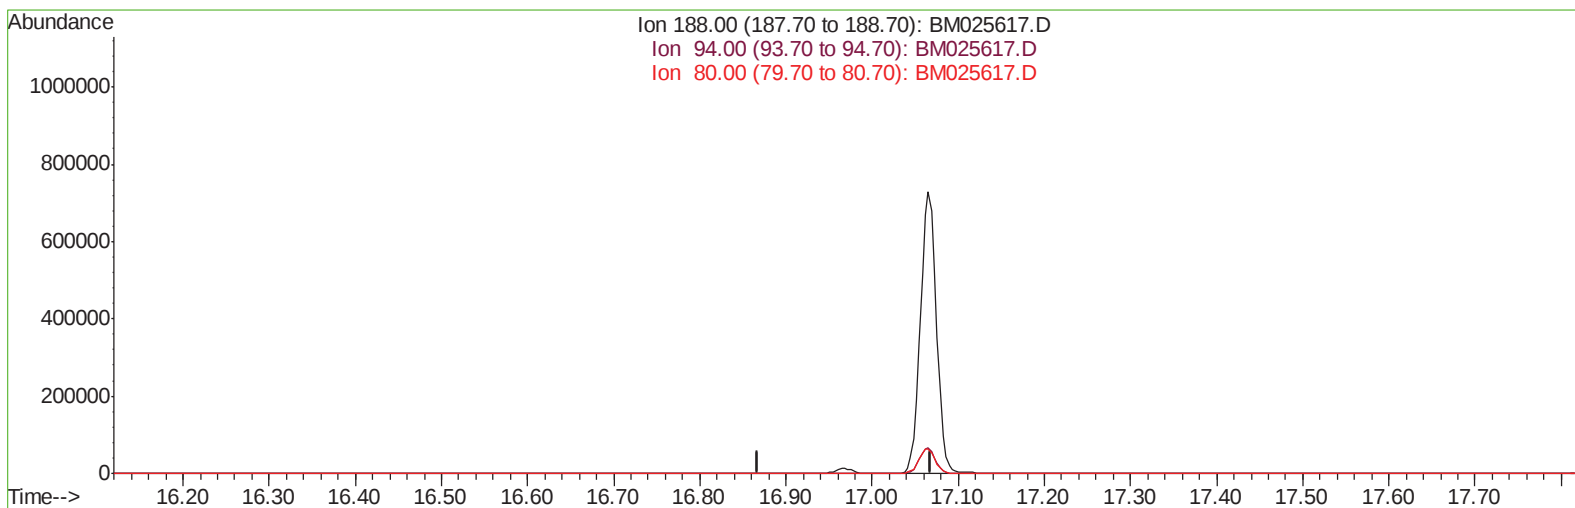

TIC: BM025617.D

(10) Phenanthrene-d10 (I)

16.968min (-16.968) 0.00ng/ul

response 0

Ion	Exp%	Act%
188.00	100	0.00
94.00	7.10	0.00#
80.00	8.70	0.00#
0.00	0.00	0.00




Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031720\
 Data File : BM025617.D
 Acq On : 17 Mar 2020 19:08
 Operator : CG/JU
 Sample : L1516-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD27

Manual Integrations
 APPROVED

mohammad
 3/18/2020 9:02:02 AM

Quant Time: Mar 18 01:16:16 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 17 17:05:05 2020
 Response via : Initial Calibration

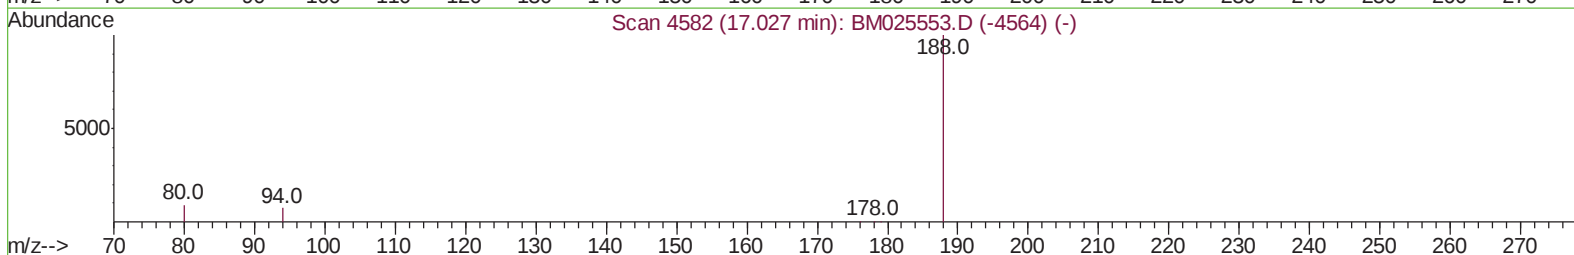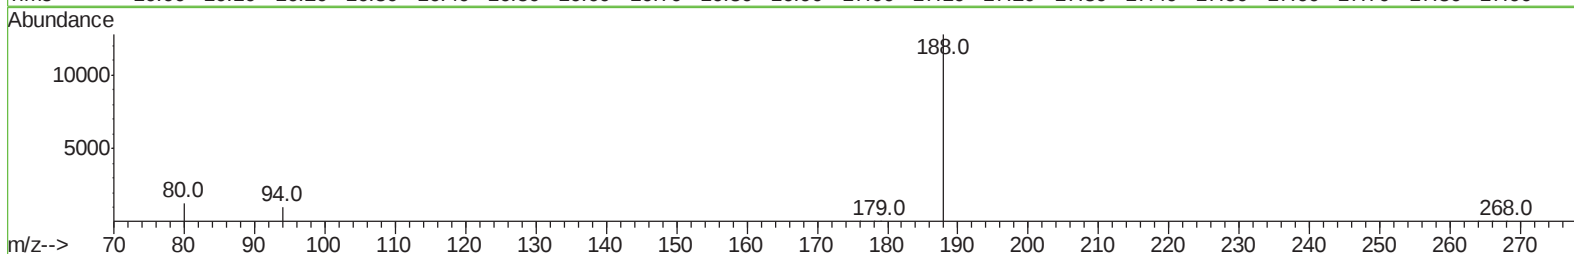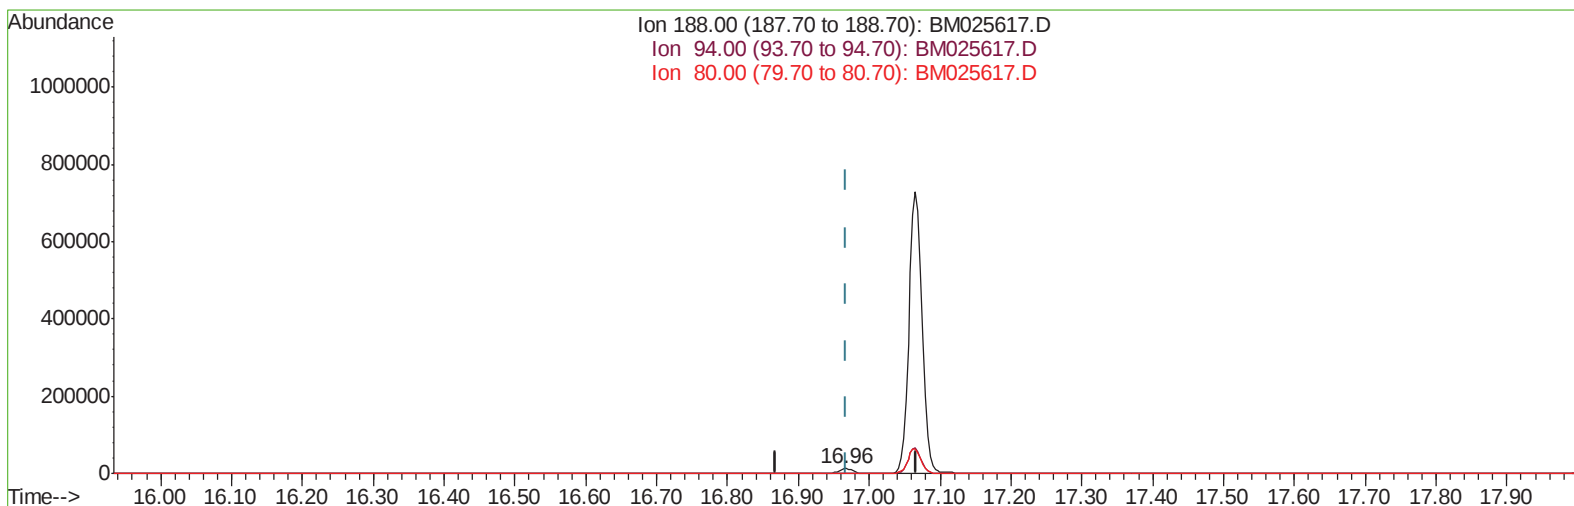

TIC: BM025617.D

(10) Phenanthrene-d10 (I)

16.964min (-0.004) 0.40ng/ul m

response 17281

Ion	Exp%	Act%
188.00	100	100
94.00	7.10	8.19
80.00	8.70	9.98
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031720\
 Data File : BM025617.D
 Acq On : 17 Mar 2020 19:08
 Operator : CG/JU
 Sample : L1516-09
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DBD27

Manual Integrations
 APPROVED

mohammad
 3/18/2020 9:02:02 AM

Quant Time: Mar 18 01:37:38 2020
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 17 17:05:05 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.59	152	2818	0.40	ng/ul	0.00
2) Naphthalene-d8	10.35	136	11309	0.40	ng/ul	0.00
6) Acenaphthene-d10	14.22	164	7626	0.40	ng/ul	0.00
10) Phenanthrene-d10	16.96	188	17281m	0.40	ng/ul	0.00
16) Chrysene-d12	21.16	240	18880	0.40	ng/ul	0.00
20) Perylene-d12	23.31	264	20948	0.40	ng/ul	0.00
System Monitoring Compounds						
4) 2-Methylnaphthalene-d10	11.95	152	4462	0.22	ng/ul	0.00
14) Fluoranthene-d10	19.00	212	11709	0.25	ng/ul	0.00
Target Compounds						
15) Fluoranthene	19.03	202	2268	0.038	ng/ul	86
17) Pyrene	19.39	202	1769	0.021	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031720\
Data File : BM025617.D
Acq On : 17 Mar 2020 19:08
Operator : CG/JU
Sample : L1516-09
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DBD27

Manual Integrations
APPROVED

mohammad
3/18/2020 9:02:02 AM

Quant Time: Mar 18 01:37:38 2020
Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM030920.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 17 17:05:05 2020
Response via : Initial Calibration

