

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
 Data File : BM034268.D
 Acq On : 17 Mar 2022 09:58
 Operator : CG/JU
 Sample : PB143208BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143208BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034268.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.502	378	385	395	rBV	4174914	6119294	47.11%	10.389%
2	7.107	650	658	676	rBV	3954101	6393752	49.22%	10.855%
3	7.943	793	800	810	rBV	774608	1249032	9.62%	2.121%
4	9.107	990	998	1010	rBV	2474485	4110029	31.64%	6.978%
5	10.760	1271	1279	1289	rBV	1016286	1742578	13.41%	2.959%
6	13.213	1689	1696	1708	rBV	6623323	9646572	74.26%	16.378%
7	14.583	1922	1929	1941	rBV	1633485	2374489	18.28%	4.031%
8	16.066	2174	2181	2204	rBV	5135770	7306541	56.25%	12.405%
9	17.324	2389	2395	2408	rBV	1797875	2630356	20.25%	4.466%
10	19.942	2834	2840	2859	rBV	10593097	12990442	100.00%	22.055%
11	21.495	3099	3104	3123	rBV	1569687	2378867	18.31%	4.039%
12	23.906	3507	3514	3527	rBV2	870296	1957663	15.07%	3.324%




Sum of corrected areas: 58899615

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
Data File : BM034268.D
Acq On : 17 Mar 2022 09:58
Operator : CG/JU
Sample : PB143208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

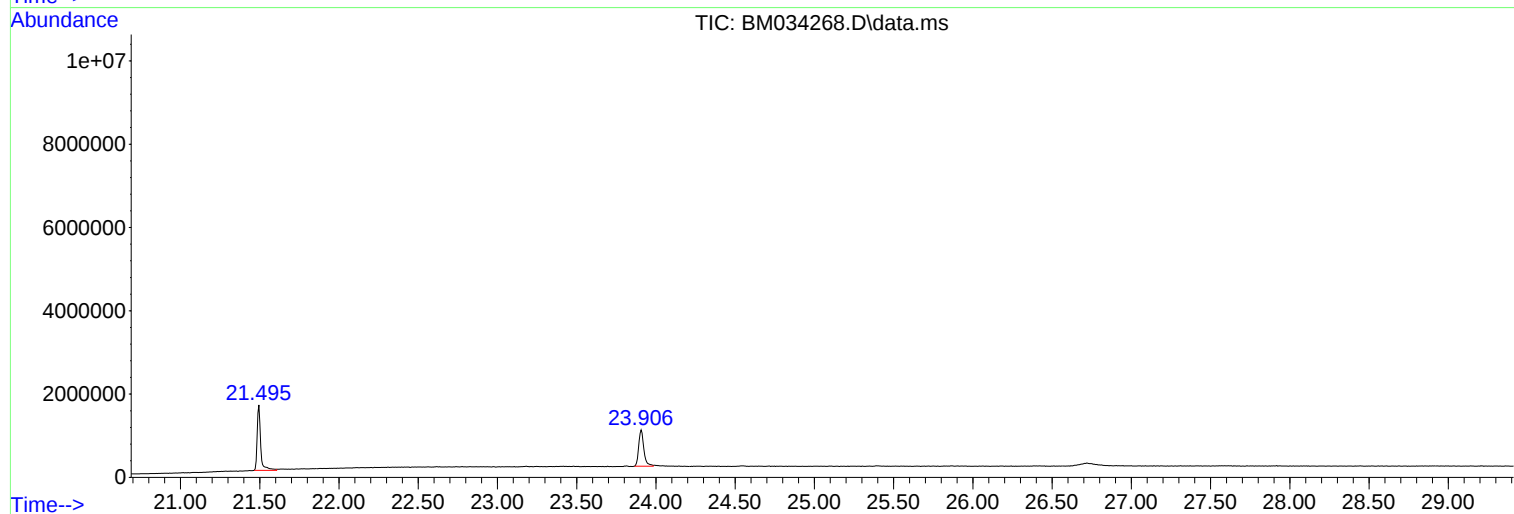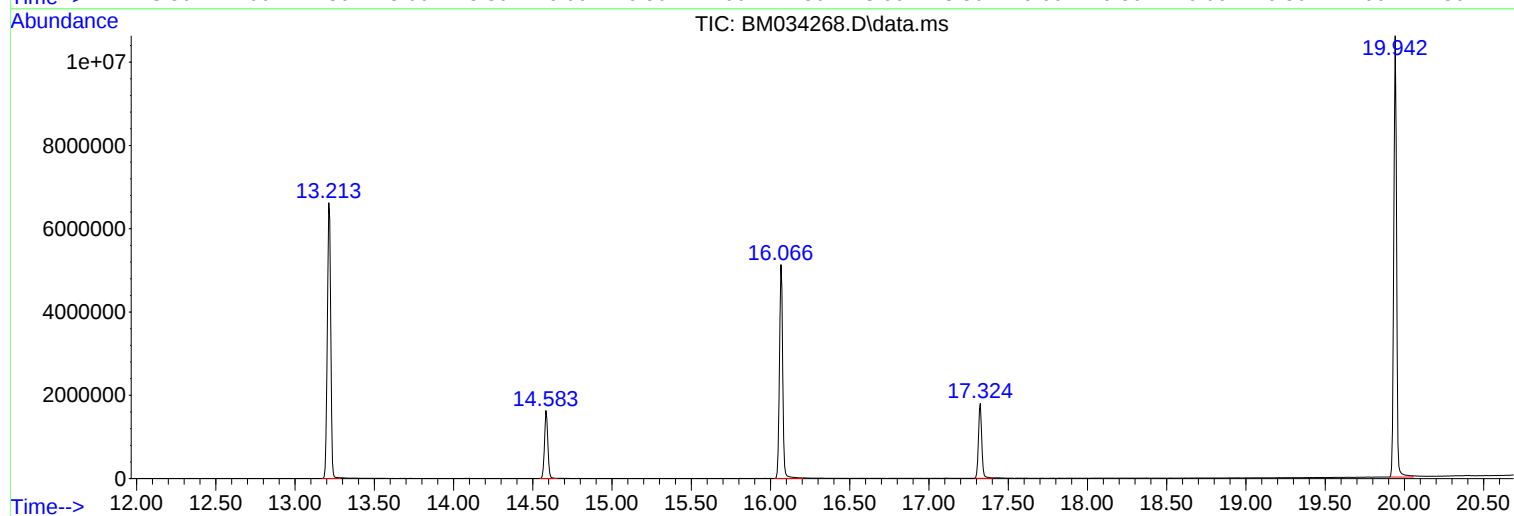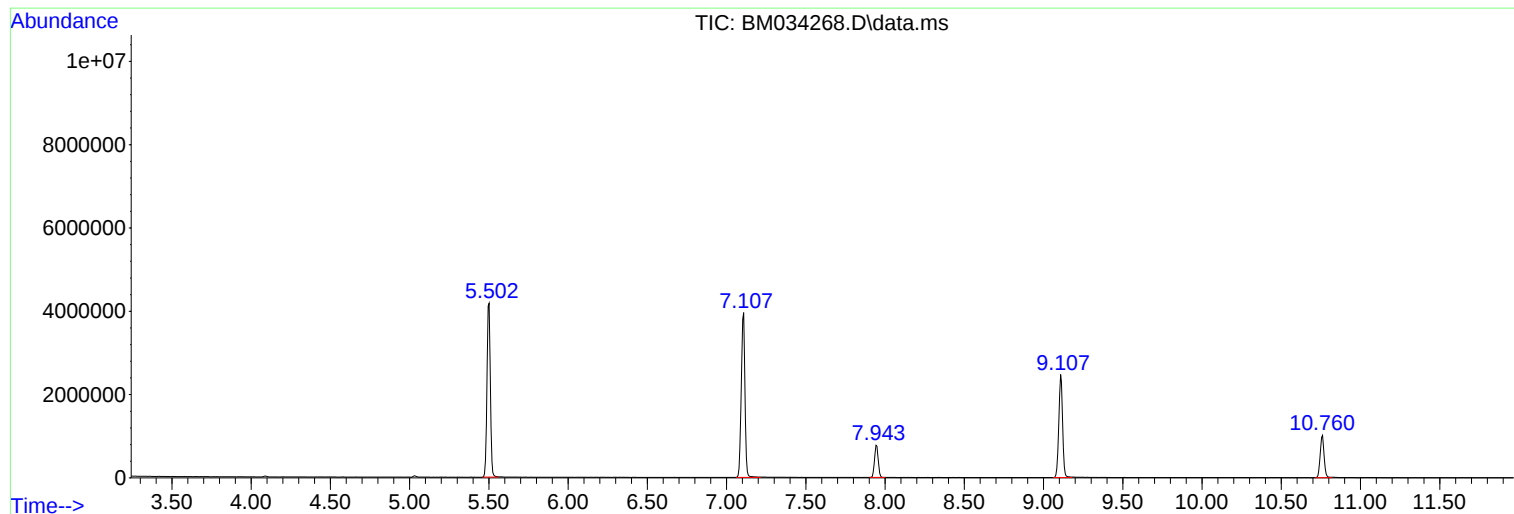

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
Data File : BM034268.D
Acq On : 17 Mar 2022 09:58
Operator : CG/JU
Sample : PB143208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
Data File : BM034268.D
Acq On : 17 Mar 2022 09:58
Operator : CG/JU
Sample : PB143208BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143208BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------