

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
 Data File : BM034271.D
 Acq On : 17 Mar 2022 11:47
 Operator : CG/JU
 Sample : PB143209BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143209BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034271.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.502	378	385	396	rBV	3780039	5520380	45.81%	10.280%
2	7.107	650	658	680	rBV	3644467	5814284	48.25%	10.828%
3	7.948	794	801	811	rVB	691920	1116374	9.26%	2.079%
4	9.107	990	998	1012	rBV	2197023	3691019	30.63%	6.874%
5	10.760	1271	1279	1288	rBV	878690	1528629	12.68%	2.847%
6	13.213	1689	1696	1708	rBV	5926222	8608864	71.44%	16.032%
7	14.583	1923	1929	1942	rBV	1433622	2110431	17.51%	3.930%
8	16.066	2174	2181	2206	rBV	4526555	6652334	55.20%	12.388%
9	17.324	2388	2395	2409	rBV	1606571	2375130	19.71%	4.423%
10	19.942	2834	2840	2860	rBV	9664508	12050955	100.00%	22.442%
11	21.495	3099	3104	3119	rBV	1492340	2234965	18.55%	4.162%
12	23.906	3507	3514	3527	rBV	890687	1995122	16.56%	3.715%




Sum of corrected areas: 53698487

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
Data File : BM034271.D
Acq On : 17 Mar 2022 11:47
Operator : CG/JU
Sample : PB143209BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143209BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

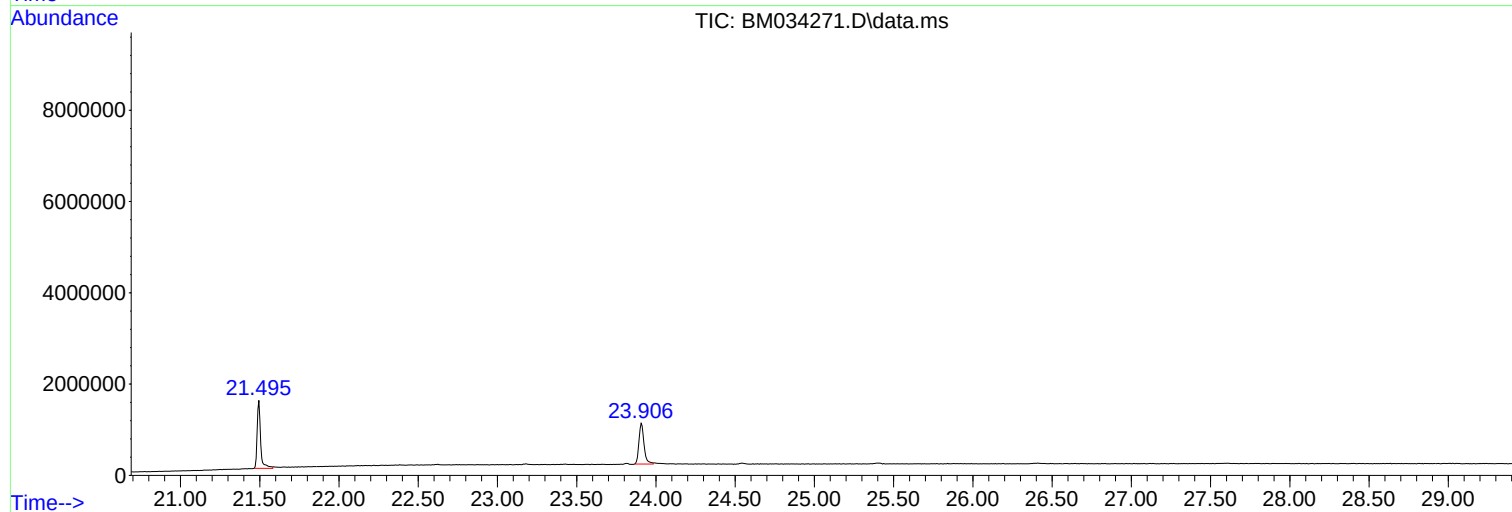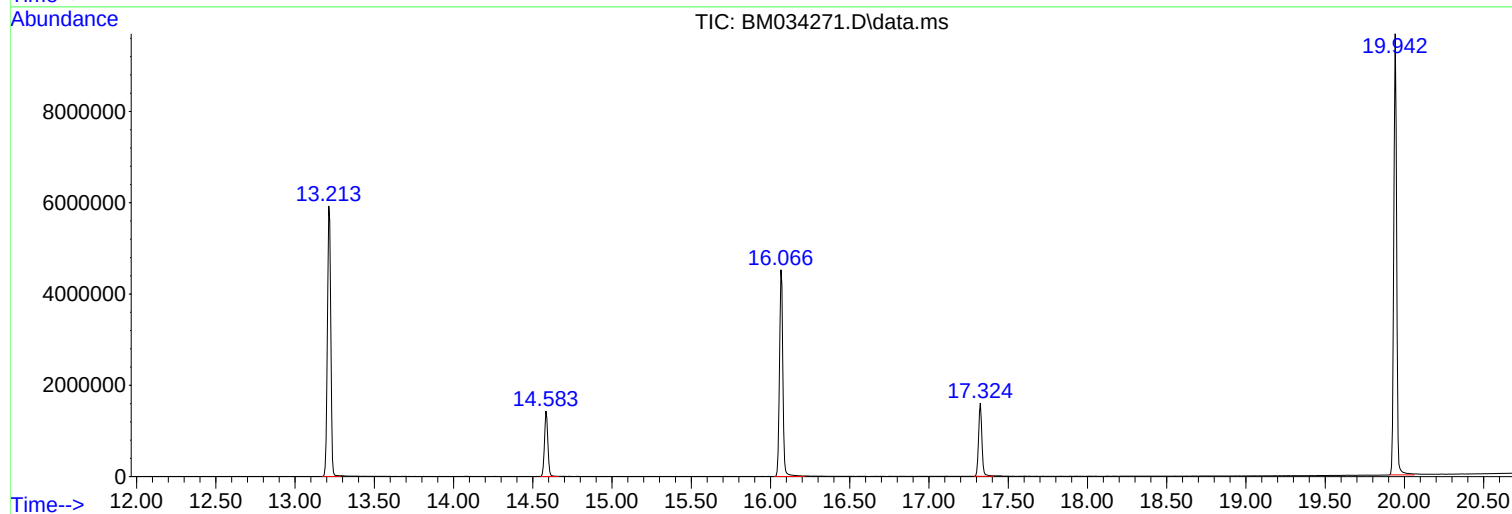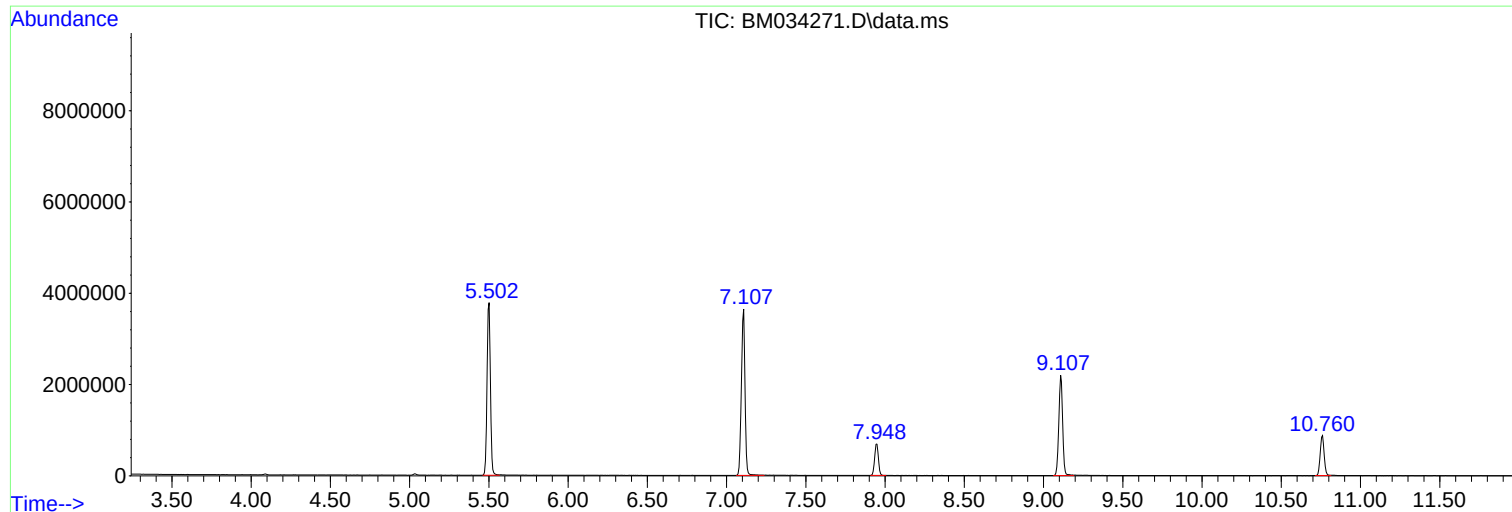

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
Data File : BM034271.D
Acq On : 17 Mar 2022 11:47
Operator : CG/JU
Sample : PB143209BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143209BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
Data File : BM034271.D
Acq On : 17 Mar 2022 11:47
Operator : CG/JU
Sample : PB143209BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143209BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------