


Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
 Data File : BM034266.D
 Acq On : 17 Mar 2022 08:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 16 02:38:26 2022

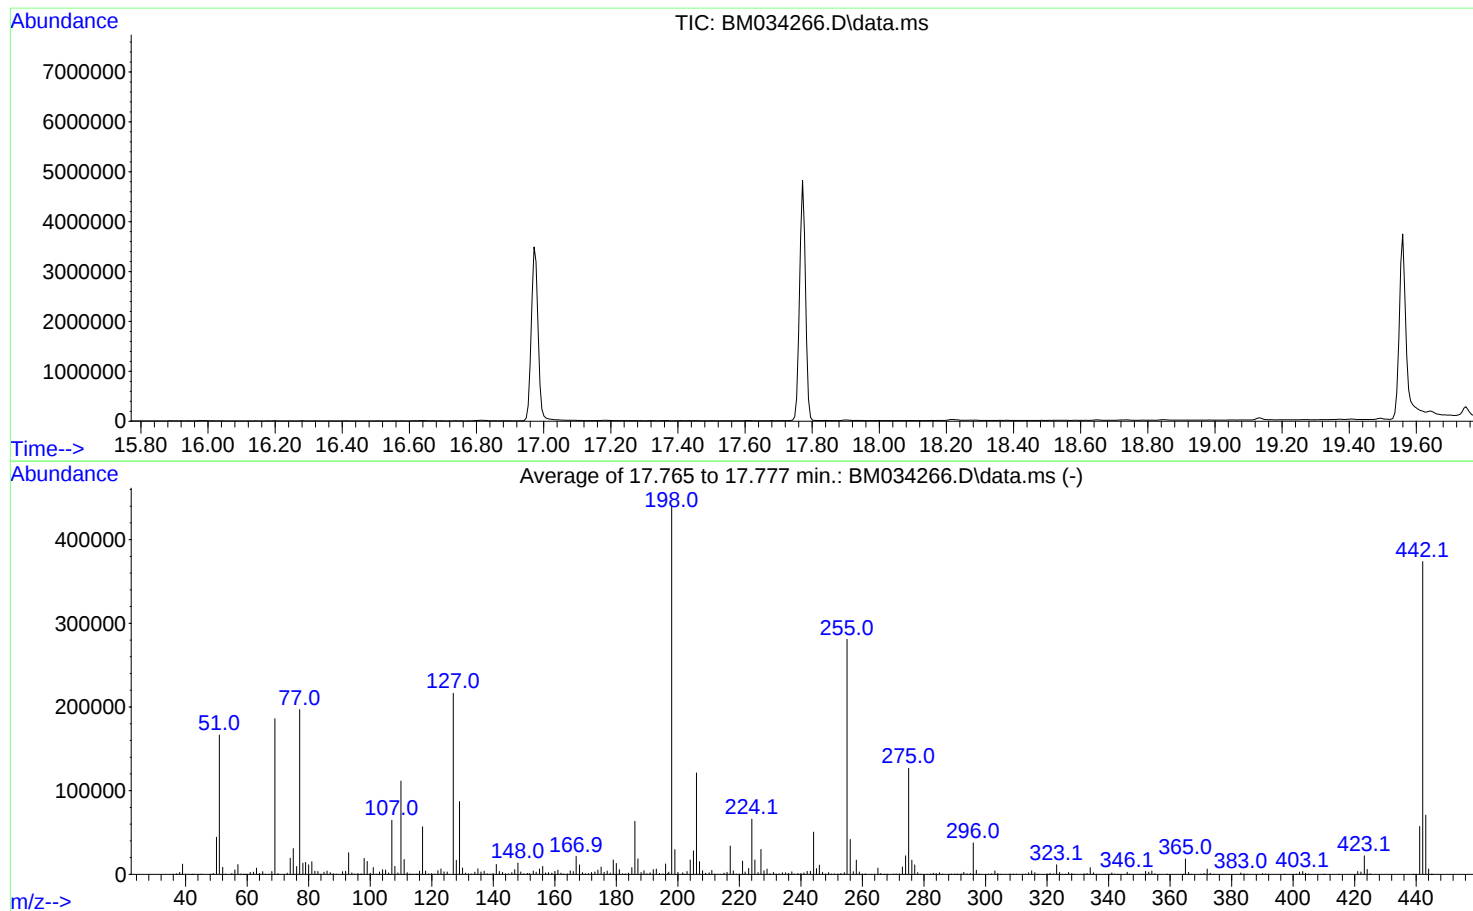




AutoFind: Scans 2470, 2471, 2472; Background Corrected with Scan 2463

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	37.9	166583	PASS
68	69	0.00	2	1.9	3457	PASS
69	198	0.00	100	42.3	186133	PASS
70	69	0.00	2	0.5	903	PASS
127	198	10	80	49.2	216427	PASS
197	198	0.00	2	0.6	2606	PASS
198	198	100	100	100.0	439595	PASS
199	198	5	9	6.7	29557	PASS
275	198	10	60	28.8	126763	PASS
365	198	1	100	4.2	18277	PASS
441	198	0.01	100	13.0	57251	PASS
442	442	50	100	100.0	373760	PASS
443	442	15	24	18.9	70811	PASS

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
 Data File : BM034266.D
 Acq On : 17 Mar 2022 08:46
 Operator : CG/JU
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Quant Time: Mar 17 14:34:26 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 16 02:38:26 2022
 Response via : Initial Calibration

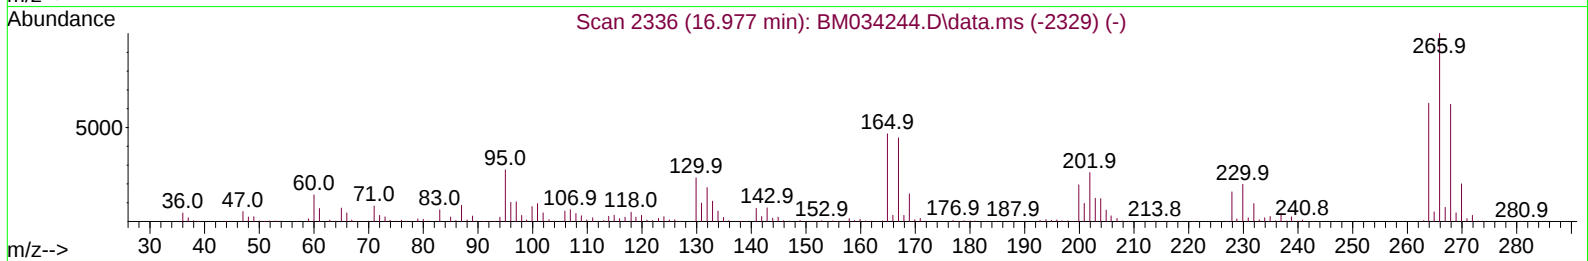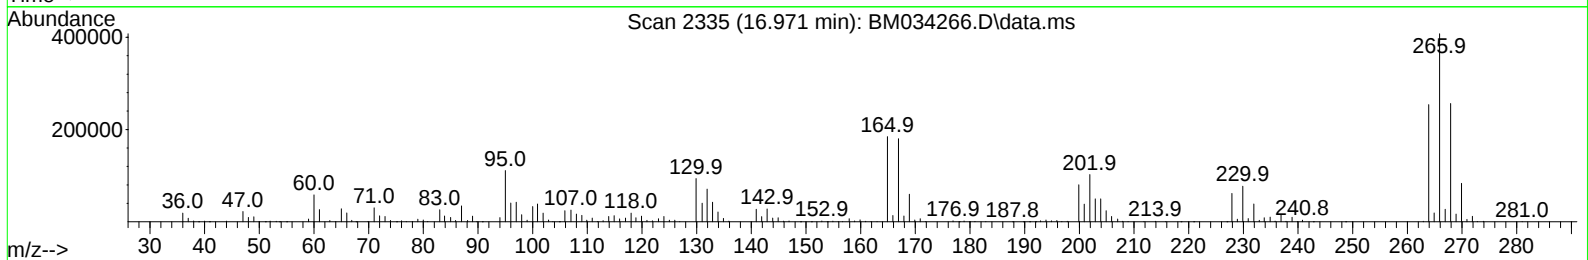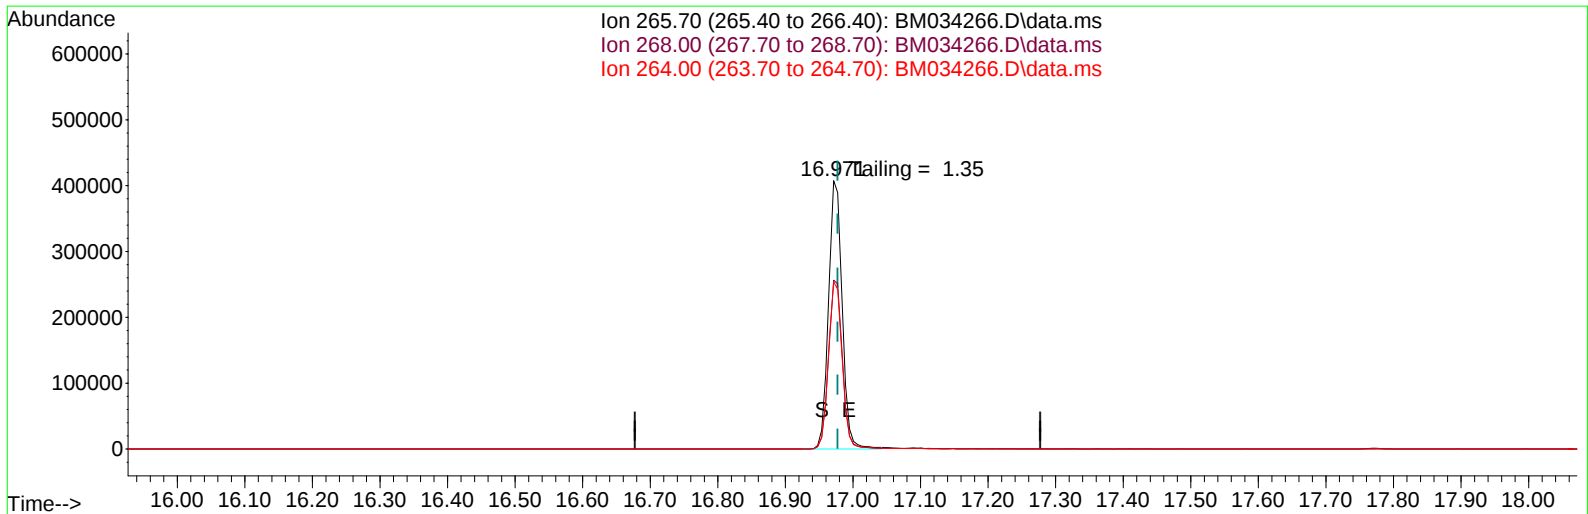

TIC: BM034266.D\data.ms

(70) Pentachlorophenol (C)

16.971min (-0.006) 78280.69 ng




response 574476

Ion	Exp%	Act%
265.70	100.00	100.00
268.00	62.30	62.91
264.00	62.90	62.33
0.00	0.00	0.00

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031722\
Data File : BM034266.D
Acq On : 17 Mar 2022 08:46
Operator : CG/JU
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP

Quant Time: Mar 17 14:34:26 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration

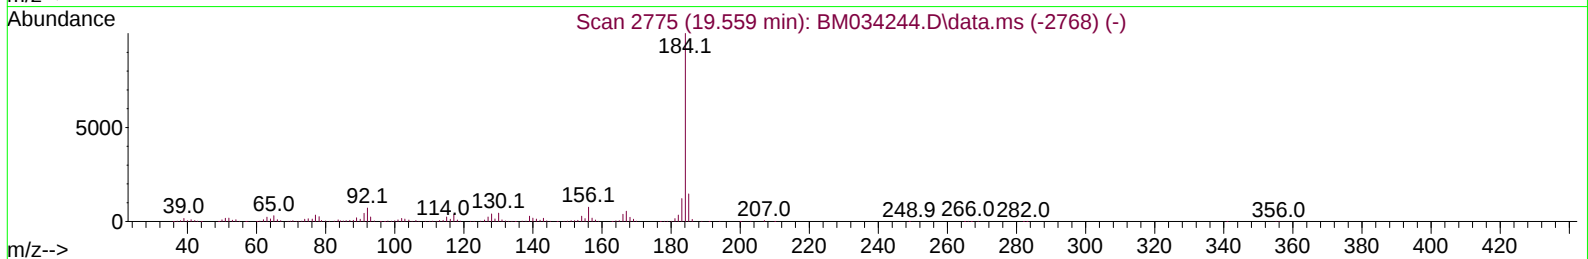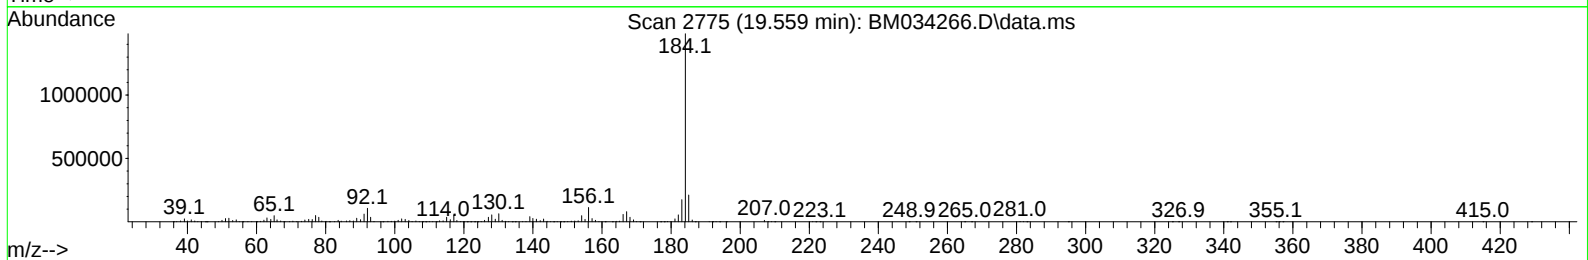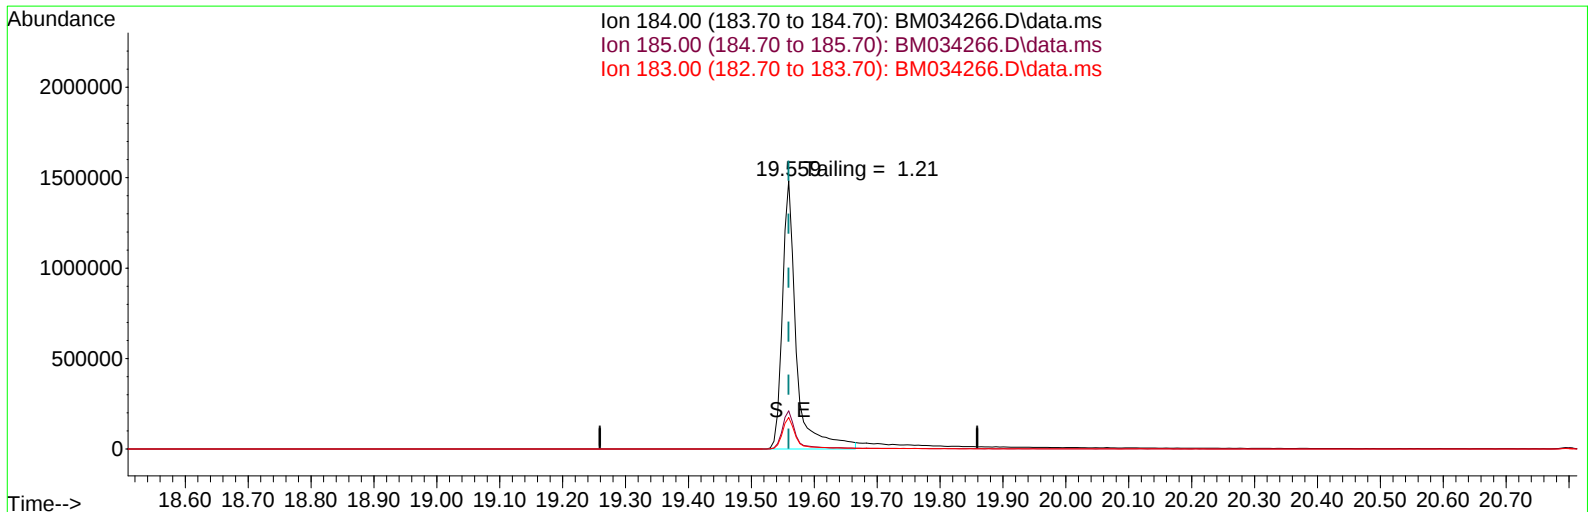

TIC: BM034266.D\data.ms

(77) Benzidine

19.559min (+ 0.000) 23641.02 ng

response 2490586

Ion	Exp%	Act%
184.00	100.00	100.00
185.00	14.60	14.27
183.00	12.20	11.75
0.00	0.00	0.00

DDT Breakdown

Date	Instrument Name	DFTPP Data File
3/17/2022	BNA_M	<u>BM034266.D</u>
Compound Name	Response	Retention Time
DDT	1675282	20.79
DDD	9991	20.35
DDE	1516	19.84
SUM(DDD+DDE)	SUM(DDT+DDD+DDE)	% Breakdown Of DDT
11507	1686789	0.68

Instrument :
BNA_M
ClientSampleId :
DFTPP