


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031816\
 Data File : BM004678.D
 Acq On : 18 Mar 2016 12:17
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM031816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 19 07:50:46 2016

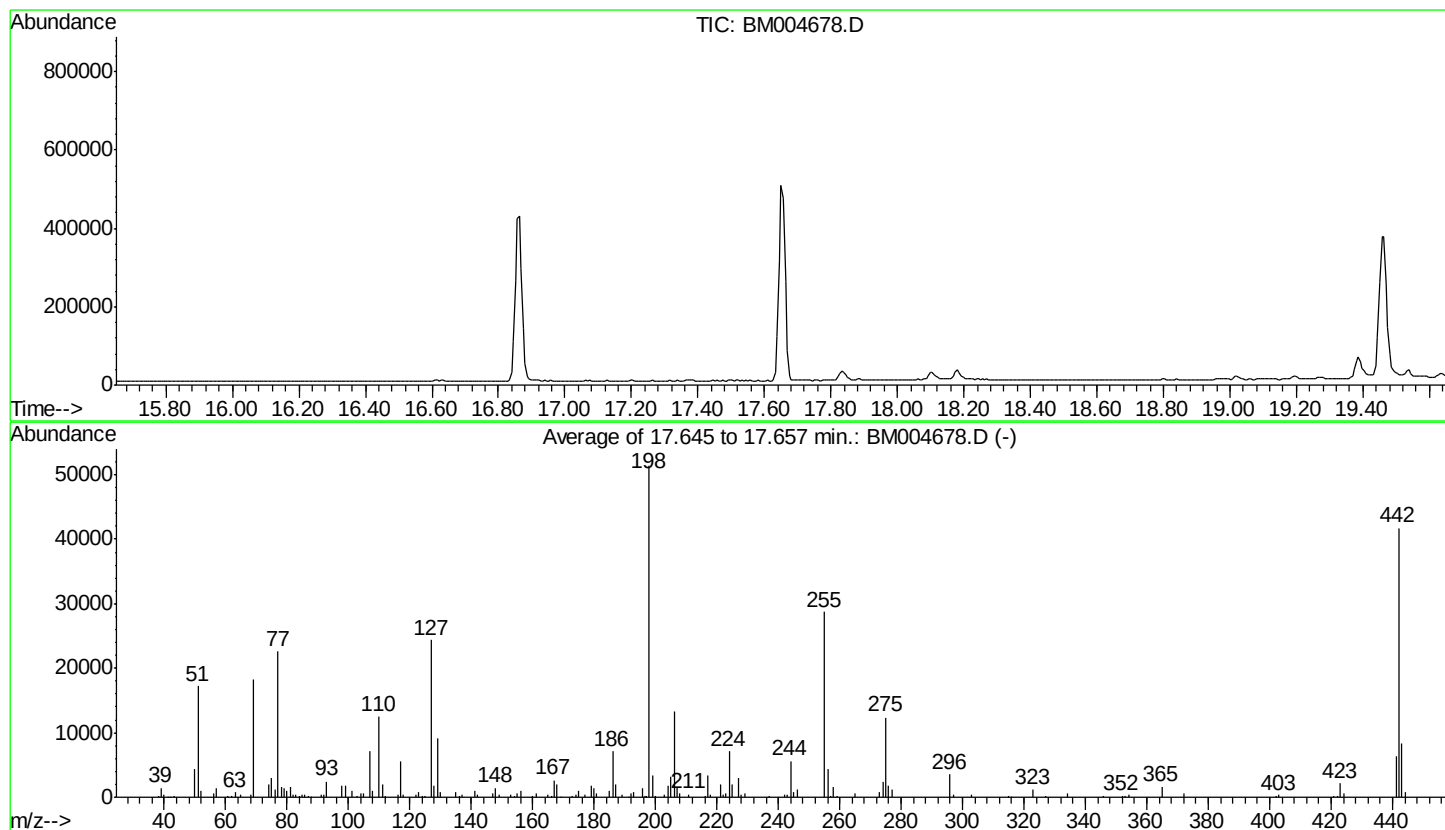

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.5	17209	PASS
68	69	0.00	2	1.9	348	PASS
69	198	0.00	100	35.5	18256	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	47.4	24354	PASS
197	198	0.00	2	0.5	236	PASS
198	198	100	100	100.0	51413	PASS
199	198	5	9	6.8	3477	PASS
275	198	10	60	24.1	12380	PASS
365	198	1	100	3.1	1599	PASS
441	442	0.01	24	15.2	6366	PASS
442	198	50	100	81.2	41760	PASS
443	442	15	24	20.0	8339	PASS