


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM031816\
 Data File : BM004688.D
 Acq On : 18 Mar 2016 18:56
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM031816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 19 07:50:46 2016

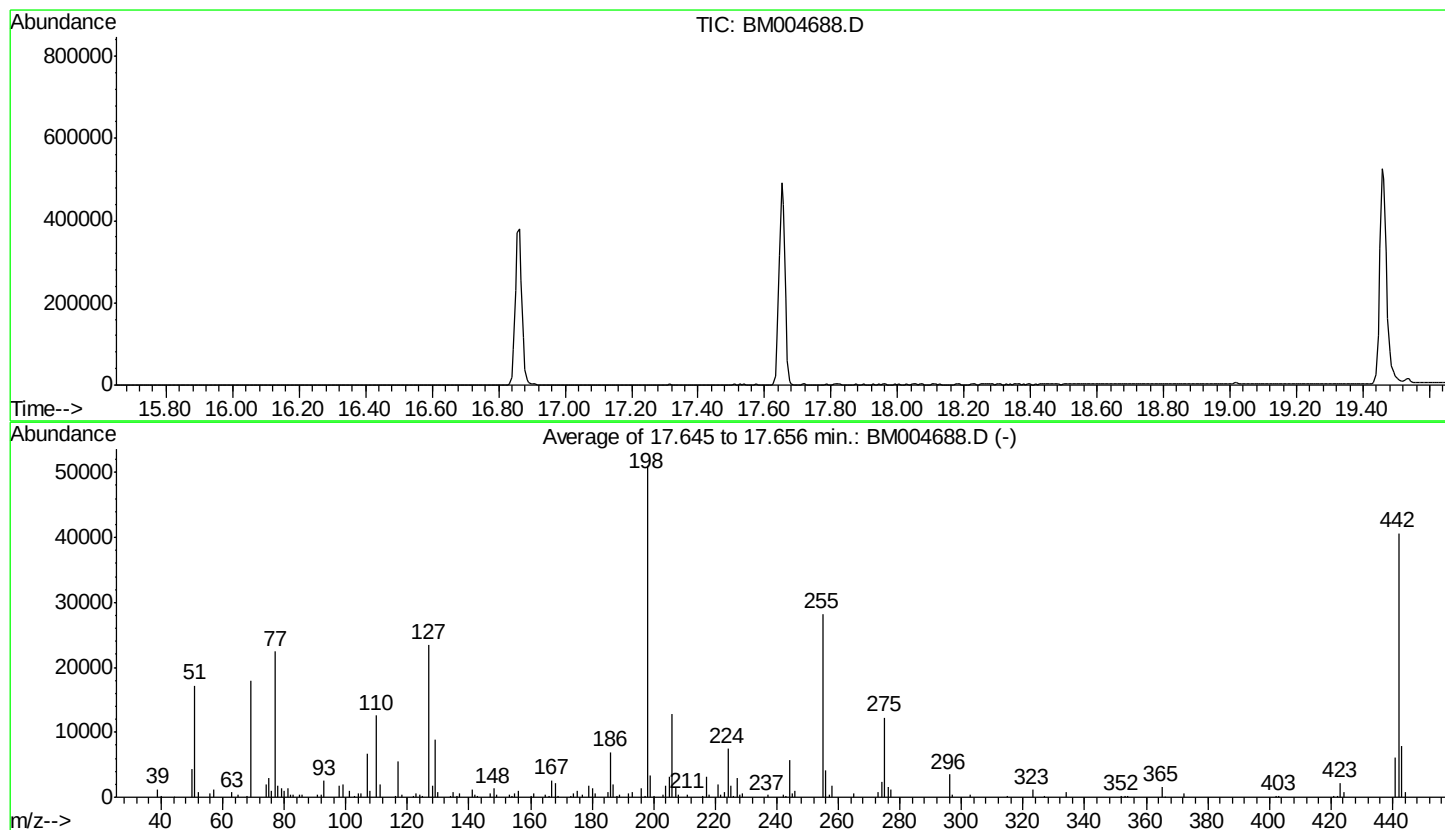

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.7	17193	PASS
68	69	0.00	2	1.3	233	PASS
69	198	0.00	100	35.2	17988	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	46.0	23464	PASS
197	198	0.00	2	0.5	237	PASS
198	198	100	100	100.0	51053	PASS
199	198	5	9	6.7	3438	PASS
275	198	10	60	24.1	12279	PASS
365	198	1	100	3.1	1596	PASS
441	442	0.01	24	15.1	6154	PASS
442	198	50	100	79.6	40621	PASS
443	442	15	24	19.3	7843	PASS