


Data Path : Z:\HPCHEM1\BNA_M\Data\BM031915\
 Data File : BM000724.D
 Acq On : 19 Mar 2015 10:06
 Operator : TP/IZ
 Sample : DFTPP40
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP40

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM031915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 15:39:49 2015

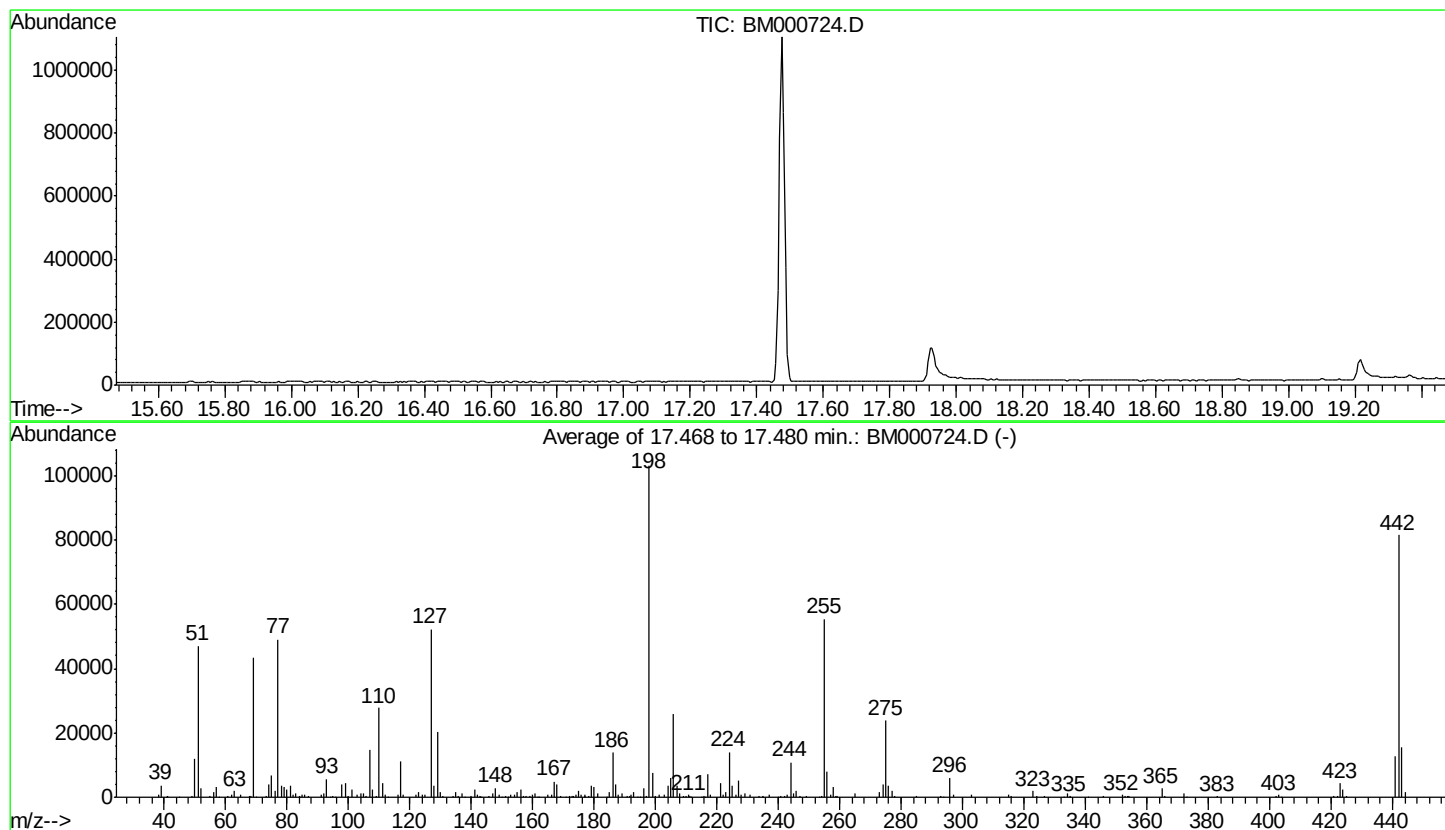

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.7	47154	PASS
68	69	0.00	2	1.2	522	PASS
69	198	0.00	100	42.2	43472	PASS
70	69	0.00	2	0.3	119	PASS
127	198	10	80	50.8	52317	PASS
197	198	0.00	2	0.5	473	PASS
198	198	100	100	100.0	103074	PASS
199	198	5	9	7.5	7744	PASS
275	198	10	60	23.1	23850	PASS
365	198	1	100	2.6	2699	PASS
441	443	0.01	100	81.4	12797	PASS
442	198	50	100	79.0	81453	PASS
443	442	15	24	19.3	15715	PASS