

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031921\
 Data File : BM029169.D
 Acq On : 19 Mar 2021 14:14
 Operator : CG/JU
 Sample : M1344-01
 Misc : SFAM-MDL-W-01
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Manual Integrations
 APPROVED

mohammad
 3/22/2021 2:48:48 PM

Quant Time: Mar 19 14:48:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM031921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 19 12:41:26 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.77	152	78840	20.00	ng/ul	0.00
20) Naphthalene-d8	10.55	136	298411	20.00	ng/ul	0.00
38) Acenaphthene-d10	14.39	164	188067	20.00	ng/ul	0.00
64) Phenanthrene-d10	17.13	188	415855	20.00	ng/ul	0.00
79) Chrysene-d12	21.30	240	469859	20.00	ng/ul	0.00
88) Perylene-d12	23.54	264	507789	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.29	96	8462	4.22	ng/uL	0.00
4) Pyridine-d5	3.69	84	133829	25.53	ng/ul	0.00
7) Phenol-d5	6.93	99	192704	30.95	ng/ul	0.00
9) Bis-(2-Chloroethyl)ether-d	7.11	67	120556	33.50	ng/ul	0.00
11) 2-Chlorophenol-d4	7.30	132	160054	33.03	ng/ul	0.00
15) 4-Methylphenol-d8	8.47	113	148805	30.79	ng/ul	0.00
21) Nitrobenzene-d5	8.92	128	65993	34.77	ng/ul	0.00
24) 2-Nitrophenol-d4	9.64	143	64523	35.66	ng/ul	0.00
28) 2,4-Dichlorophenol-d3	10.17	165	149696	31.57	ng/ul	0.00
31) 4-Chloroaniline-d4	10.69	131	201701	30.07	ng/ul	0.00
46) Dimethylphthalate-d6	13.81	166	474357	33.44	ng/ul	0.00
49) Acenaphthylene-d8	14.09	160	571460	34.08	ng/ul	0.00
54) 4-Nitrophenol-d4	14.57	143	68280	29.56	ng/ul	0.00
60) Fluorene-d10	15.39	176	405955	33.26	ng/ul	0.00
65) 4,6-Dinitro-2-methylphenol	15.49	200	51332	26.18	ng/ul	0.00
73) Anthracene-d10	17.23	188	634965	31.97	ng/ul	0.00
81) Pyrene-d10	19.52	212	731037	33.34	ng/ul	0.00
92) Benzo(a)pyrene-d12	23.40	264	908098	33.59	ng/ul	0.00

Target Compounds

					Ovalue
2) 1,4-Dioxane	3.32	88	2710	1.346	ng/uL 92
5) Pyridine	3.71	79	22723	4.219	ng/ul# 54
6) Benzaldehyde	6.92	77	17386	5.203	ng/ul 95
8) Phenol	6.96	94	29265	4.472	ng/ul 95
10) Bis(2-Chloroethyl)ether	7.20	93	21495	4.445	ng/ul 93
12) 2-Chlorophenol	7.33	128	23603	4.565	ng/ul 99
13) 2-Methylphenol	8.20	108	20005	4.144	ng/ul 94
14) 2,2'-oxybis(1-Chloropropan	8.30	45	29024	4.580	ng/ul 97
16) Acetophenone	8.59	105	34981	4.429	ng/ul 94
17) N-Nitroso-di-n-propylamine	8.57	70	17026	4.532	ng/ul 98
18) 4-Methylphenol	8.53	108	22209	4.333	ng/ul 97
19) Hexachloroethane	8.85	117	9768	4.411	ng/ul 92
22) Nitrobenzene	8.96	77	27664	4.999	ng/ul 94
23) Isophorone	9.49	82	43914	4.442	ng/ul 99
25) 2-Nitrophenol	9.67	139	10402	4.990	ng/ul 94
26) 2,4-Dimethylphenol	9.73	107	25589	4.517	ng/ul 95
27) Bis(2-Chloroethoxy)methane	9.97	93	26382	4.467	ng/ul 98
29) 2,4-Dichlorophenol	10.20	162	22129	4.611	ng/ul 91
30) Naphthalene	10.60	128	73966	4.575	ng/ul 99
32) 4-Chloroaniline	10.70	127	30205	4.427	ng/ul 100
33) Hexachlorobutadiene	10.89	225	15140	4.393	ng/ul 97
34) Caprolactam	11.48	113	4687m	3.843	ng/ul

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031921\
 Data File : BM029169.D
 Acq On : 19 Mar 2021 14:14
 Operator : CG/JU
 Sample : M1344-01
 Misc : SFAM-MDL-W-01
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Manual Integrations
 APPROVED

mohammad
 3/22/2021 2:48:48 PM

Quant Time: Mar 19 14:48:13 2021
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM031921.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 19 12:41:26 2021
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
35) 4-Chloro-3-methylphenol	11.83	107	20458	4.388	ng/ul	96
36) 2-Methylnaphthalene	12.22	142	52871	4.629	ng/ul	95
37) 1-Methylnaphthalene	12.43	142	51078	4.530	ng/ul#	98
39) 1,2,4,5-Tetrachlorobenzene	12.58	216	27998	4.309	ng/ul	98
40) Hexachlorocyclopentadiene	12.57	237	15752	3.690	ng/ul	93
41) 2,4,6-Trichlorophenol	12.82	196	14765	4.132	ng/ul	91
42) 2,4,5-Trichlorophenol	12.89	196	17217	4.525	ng/ul	84
43) 1,1'-Biphenyl	13.23	154	67276	4.394	ng/ul#	97
44) 2-Chloronaphthalene	13.27	162	51985	4.301	ng/ul	99
45) 2-Nitroaniline	13.47	65	10890	4.200	ng/ul	96
47) Dimethylphthalate	13.86	163	66203	4.560	ng/ul	98
48) 2,6-Dinitrotoluene	13.96	165	9341	4.134	ng/ul	97
50) Acenaphthylene	14.12	152	79779	4.600	ng/ul	99
51) 3-Nitroaniline	14.29	138	9380	3.754	ng/ul	98
52) Acenaphthene	14.46	153	56940	4.422	ng/ul	98
53) 2,4-Dinitrophenol	14.50	184	3981	3.284	ng/ul	90
55) 4-Nitrophenol	14.59	109	9481	4.314	ng/ul#	80
56) Dibenzofuran	14.79	168	81897	4.576	ng/ul	100
57) 2,4-Dinitrotoluene	14.75	165	13632	4.228	ng/ul	95
58) 2,3,4,6-Tetrachlorophenol	15.02	232	12429	4.076	ng/ul#	92
59) Diethylphthalate	15.22	149	64224	4.493	ng/ul	97
61) Fluorene	15.44	166	68085	4.547	ng/ul	100
62) 4-Chlorophenyl-phenylether	15.44	204	33222	4.420	ng/ul	94
63) 4-Nitroaniline	15.44	138	10181	3.904	ng/ul	93
66) 4,6-Dinitro-2-methylphenol	15.51	198	7915	3.838	ng/ul#	84
67) N-Nitrosodiphenylamine	15.65	169	55624	4.187	ng/ul	95
68) 4-Bromophenyl-phenylether	16.33	248	18671	4.219	ng/ul	93
69) Hexachlorobenzene	16.44	284	22095	4.482	ng/ul	98
70) Atrazine	16.60	200	19064	3.746	ng/ul	97
71) Pentachlorophenol	16.77	266	9062	3.237	ng/ul	96
72) Phenanthrene	17.17	178	111110	4.526	ng/ul	99
74) Anthracene	17.26	178	113498	4.499	ng/ul	99
75) 1,2,3,4-Tetrachlorobenzene	13.19	216	28309	4.215	ng/uL	99
76) Pentachlorobenzene	14.71	250	25361	3.868	ng/uL	98
77) Carbazole	17.53	167	98260	4.232	ng/ul	98
78) Di-n-butylphthalate	18.10	149	93459	3.897	ng/ul	98
80) Fluoranthene	19.18	202	125740	4.463	ng/ul	99
82) Pyrene	19.54	202	139777	4.733	ng/ul#	98
83) Butylbenzylphthalate	20.45	149	37997	3.662	ng/ul	98
84) 3,3'-Dichlorobenzidine	21.22	252	38058	3.911	ng/ul	94
85) Benzo(a)anthracene	21.28	228	133593	4.407	ng/ul	99
86) Bis(2-ethylhexyl)phthalate	21.23	149	59331	3.479	ng/ul	100
87) Chrysene	21.33	228	136686	4.612	ng/ul	99
89) Di-n-octyl phthalate	22.11	149	99707	3.078	ng/ul	100
90) Benzo(b)fluoranthene	22.86	252	149227	4.547	ng/ul	99
91) Benzo(k)fluoranthene	22.90	252	140193	4.275	ng/ul	100
93) Benzo(a)pyrene	23.44	252	134618	4.527	ng/ul	97
94) Indeno(1,2,3-cd)pyrene	25.80	276	173518	4.339	ng/ul	98
95) Dibenzo(a,h)anthracene	25.81	278	144432	4.281	ng/ul	99
96) Benzo(g,h,i)perylene	26.49	276	143966	4.390	ng/ul	99

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM031921\
Data File : BM029169.D
Acq On : 19 Mar 2021 14:14
Operator : CG/JU
Sample : M1344-01
Misc : SFAM-MDL-W-01
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03


Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

Quant Time: Mar 19 14:48:13 2021
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\SFAM-EPA-BM031921.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 19 12:41:26 2021
Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
--------------------	------	------	----------	------	-------	----------

(#) = qualifier out of range (m) = manual integration (+) = signals summed



#2

1,4-Dioxane

Concen: 1.346 ng/uL

RT: 3.32 min Scan# 73

Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion:	88	Resp:	2710
Ion	Ratio	Lower	Upper
88	100		
43	40.8	28.7	43.1
58	65.1	57.7	86.5

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

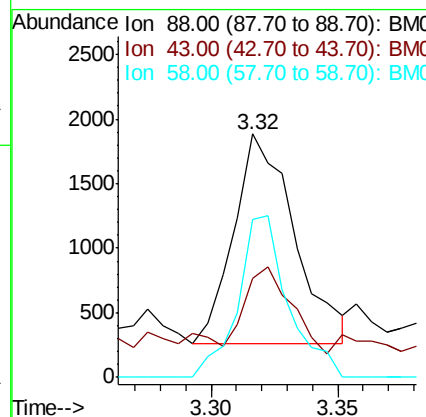

#5

Pyridine

Concen: 4.219 ng/uL




RT: 3.71 min Scan# 140


Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Tgt Ion:	79	Resp:	22723
Ion	Ratio	Lower	Upper
79	100		
52	129.9	60.6	91.0#
51	45.2	30.2	45.2

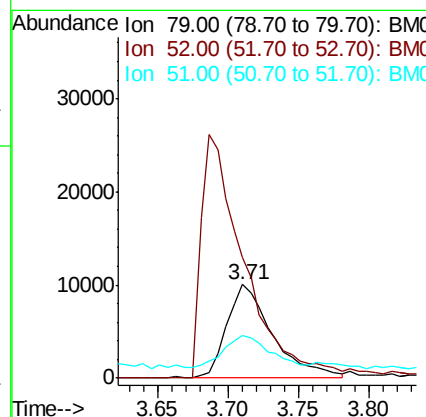



#6

Benzaldehyde

Concen: 5.203 ng/ul

RT: 6.92 min Scan# 686

Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
77	100		
105	95.5	74.8	112.2
106	78.5	69.0	103.6

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM



#8

Phenol

Concen: 4.472 ng/ul




RT: 6.96 min Scan# 692


Delta R.T. -0.01 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
94	100		
65	36.0	25.1	37.7
66	46.3	35.4	53.0









#10
Bis(2-Chloroethyl)ether
Concen: 4.445 ng/ul
RT: 7.20 min Scan# 734
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
93	100		
63	71.2	63.7	95.5
95	34.3	26.3	39.5




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

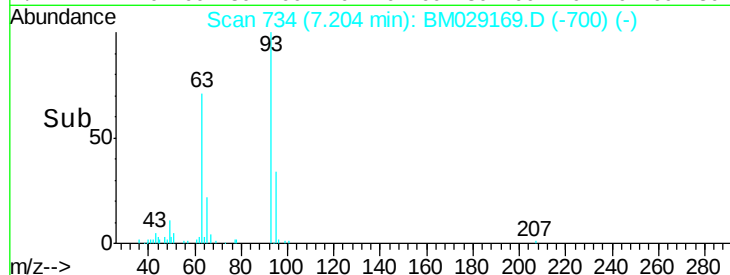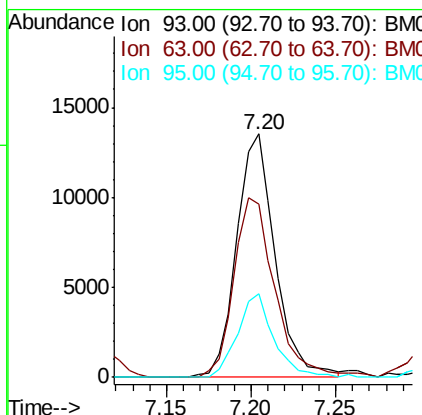

#12
2-Chlorophenol
Concen: 4.565 ng/ul
RT: 7.33 min Scan# 756
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
128	100		
64	47.6	37.5	56.3
130	32.2	26.5	39.7









#13
2-Methylphenol
Concen: 4.144 ng/ul
RT: 8.20 min Scan# 904
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
108	100		
107	84.7	71.9	107.9




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

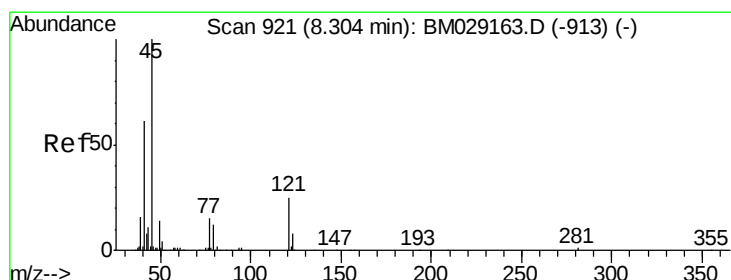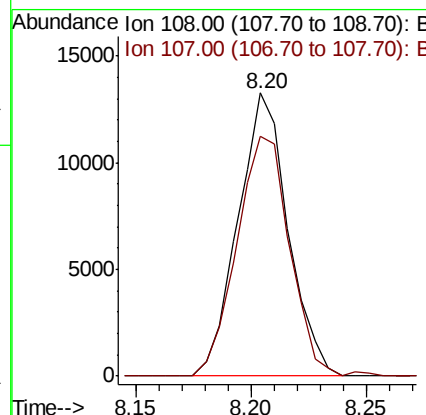

#14
2,2'-oxybis(1-Chloropropane)
Concen: 4.580 ng/ul
RT: 8.30 min Scan# 921
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
45	100		
77	17.4	12.7	19.1
79	11.2	9.8	14.6

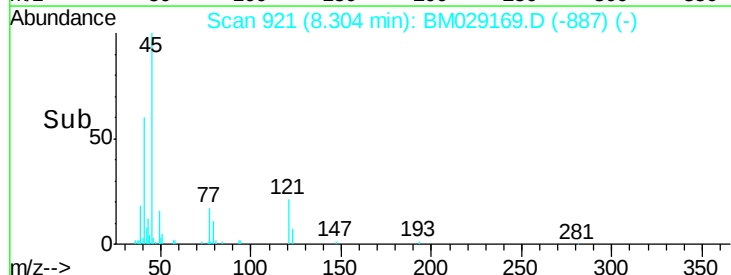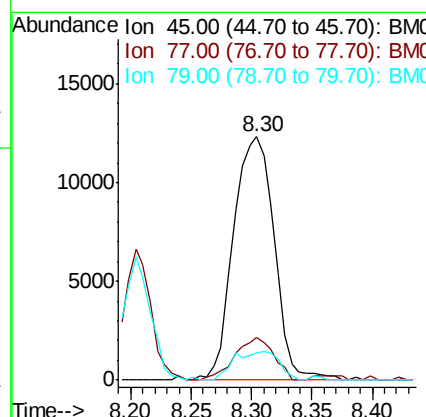







#16
Acetophenone
Concen: 4.429 ng/ul
RT: 8.59 min Scan# 969
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion:	105	Resp:	34981
Ion Ratio	Lower	Upper	
105	100		
77	88.0	66.2	99.2
51	32.8	23.2	34.8




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

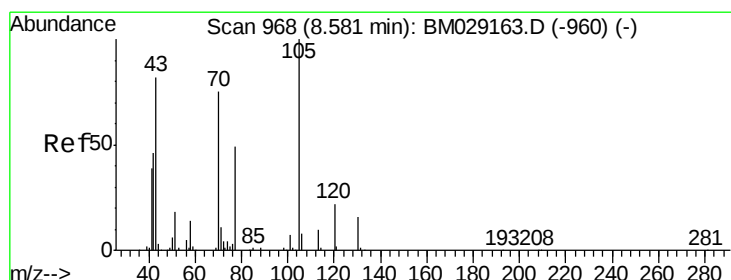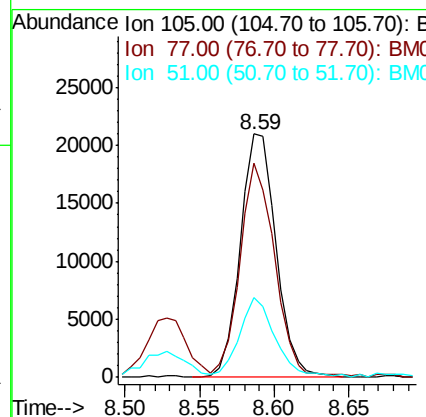

#17
N-Nitroso-di-n-propylamine
Concen: 4.532 ng/ul
RT: 8.57 min Scan# 967
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion:	70	Resp:	17026
Ion Ratio	Lower	Upper	
70	100		
42	63.2	50.7	76.1
101	9.4	7.0	10.4
130	23.9	16.9	25.3

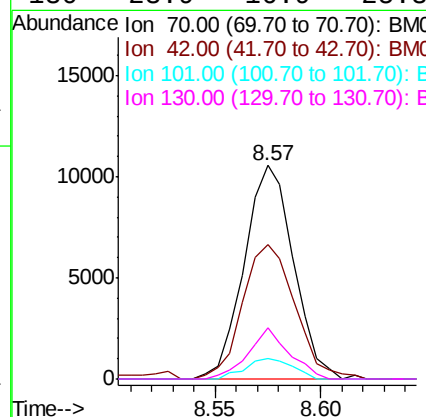

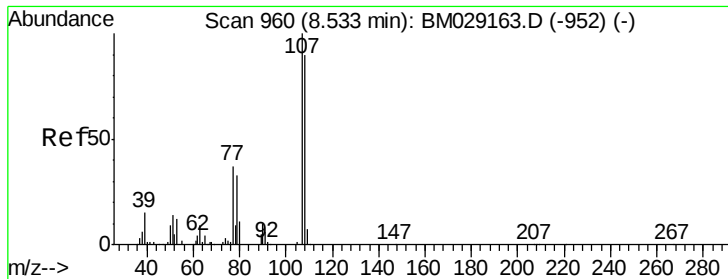





#18
4-Methylphenol
Concen: 4.333 ng/ul
RT: 8.53 min Scan# 960
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
108	100		
107	107.3	88.8	133.2




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

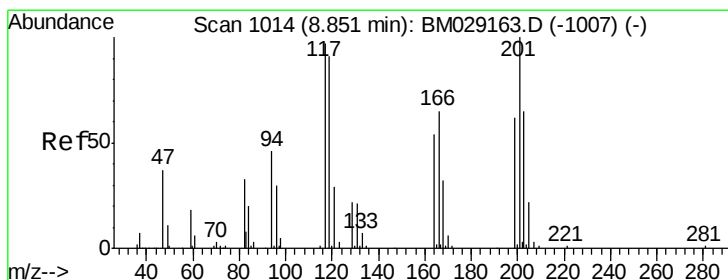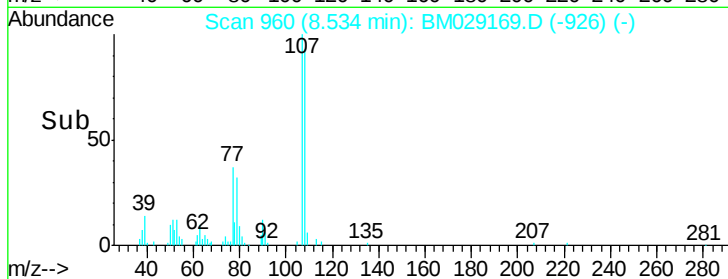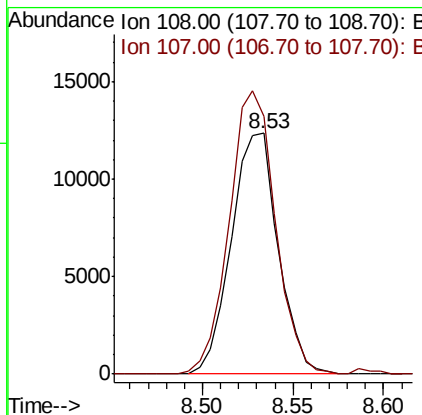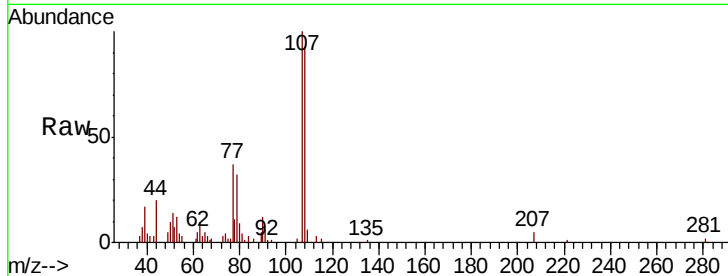

#19
Hexachloroethane
Concen: 4.411 ng/ul
RT: 8.85 min Scan# 1013
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
117	100		
201	107.2	82.4	123.6
199	53.6	51.0	76.6

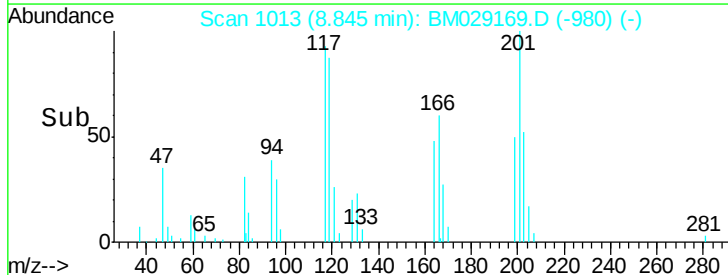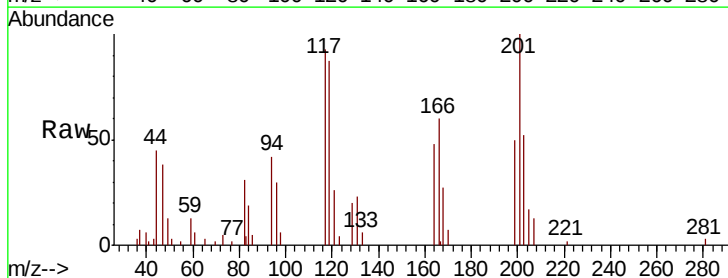







#22
Nitrobenzene
Concen: 4.999 ng/ul
RT: 8.96 min Scan# 1033
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
77	100		
123	43.4	30.9	46.3
65	13.5	10.2	15.4




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM



#23
Isophorone
Concen: 4.442 ng/ul
RT: 9.49 min Scan# 1122
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
82	100		
95	7.4	6.2	9.2
138	18.3	15.1	22.7









#25
2-Nitrophenol
Concen: 4.990 ng/ul
RT: 9.67 min Scan# 1153
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
139	100		
65	60.0	46.2	69.4
109	27.7	27.0	40.4




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

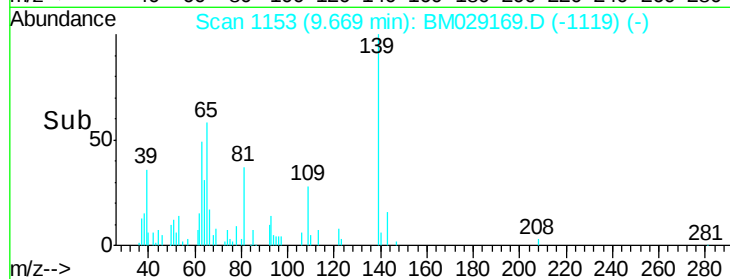

#26
2,4-Dimethylphenol
Concen: 4.517 ng/ul
RT: 9.73 min Scan# 1163
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
107	100		
121	53.3	40.2	60.2
122	78.3	66.2	99.2



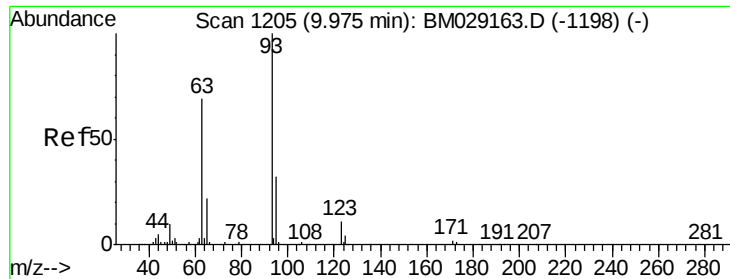





#27
 Bis(2-Chloroethoxy)methane
 Concen: 4.467 ng/ul
 RT: 9.97 min Scan# 1204
 Delta R.T. -0.01 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Tot Ion:	93	Resp:	26382
Ion	Ratio	Lower	Upper
93	100		
95	32.7	25.6	38.4
123	12.2	9.0	13.4




Manual Integrations
 APPROVED


mohammad
 3/22/2021 2:48:48 PM

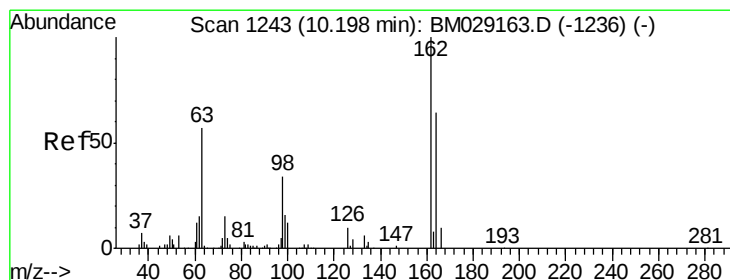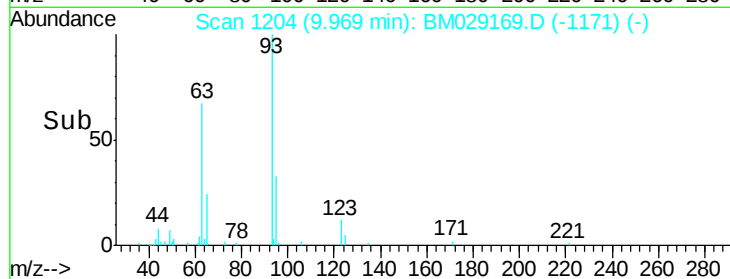

#29
 2,4-Dichlorophenol
 Concen: 4.611 ng/ul
 RT: 10.20 min Scan# 1243
 Delta R.T. 0.00 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Tgt Ion:	162	Resp:	22129
Ion	Ratio	Lower	Upper
162	100		
164	74.9	51.8	77.6
98	33.6	27.2	40.8









#30
Naphthalene
Concen: 4.575 ng/ul
RT: 10.60 min Scan# 1312
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
128	100		
129	10.9	8.6	13.0
127	12.9	10.7	16.1




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

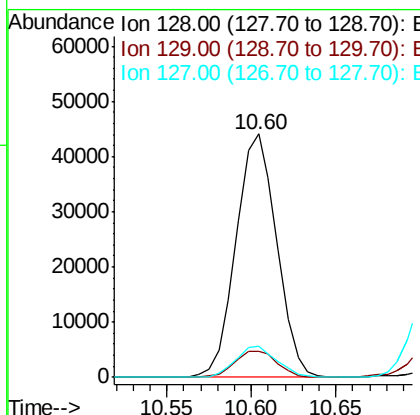

#32
4-Chloroaniline
Concen: 4.427 ng/ul
RT: 10.70 min Scan# 1329
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
127	100		
129	33.3	26.6	39.8









#33
Hexachlorobutadiene
Concen: 4.393 ng/ul
RT: 10.89 min Scan# 1361
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
225	100		
223	63.6	49.3	73.9
227	61.2	46.9	70.3




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

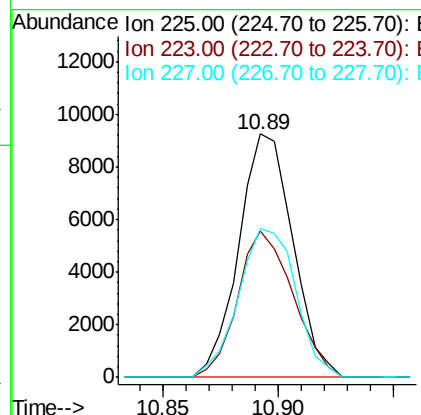

#34
Caprolactam
Concen: 3.843 ng/ul m
RT: 11.48 min Scan# 1461
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
113	100		
55	160.3	116.7	175.1
56	120.6	91.4	137.0

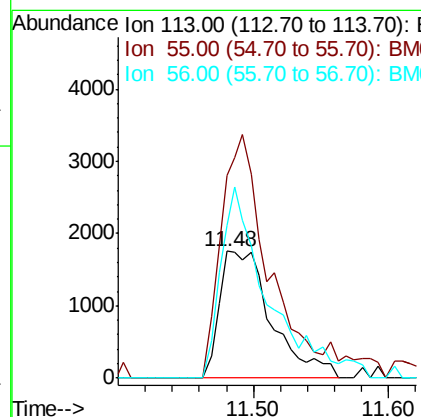







#35
 4-Chloro-3-methylphenol
 Concen: 4.388 ng/ul
 RT: 11.83 min Scan# 1520
 Delta R.T. 0.00 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
107	100		
144	25.1	22.4	33.6
142	78.8	66.0	99.0




Manual Integrations
 APPROVED


mohammad
 3/22/2021 2:48:48 PM

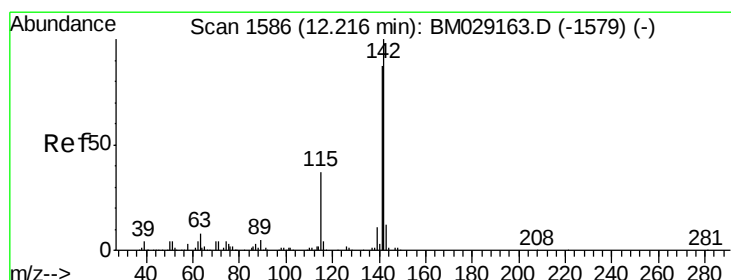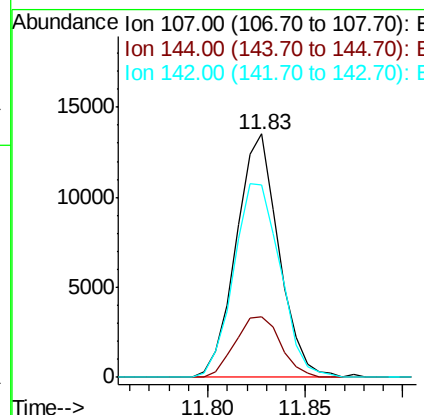

#36
 2-Methylnaphthalene
 Concen: 4.629 ng/ul
 RT: 12.22 min Scan# 1586
 Delta R.T. 0.00 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
142	100		
141	91.8	69.8	104.8

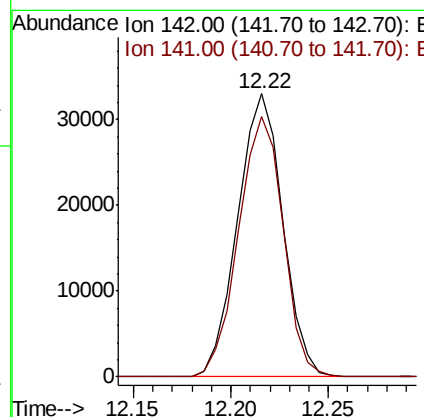







#37
1-Methylnaphthalene
Concen: 4.530 ng/ul
RT: 12.43 min Scan# 1623
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
142	100		
141	94.7	74.0	111.0
116	4.8	3.1	4.7




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

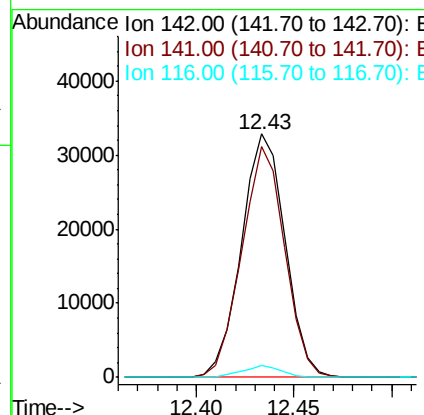

#39
1,2,4,5-Tetrachlorobenzene
Concen: 4.309 ng/ul
RT: 12.58 min Scan# 1648
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
216	100		
214	76.9	63.1	94.7
179	21.3	16.9	25.3
108	18.2	14.2	21.2

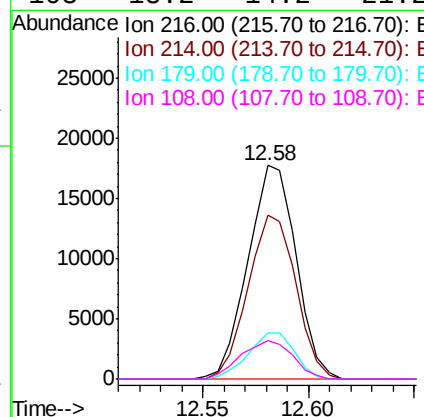

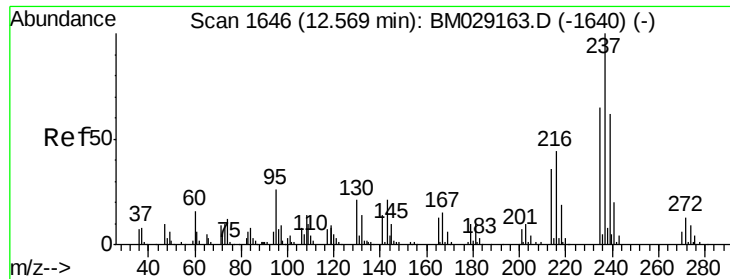





#40
Hexachlorocyclopentadiene
Concen: 3.690 ng/ul
RT: 12.57 min Scan# 1646
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
237	100		
235	59.6	52.2	78.2
272	11.6	11.0	16.6




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

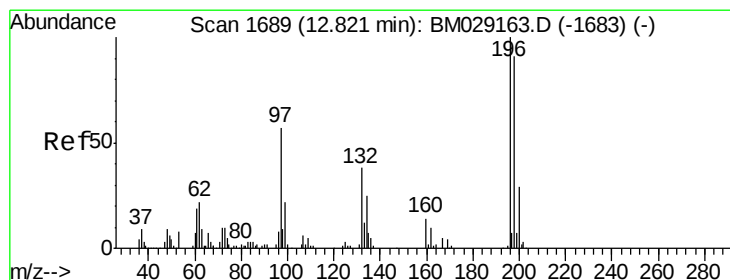

#41
2,4,6-Trichlorophenol
Concen: 4.132 ng/ul
RT: 12.82 min Scan# 1689
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
196	100		
198	101.2	73.2	109.8
200	30.5	23.1	34.7









#42
 2,4,5-Trichlorophenol
 Concen: 4.525 ng/ul
 RT: 12.89 min Scan# 1700
 Delta R.T. -0.01 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
196	100		
198	79.7	78.8	118.2
200	29.0	25.8	38.8




Manual Integrations
 APPROVED


mohammad
 3/22/2021 2:48:48 PM

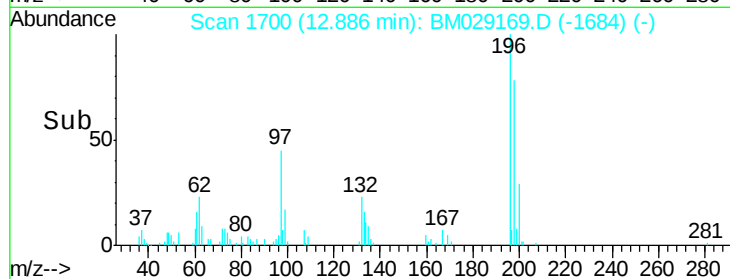

#43
 1,1'-Biphenyl
 Concen: 4.394 ng/ul
 RT: 13.23 min Scan# 1758
 Delta R.T. -0.01 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
154	100		
153	40.6	31.9	47.9
76	15.8	9.4	14.0

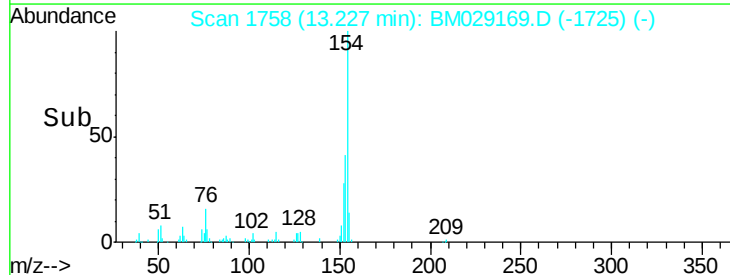







#44
2-Chloronaphthalene
Concen: 4.301 ng/ul
RT: 13.27 min Scan# 1765
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion:	162	Resp:	51985
Ion Ratio	Lower	Upper	
162	100		
164	33.3	25.9	38.9
127	36.9	29.5	44.3




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM



#45
2-Nitroaniline
Concen: 4.200 ng/ul
RT: 13.47 min Scan# 1799
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion:	65	Resp:	10890
Ion Ratio	Lower	Upper	
65	100		
92	66.4	51.2	76.8
138	91.9	77.0	115.4

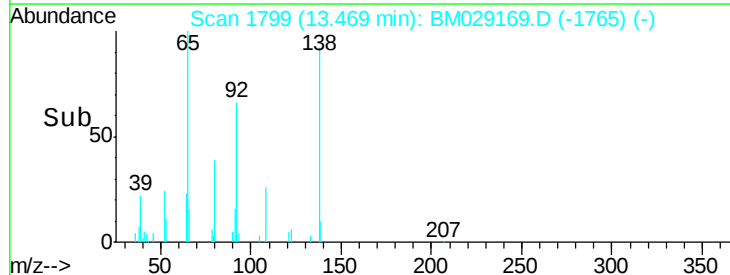







#47
Dimethylphthalate
Concen: 4.560 ng/ul
RT: 13.86 min Scan# 1865
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
163	100		
194	4.1	2.9	4.3
164	8.4	7.4	11.2




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

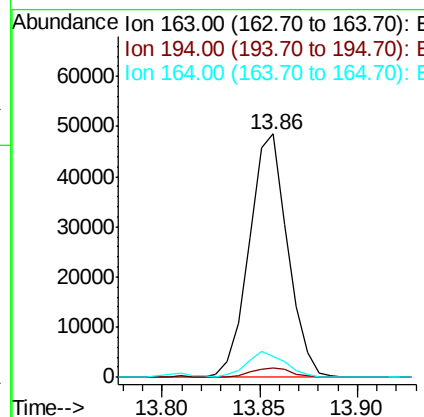

#48
2,6-Dinitrotoluene
Concen: 4.134 ng/ul
RT: 13.96 min Scan# 1883
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
165	100		
89	60.9	50.6	75.8
121	22.1	18.7	28.1

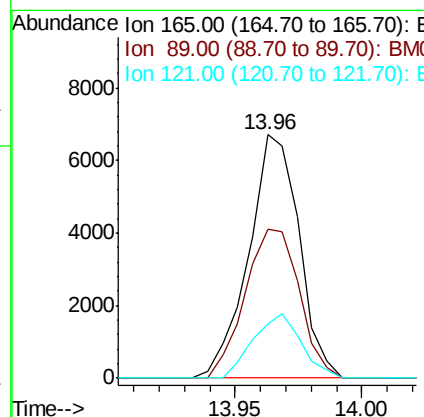



#50

Acenaphthylene

Concen: 4.600 ng/ul

RT: 14.12 min Scan# 1909

Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion:	152	Resp:	79779
Ion Ratio	Lower	Upper	
152	100		
151	20.6	16.2	24.2
153	14.2	10.6	16.0

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

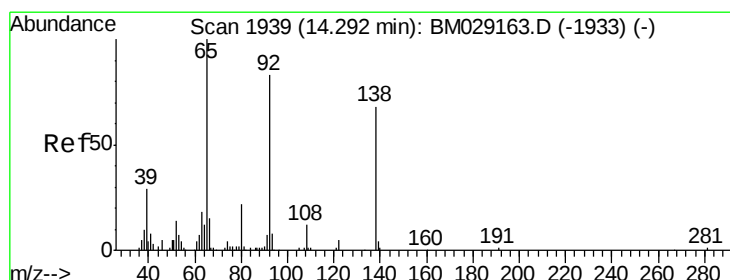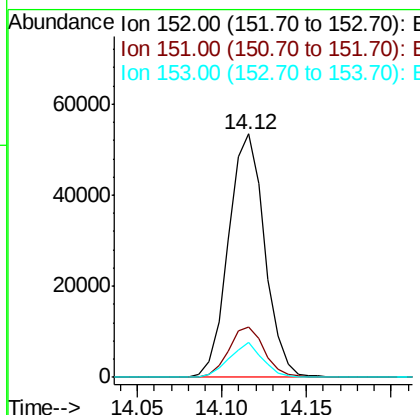

#51

3-Nitroaniline

Concen: 3.754 ng/ul




RT: 14.29 min Scan# 1939


Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Tgt Ion:	138	Resp:	9380
Ion Ratio	Lower	Upper	
138	100		
108	16.3	14.0	21.0
92	123.7	97.2	145.8





#52

Acenaphthene

Concen: 4.422 ng/ul

RT: 14.46 min Scan# 1967

Delta R.T. -0.01 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion:153	Resp:	56940
Ion Ratio	Lower	Upper
153	100	
152	48.8	38.1 57.1
154	85.8	67.0 100.6

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

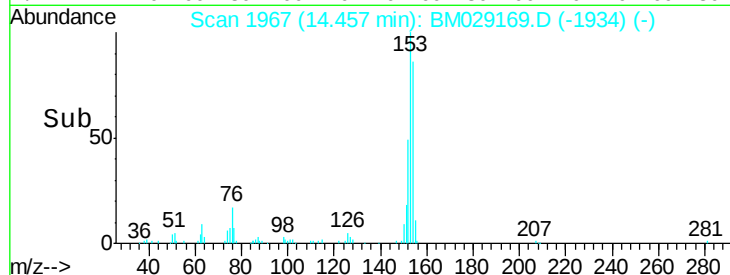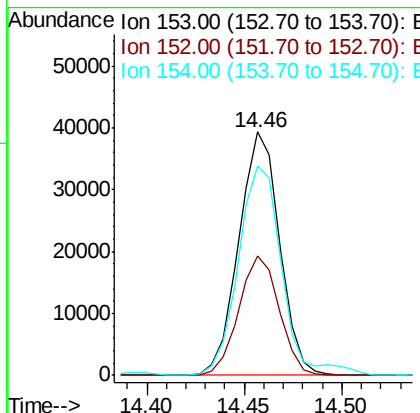

#53

2,4-Dinitrophenol

Concen: 3.284 ng/ul




RT: 14.50 min Scan# 1974


Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Tgt Ion:184	Resp:	3981
Ion Ratio	Lower	Upper
184	100	
63	67.1	49.3 73.9
154	50.6	48.3 72.5





#55

4-Nitrophenol

Concen: 4.314 ng/ul

RT: 14.59 min Scan# 1989

Delta R.T. -0.01 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M


ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
109	100		
139	113.0	94.2	141.4
65	172.9	105.9	158.9#

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM






Abundance

Ion 109.00 (108.70 to 109.70): E

Ion 139.00 (138.70 to 139.70): E

Ion 65.00 (64.70 to 65.70): BM

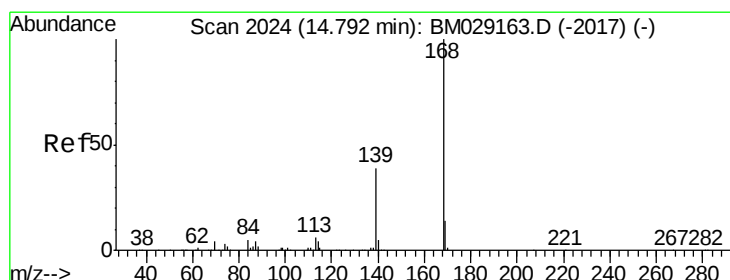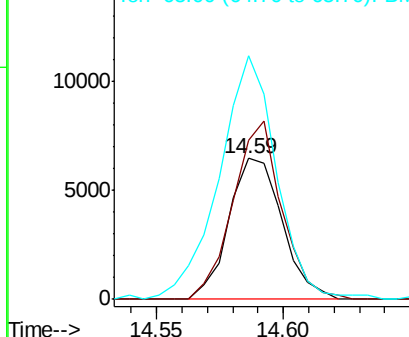

#56

Dibenzofuran

Concen: 4.576 ng/ul


RT: 14.79 min Scan# 2024

Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14



Tgt Ion	Ratio	Lower	Upper
168	100		
139	38.7	31.0	46.6




Abundance

Ion 168.00 (167.70 to 168.70): E

Ion 139.00 (138.70 to 139.70): E

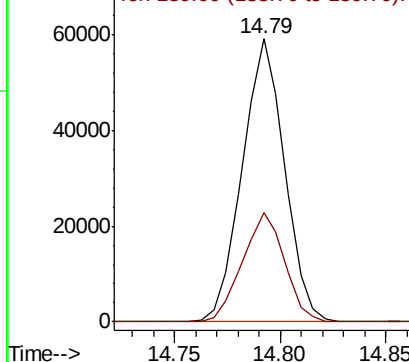







#57
2,4-Dinitrotoluene
Concen: 4.228 ng/ul
RT: 14.75 min Scan# 2017
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
165	100		
63	55.0	41.0	61.4
182	2.7	2.6	3.8




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

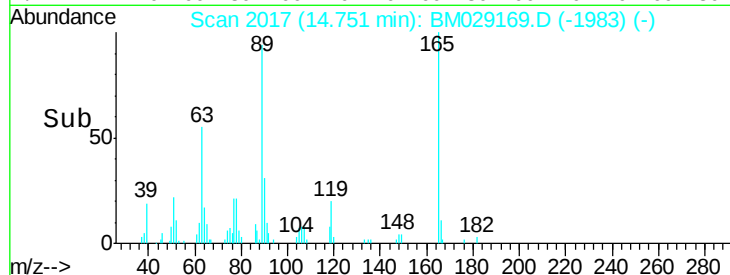

#58
2,3,4,6-Tetrachlorophenol
Concen: 4.076 ng/ul
RT: 15.02 min Scan# 2062
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
232	100		
131	51.4	35.6	53.4
130	2.0	2.7	4.1#
166	33.2	24.6	37.0

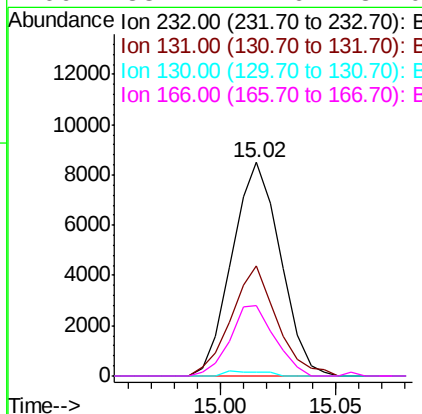







#59
Diethylphthalate
Concen: 4.493 ng/ul
RT: 15.22 min Scan# 2097
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
149	100		
177	22.7	17.2	25.8
150	11.4	10.2	15.4




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

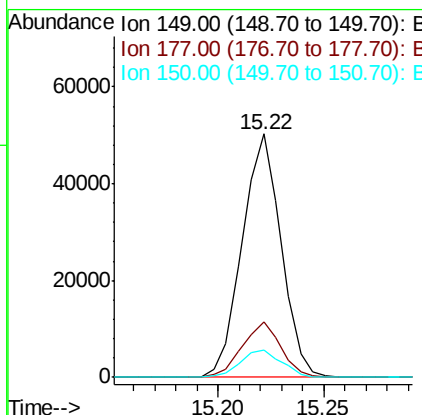

#61
Fluorene
Concen: 4.547 ng/ul
RT: 15.44 min Scan# 2134
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
166	100		
165	96.7	77.2	115.8
167	12.7	10.7	16.1









#62
4-Chlorophenyl-phenylether
Concen: 4.420 ng/ul
RT: 15.44 min Scan# 2134
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
204	100		
206	31.1	25.4	38.0
141	67.5	48.6	73.0




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

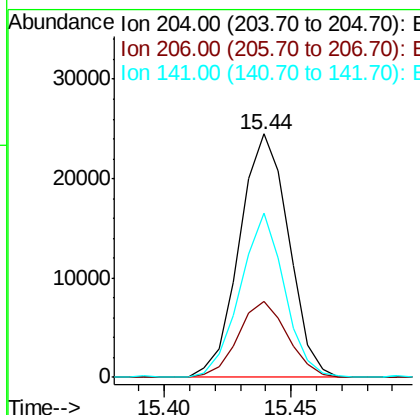

#63
4-Nitroaniline
Concen: 3.904 ng/ul
RT: 15.44 min Scan# 2135
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
138	100		
92	50.4	43.4	65.0
108	83.8	73.1	109.7









#66
 4,6-Dinitro-2-methylphenol
 Concen: 3.838 ng/ul
 RT: 15.51 min Scan# 2146
 Delta R.T. 0.00 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
198	100		
182	7.2	3.7	5.5#
77	37.7	23.0	34.4#




Manual Integrations
 APPROVED


mohammad
 3/22/2021 2:48:48 PM



#67
 N-Nitrosodiphenylamine
 Concen: 4.187 ng/ul
 RT: 15.65 min Scan# 2170
 Delta R.T. 0.00 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
169	100		
168	72.1	53.9	80.9
167	37.1	28.3	42.5









#68
4-Bromophenyl-phenylether
Concen: 4.219 ng/ul
RT: 16.33 min Scan# 2285
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
248	100		
250	96.3	75.2	112.8
141	84.0	59.0	88.6




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

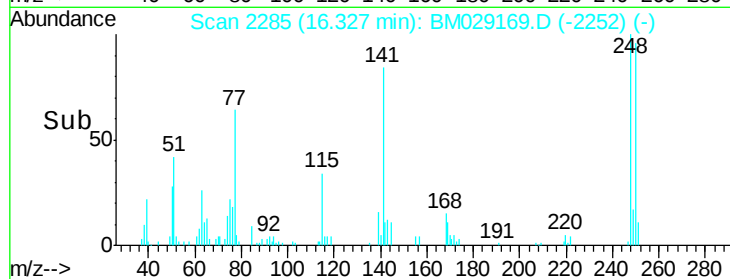

#69
Hexachlorobenzene
Concen: 4.482 ng/ul
RT: 16.44 min Scan# 2304
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
284	100		
142	39.2	30.9	46.3
249	31.7	27.1	40.7









#70
Atrazine
Concen: 3.746 ng/ul
RT: 16.60 min Scan# 2331
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion:	200	Resp:	19064
Ion Ratio	Lower	Upper	
200	100		
173	22.8	19.2	28.8
215	49.6	37.5	56.3




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM



#71
Pentachlorophenol
Concen: 3.237 ng/ul
RT: 16.77 min Scan# 2361
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion:	266	Resp:	9062
Ion Ratio	Lower	Upper	
266	100		
264	55.6	49.2	73.8
268	60.1	47.7	71.5





#72

Phenanthrene

Concen: 4.526 ng/ul

RT: 17.17 min Scan# 2428

Delta R.T. -0.01 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion:178	Resp:	111110
Ion Ratio	Lower	Upper
178	100	
179	15.6	12.1 18.1
176	18.6	15.0 22.4

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

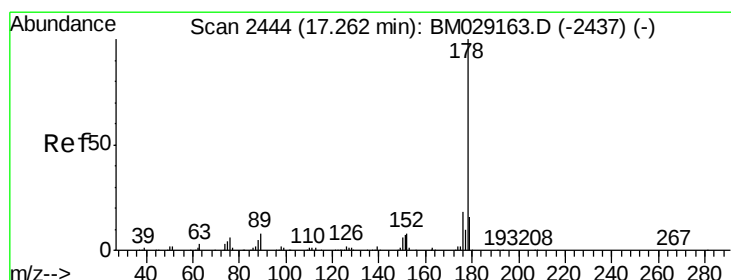

#74

Anthracene

Concen: 4.499 ng/ul




RT: 17.26 min Scan# 2444


Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Tgt Ion:178	Resp:	113498
Ion Ratio	Lower	Upper
178	100	
179	14.6	12.6 18.8
176	18.3	14.7 22.1





#75

1,2,3,4-Tetrachlorobenzene

Concen: 4.215 ng/uL

RT: 13.19 min Scan# 1752

Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion:	216	Resp:	28309
Ion Ratio	Lower	Upper	
216	100		
214	77.7	62.8	94.2
218	47.9	38.1	57.1

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

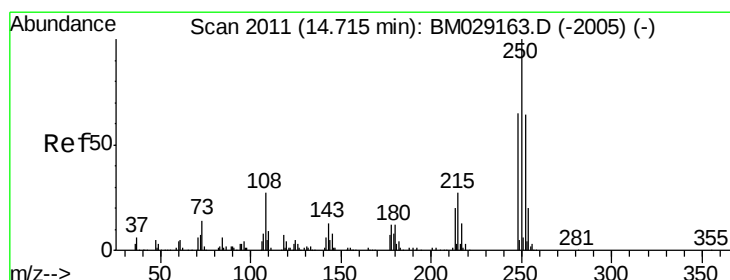

#76

Pentachlorobenzene

Concen: 3.868 ng/uL




RT: 14.71 min Scan# 2010


Delta R.T. -0.01 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Tgt Ion:	250	Resp:	25361
Ion Ratio	Lower	Upper	
250	100		
248	66.8	52.2	78.2
252	65.8	50.9	76.3









#77
 Carbazole
 Concen: 4.232 ng/ul
 RT: 17.53 min Scan# 2489
 Delta R.T. 0.00 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Instrument :
 BNA_M
 ClientSampleId :
 MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
167	100		
166	22.4	17.2	25.8
139	13.2	10.1	15.1




Manual Integrations
 APPROVED


mohammad
 3/22/2021 2:48:48 PM

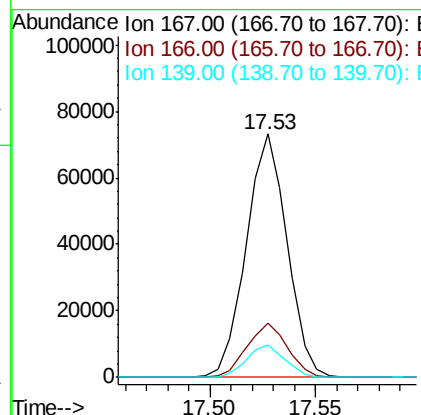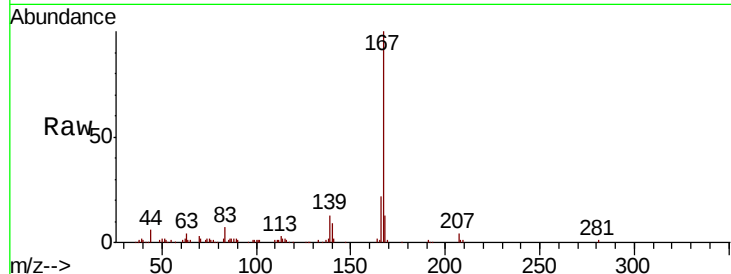

#78
 Di-n-butylphthalate
 Concen: 3.897 ng/ul
 RT: 18.10 min Scan# 2587
 Delta R.T. -0.01 min
 Lab File: BM029169.D
 Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
149	100		
150	9.9	7.1	10.7
104	6.2	4.6	7.0

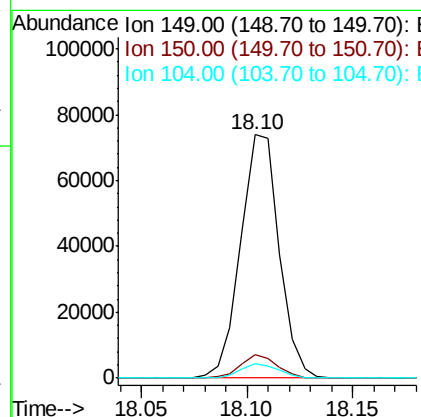







#80
Fluoranthene
Concen: 4.463 ng/ul
RT: 19.18 min Scan# 2770
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	8.7	7.5	11.3
100	7.4	5.8	8.8




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

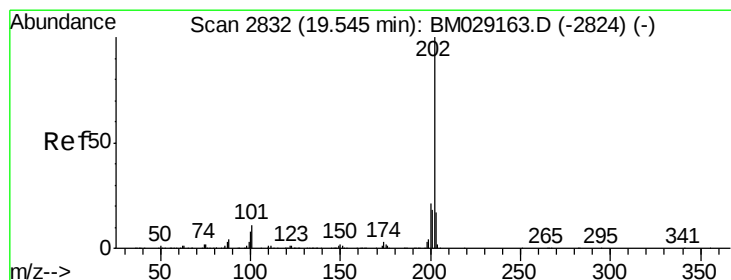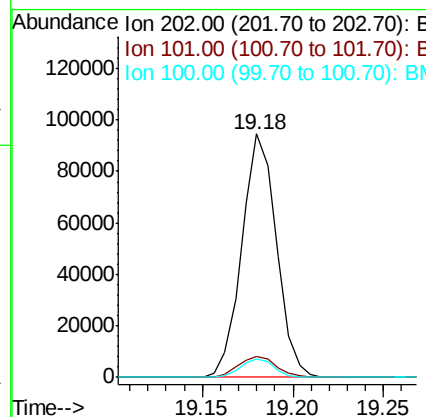

#82
Pyrene
Concen: 4.733 ng/ul
RT: 19.54 min Scan# 2832
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Resp Lower	Resp Upper
202	100		
101	11.1	8.9	13.3
100	10.2	6.8	10.2#

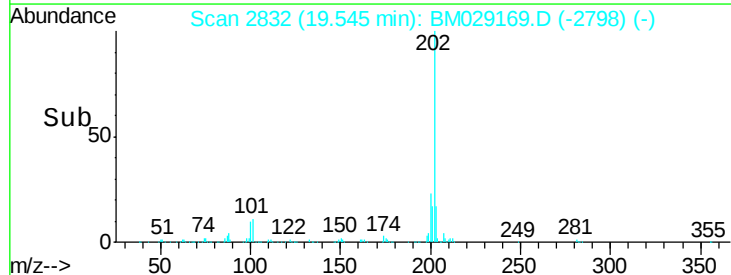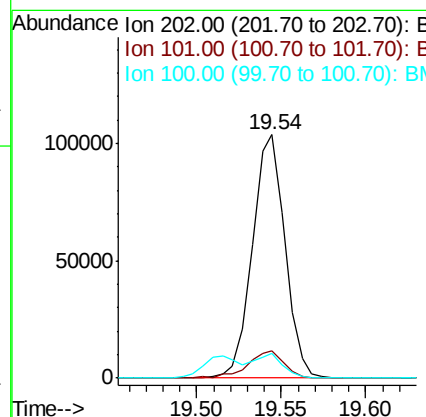







#83
Butylbenzylphthalate
Concen: 3.662 ng/ul
RT: 20.45 min Scan# 2986
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion:	149	Resp:	37997
Ion Ratio	Lower	Upper	
149	100		
91	75.5	61.8	92.6
206	19.8	16.0	24.0




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

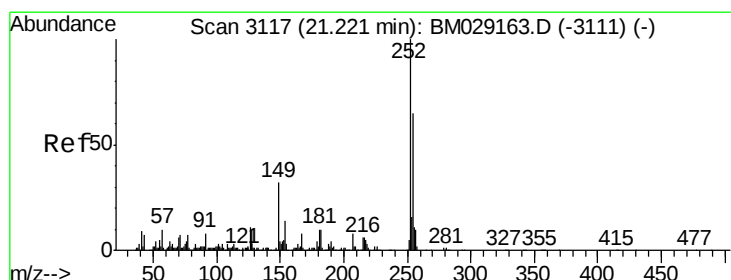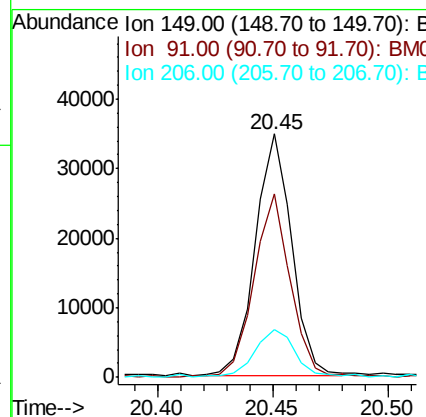

#84
3,3'-Dichlorobenzidine
Concen: 3.911 ng/ul
RT: 21.22 min Scan# 3116
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion:	252	Resp:	38058
Ion Ratio	Lower	Upper	
252	100		
254	60.5	52.1	78.1
126	9.2	8.6	13.0

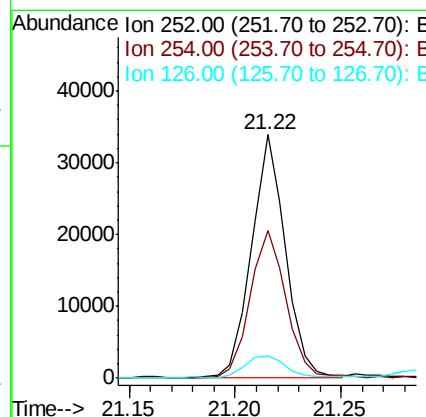

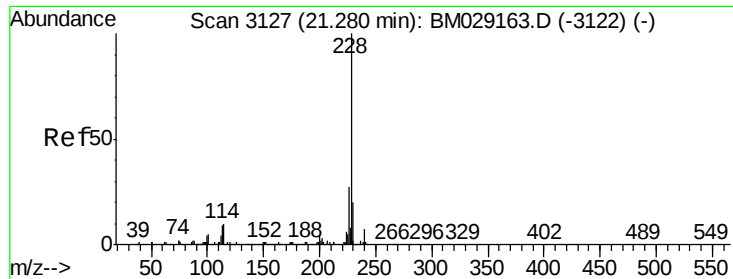

#85

Benzo(a)anthracene

Concen: 4.407 ng/ul

RT: 21.28 min Scan# 3127

Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion:	228	Resp:	133593
Ion Ratio	Lower	Upper	
228	100		
229	19.2	16.0	24.0
226	27.3	21.8	32.6

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

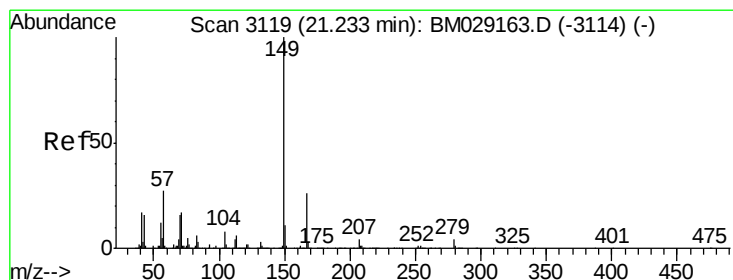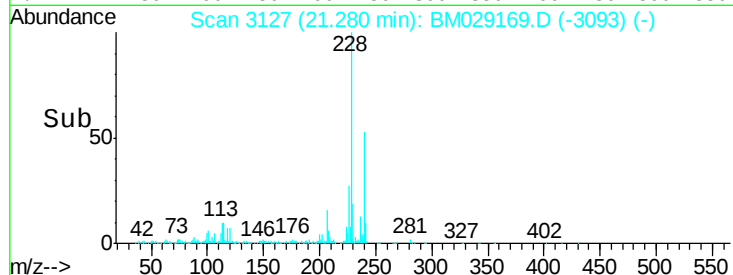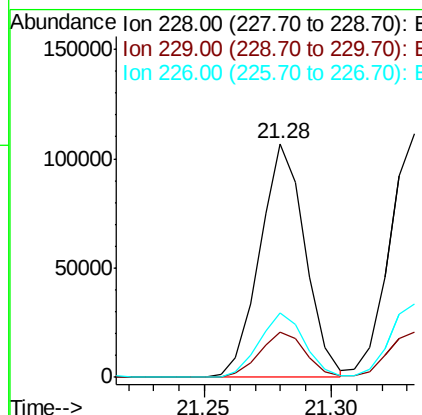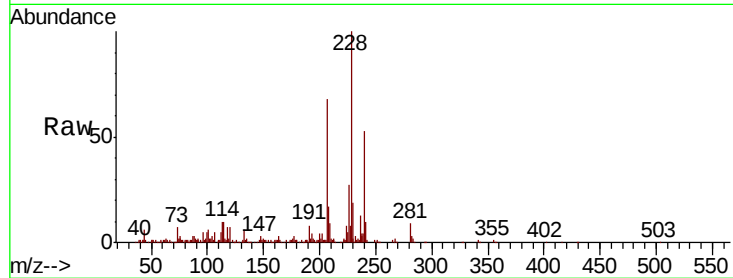

#86

Bis(2-ethylhexyl)phthalate

Concen: 3.479 ng/ul




RT: 21.23 min Scan# 3119


Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Tgt Ion:	149	Resp:	59331
Ion Ratio	Lower	Upper	
149	100		
167	25.8	20.7	31.1
279	4.3	3.4	5.0

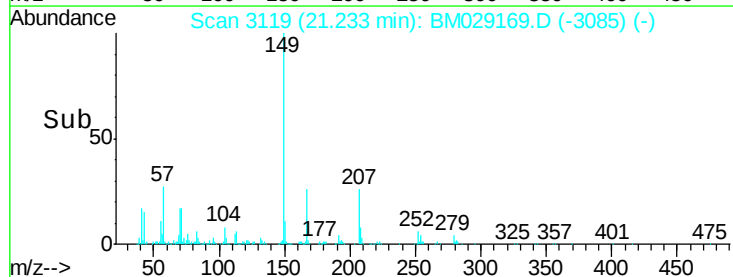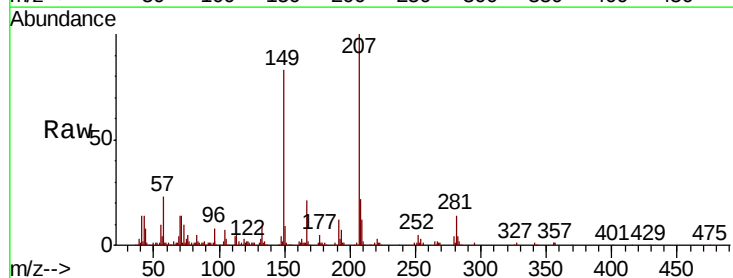







#87
Chrysene
Concen: 4.612 ng/ul
RT: 21.33 min Scan# 3136
Delta R.T. 0.00 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
228	100		
226	30.0	24.1	36.1
229	18.7	15.7	23.5




Manual Integrations
APPROVED


mohammad
3/22/2021 2:48:48 PM

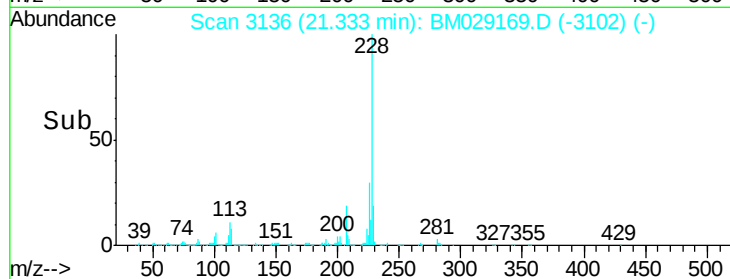

#89
Di-n-octyl phthalate
Concen: 3.078 ng/ul
RT: 22.11 min Scan# 3268
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion:149 Resp: 99707



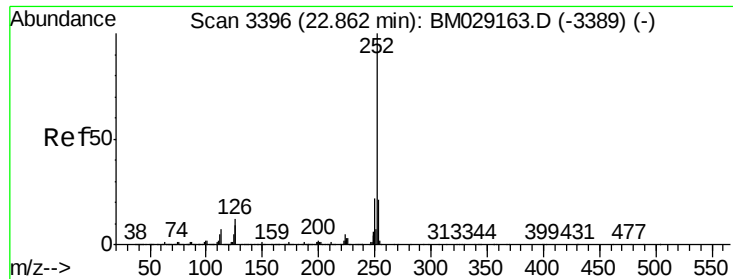

#90

Benzo(b)fluoranthene

Concen: 4.547 ng/ul

RT: 22.86 min Scan# 3396

Delta R.T. 0.00 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion:	252	Resp:	149227
Ion Ratio	Lower	Upper	
252	100		
253	21.1	16.8	25.2
125	9.6	7.4	11.0

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

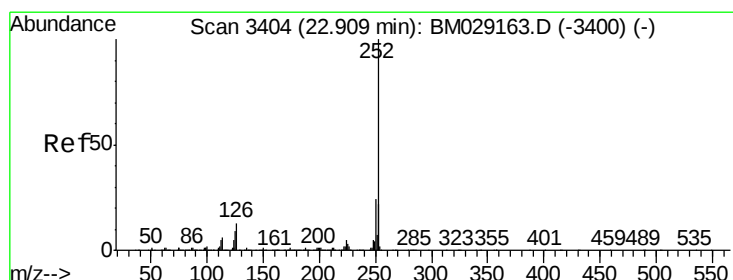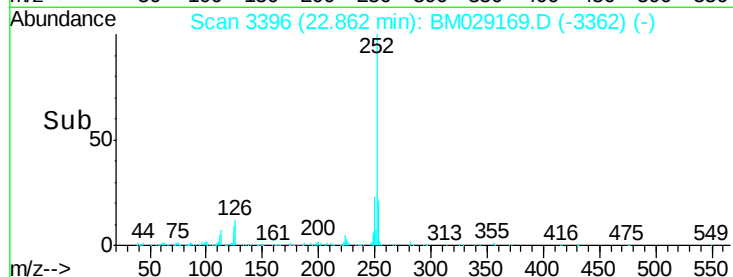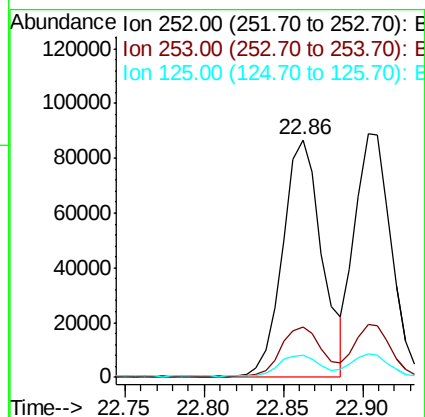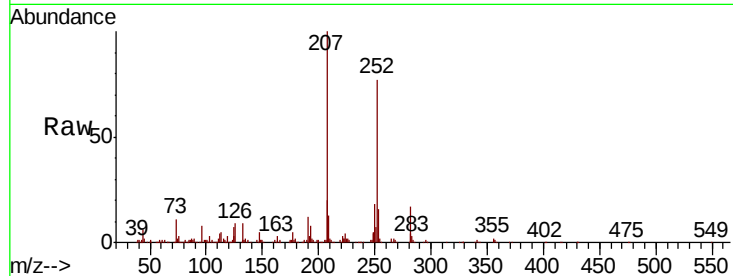

#91

Benzo(k)fluoranthene

Concen: 4.275 ng/ul




RT: 22.90 min Scan# 3403


Delta R.T. -0.01 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Tgt Ion:	252	Resp:	140193
Ion Ratio	Lower	Upper	
252	100		
253	21.8	17.6	26.4
125	9.6	7.5	11.3

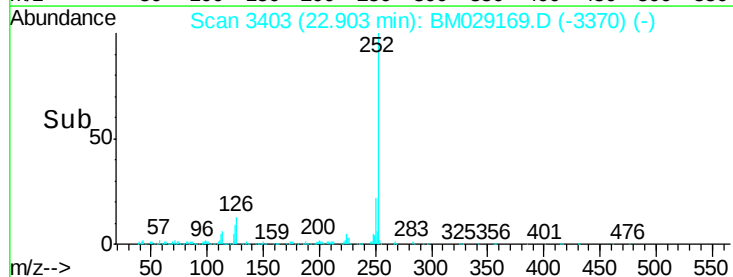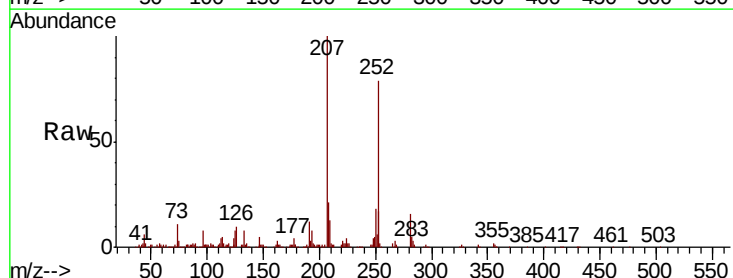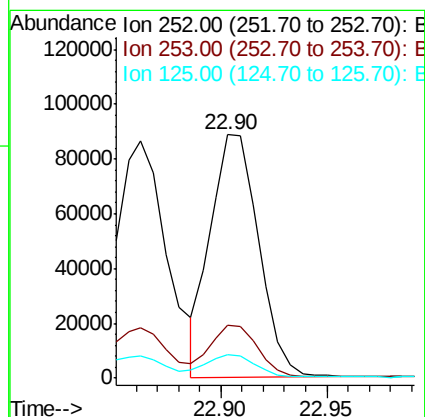



#93

Benzo(a)pyrene

Concen: 4.527 ng/ul

RT: 23.44 min Scan# 3494

Delta R.T. -0.01 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Instrument :

BNA_M





ClientSampleId :

MDL-WATER-QT2-2021-03

Tot Ion:	252	Resp:	134618
Ion Ratio	Lower	Upper	
252	100		
253	22.5	17.0	25.4
125	10.8	7.6	11.4

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

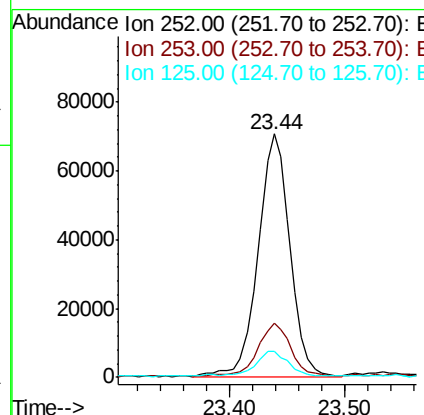

#94

Indeno(1,2,3-cd)pyrene

Concen: 4.339 ng/ul




RT: 25.80 min Scan# 3895


Delta R.T. -0.01 min

Lab File: BM029169.D

Acq: 19 Mar 2021 14:14

Tgt Ion:	276	Resp:	173518
Ion Ratio	Lower	Upper	
276	100		
138	22.5	19.2	28.8
277	24.6	20.3	30.5

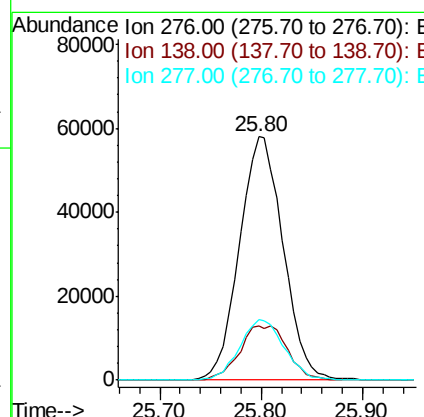







#95
Dibenzo(a,h)anthracene
Concen: 4.281 ng/ul
RT: 25.81 min Scan# 3898
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Instrument :
BNA_M
ClientSampleId :
MDL-WATER-QT2-2021-03

Tot Ion	Ratio	Lower	Upper
278	100		
139	15.7	12.7	19.1
279	23.7	19.3	28.9

Manual Integrations
APPROVED

mohammad
3/22/2021 2:48:48 PM

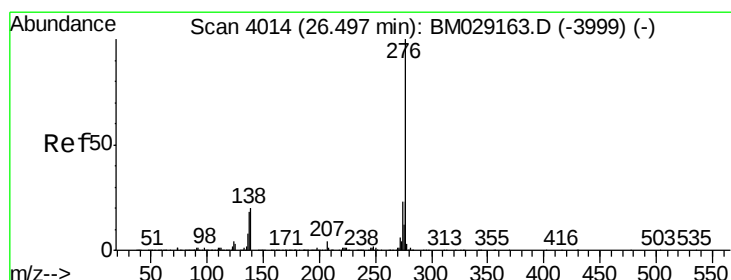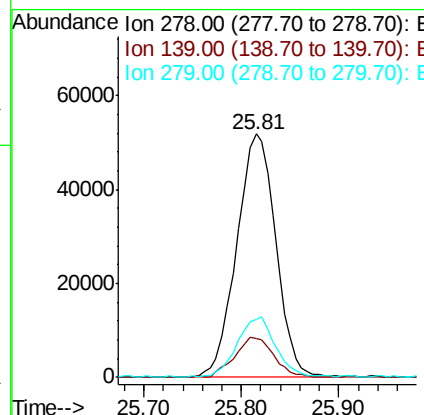

#96
Benzo(g,h,i)perylene
Concen: 4.390 ng/ul
RT: 26.49 min Scan# 4013
Delta R.T. -0.01 min
Lab File: BM029169.D
Acq: 19 Mar 2021 14:14

Tgt Ion	Ratio	Lower	Upper
276	100		
138	21.4	16.4	24.6
277	22.8	18.6	27.8

