

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
 Data File : BM044659.D
 Acq On : 19 Mar 2024 11:57
 Operator : MA/JU
 Sample : PB159639BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK639

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044659.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	25	28	42	rVB	60450	89141	2.71%	0.226%
2	3.652	93	96	115	rBV	685212	1090478	33.21%	2.766%
3	3.958	145	148	155	rVB2	14202	20260	0.62%	0.051%
4	6.869	636	643	656	rVV	745797	1245319	37.92%	3.158%
5	7.046	667	673	685	rBV	665384	1051495	32.02%	2.667%
6	7.228	697	704	716	rBV	783358	1242194	37.83%	3.150%
7	7.310	716	718	720	rVV3	4413	3549	0.11%	0.009%
8	7.693	776	783	792	rBV	669857	1080093	32.89%	2.739%
9	8.398	896	903	917	rBV	872222	1450780	44.18%	3.679%
10	8.851	973	980	992	rBV	686774	1184594	36.07%	3.004%
11	9.210	1039	1041	1046	rBV6	1825	3320	0.10%	0.008%
12	9.569	1094	1102	1117	rVV	566616	960663	29.26%	2.436%
13	10.098	1185	1192	1219	rBV	794228	1399996	42.63%	3.551%
14	10.475	1248	1256	1264	rBV	904996	1491364	45.42%	3.782%
15	10.622	1274	1281	1298	rBV	781026	1481727	45.12%	3.758%
16	12.092	1526	1531	1537	rBV6	9606	19355	0.59%	0.049%
17	12.386	1577	1581	1584	rBV5	2873	3872	0.12%	0.010%
18	13.239	1721	1726	1733	rVB4	11242	17817	0.54%	0.045%
19	13.763	1807	1815	1824	rBV	1294864	1869444	56.93%	4.741%
20	14.033	1854	1861	1870	rBV	1580904	2315172	70.50%	5.872%
21	14.339	1906	1913	1925	rBV	1237296	1793561	54.62%	4.549%
22	14.551	1942	1949	1972	rBV	388819	838307	25.53%	2.126%
23	15.339	2076	2083	2093	rBV	1962215	2796597	85.17%	7.093%
24	15.469	2099	2105	2119	rBV	554628	822544	25.05%	2.086%
25	15.580	2121	2124	2129	rVB4	8079	10579	0.32%	0.027%
26	16.127	2213	2217	2221	rVB4	5087	6859	0.21%	0.017%
27	17.092	2375	2381	2391	rBV	1318350	1899266	57.84%	4.817%
28	17.192	2392	2398	2416	rVB2	1926822	2821476	85.92%	7.156%
29	18.021	2535	2539	2540	rBV3	2732	3450	0.11%	0.009%
30	19.062	2711	2716	2721	rBV3	20965	28155	0.86%	0.071%
31	19.133	2724	2728	2734	rVV3	15224	23013	0.70%	0.058%
32	19.392	2770	2772	2775	rBV4	3236	4546	0.14%	0.012%
33	19.498	2783	2790	2800	rBV	2219323	3071441	93.54%	7.790%
34	21.292	3090	3095	3107	rBV	1395185	1867147	56.86%	4.735%
35	23.397	3446	3453	3461	rBV2	1730826	3283710	100.00%	8.328%
36	23.539	3470	3477	3486	rBV	1092122	2138954	65.14%	5.425%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044659.D
Acq On : 19 Mar 2024 11:57
Operator : MA/JU
Sample : PB159639BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK639

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION


Sum of corrected areas: 39430238

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044659.D
Acq On : 19 Mar 2024 11:57
Operator : MA/JU
Sample : PB159639BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

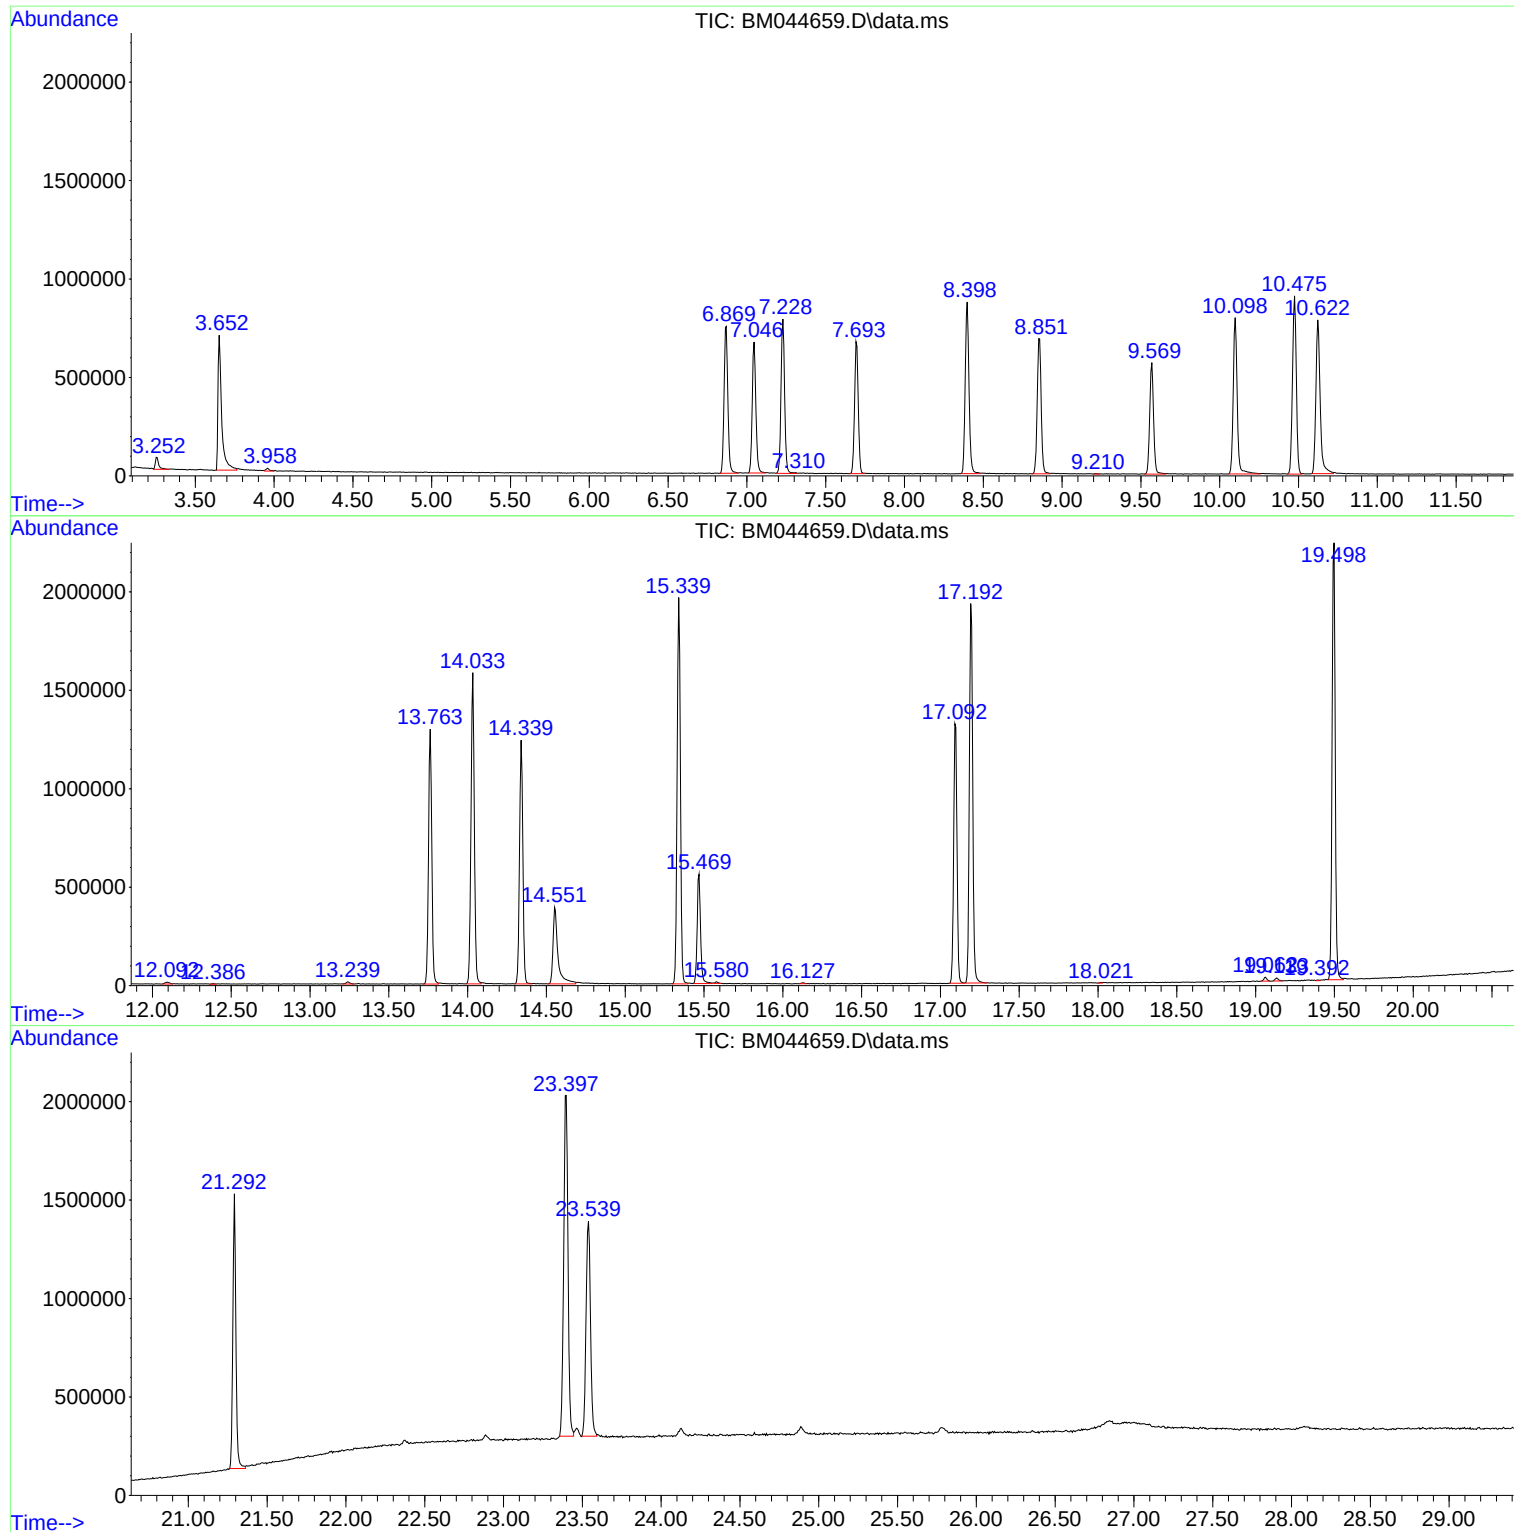

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044659.D
Acq On : 19 Mar 2024 11:57
Operator : MA/JU
Sample : PB159639BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044659.D
Acq On : 19 Mar 2024 11:57
Operator : MA/JU
Sample : PB159639BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK639

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------