

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044671.D
Acq On : 19 Mar 2024 19:23
Operator : MA/JU
Sample : PB159668BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

Signal : TIC: BM044671.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	39	rVB	60911	87249	2.51%	0.228%
2	3.652	92	96	116	rBV	681041	1083598	31.23%	2.834%
3	3.957	145	148	152	rVB	9905	12171	0.35%	0.032%
4	6.869	636	643	654	rBV	768322	1243506	35.84%	3.252%
5	7.046	666	673	686	rVB	654545	1032798	29.77%	2.701%
6	7.228	696	704	716	rBV	782234	1245403	35.90%	3.257%
7	7.693	776	783	791	rBV	596204	951922	27.44%	2.490%
8	8.398	894	903	918	rBV	882304	1468298	42.32%	3.840%
9	8.851	973	980	991	rBV	685074	1172112	33.79%	3.066%
10	9.569	1095	1102	1115	rBV	558567	957020	27.59%	2.503%
11	10.098	1184	1192	1203	rBV	797761	1380903	39.80%	3.612%
12	10.475	1248	1256	1264	rBV	761327	1294973	37.33%	3.387%
13	10.622	1272	1281	1295	rBV	789506	1462739	42.16%	3.826%
14	12.080	1525	1529	1535	rVV4	8720	18010	0.52%	0.047%
15	12.422	1582	1587	1588	rBV4	2344	4241	0.12%	0.011%
16	13.239	1719	1726	1733	rVV4	7782	14873	0.43%	0.039%
17	13.763	1808	1815	1828	rBV	1250762	1807440	52.10%	4.727%
18	14.033	1853	1861	1873	rBV	1500970	2264622	65.28%	5.923%
19	14.339	1906	1913	1924	rBV	1035823	1511868	43.58%	3.954%
20	14.551	1941	1949	1971	rBV	408981	869734	25.07%	2.275%
21	15.339	2076	2083	2092	rBV	1909786	2714505	78.24%	7.100%
22	15.469	2098	2105	2116	rBV	554974	808021	23.29%	2.113%
23	15.580	2121	2124	2129	rVB3	7742	9871	0.28%	0.026%
24	16.121	2214	2216	2221	rVB4	5217	5617	0.16%	0.015%
25	16.774	2324	2327	2332	rVB7	3153	4851	0.14%	0.013%
26	17.092	2375	2381	2391	rBV	1144658	1649030	47.53%	4.313%
27	17.192	2391	2398	2415	rVV2	1908203	2795983	80.59%	7.313%
28	18.015	2534	2538	2542	rVV7	4771	8941	0.26%	0.023%
29	18.227	2572	2574	2579	rBV6	2259	4110	0.12%	0.011%
30	18.798	2669	2671	2674	rBV4	2838	4079	0.12%	0.011%
31	19.057	2711	2715	2721	rBV3	20980	31765	0.92%	0.083%
32	19.133	2724	2728	2733	rVV	16746	22882	0.66%	0.060%
33	19.174	2733	2735	2738	rBV4	3841	5908	0.17%	0.015%
34	19.492	2783	2789	2798	rBV	2265791	3124092	90.05%	8.171%
35	21.292	3090	3095	3104	rBV	1321909	1723303	49.67%	4.507%
36	23.397	3446	3453	3460	rBV	1988966	3469324	100.00%	9.074%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044671.D
Acq On : 19 Mar 2024 19:23
Operator : MA/JU
Sample : PB159668BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	23.539	3471	3477	3490	rVB	1013696	1966816	56.69%	5.144%
----	--------	------	------	------	-----	---------	---------	--------	--------


Sum of corrected areas: 38232578

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044671.D
Acq On : 19 Mar 2024 19:23
Operator : MA/JU
Sample : PB159668BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

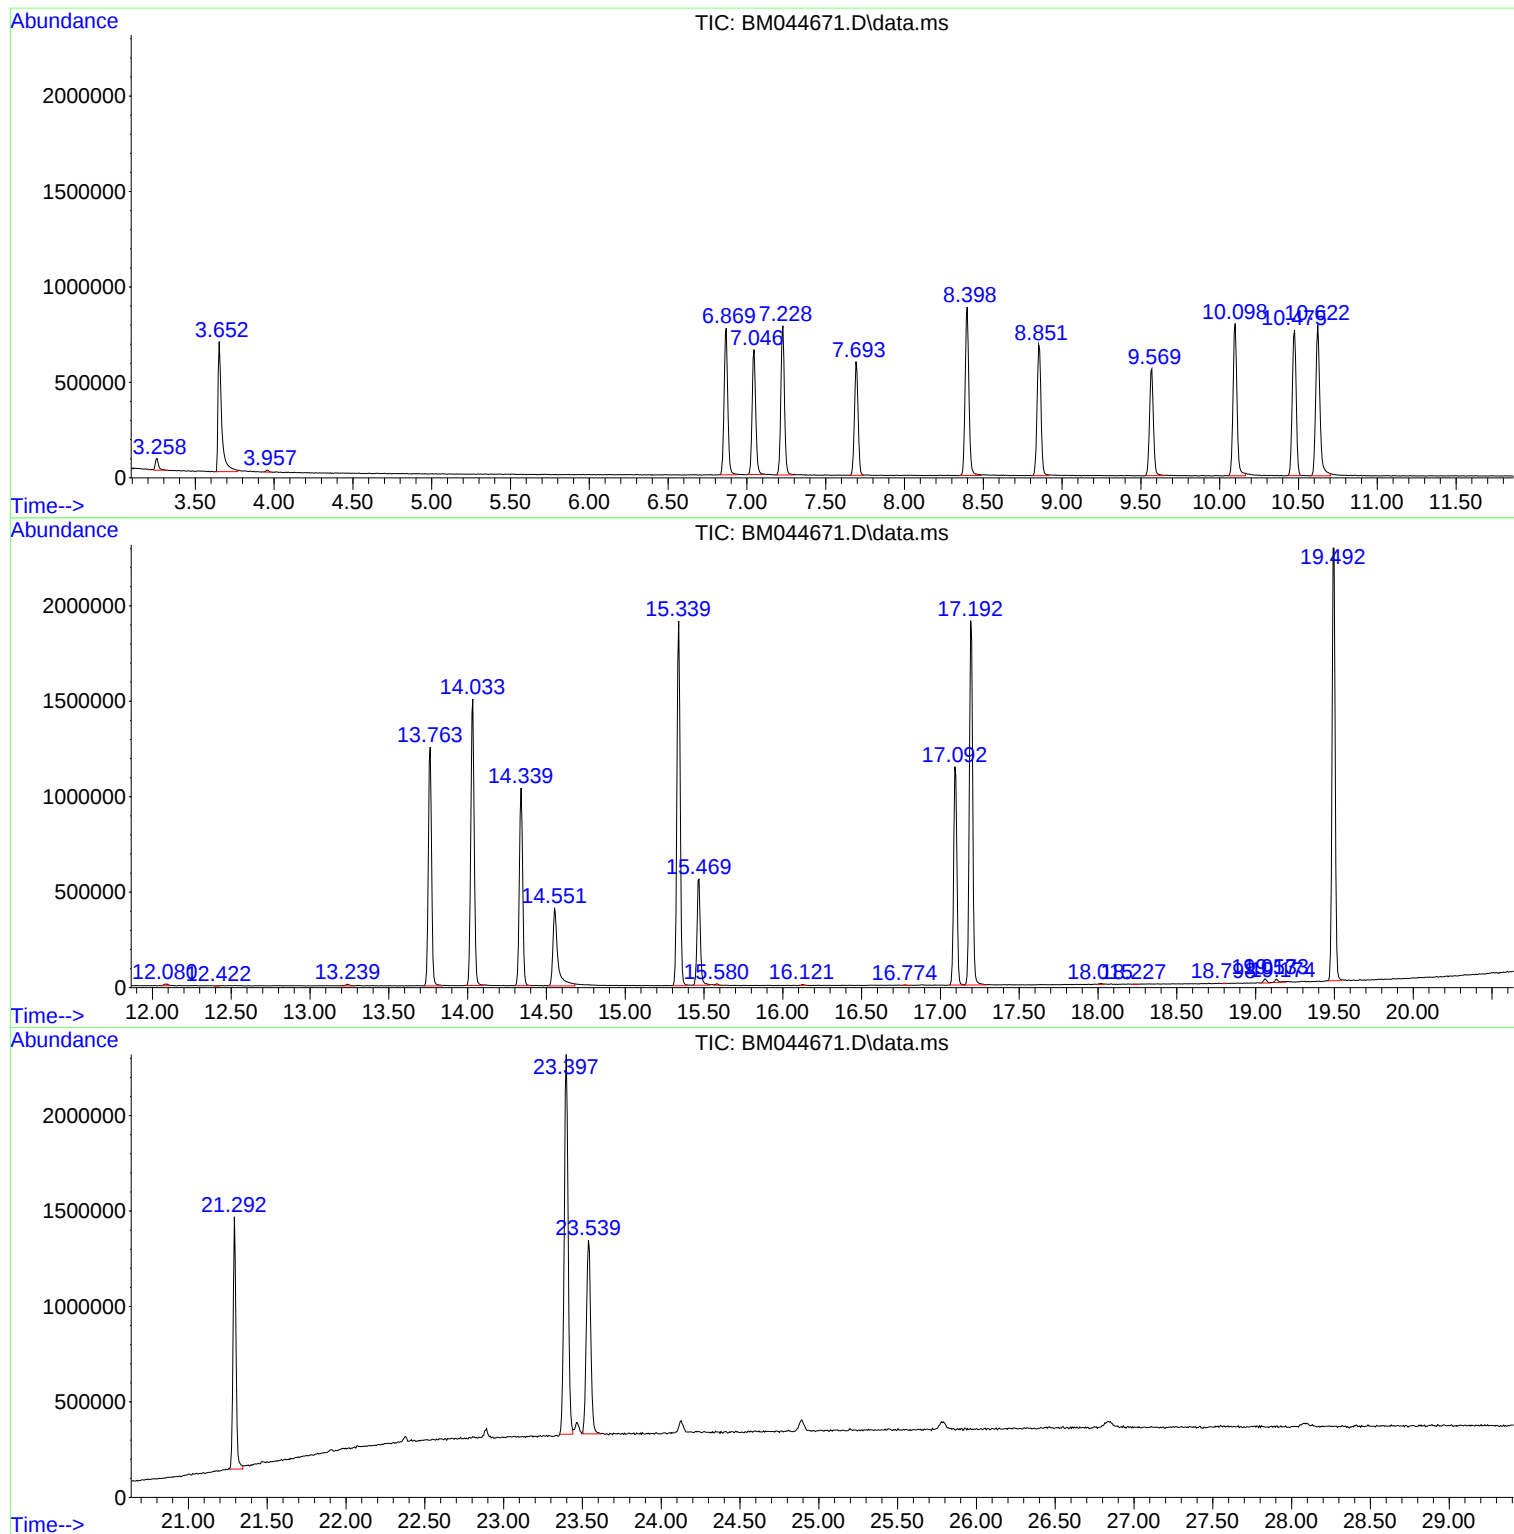

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044671.D
Acq On : 19 Mar 2024 19:23
Operator : MA/JU
Sample : PB159668BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044671.D
Acq On : 19 Mar 2024 19:23
Operator : MA/JU
Sample : PB159668BL
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK668

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------