

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
 Data File : BM044672.D
 Acq On : 19 Mar 2024 19:59
 Operator : MA/JU
 Sample : P1779-08
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0AK2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044672.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.222	17	23	41	rVB	4214597	6096413	100.00%	13.137%
2	3.663	95	98	114	rBV	139386	270388	4.44%	0.583%
3	3.963	145	149	152	rVB2	11275	15228	0.25%	0.033%
4	4.463	228	234	244	rVB	741320	1082446	17.76%	2.332%
5	5.098	338	342	349	rBV8	8233	12455	0.20%	0.027%
6	6.675	605	610	615	rBV7	3690	7841	0.13%	0.017%
7	6.869	636	643	654	rVB	188244	314014	5.15%	0.677%
8	7.045	666	673	688	rBV	780750	1268975	20.82%	2.734%
9	7.228	697	704	713	rBV	709451	1132099	18.57%	2.439%
10	7.304	715	717	721	rVV5	8599	10232	0.17%	0.022%
11	7.692	776	783	794	rBV	588092	934644	15.33%	2.014%
12	7.804	797	802	807	rVB	16721	29765	0.49%	0.064%
13	8.034	838	841	846	rVB7	4625	7404	0.12%	0.016%
14	8.398	896	903	915	rBV	502377	847711	13.91%	1.827%
15	8.851	972	980	995	rBV	845910	1427195	23.41%	3.075%
16	9.569	1094	1102	1112	rBV	655434	1092014	17.91%	2.353%
17	10.098	1183	1192	1209	rBV	857111	1508841	24.75%	3.251%
18	10.475	1249	1256	1263	rBV	743865	1265458	20.76%	2.727%
19	10.622	1273	1281	1299	rBV	780042	1422296	23.33%	3.065%
20	12.075	1522	1528	1535	rBV3	14636	27476	0.45%	0.059%
21	13.239	1720	1726	1733	rVB3	16648	26232	0.43%	0.057%
22	13.763	1808	1815	1826	rBV	1538354	2165909	35.53%	4.667%
23	14.033	1852	1861	1875	rBV	1817229	2758775	45.25%	5.945%
24	14.339	1906	1913	1922	rBV	1027491	1500720	24.62%	3.234%
25	14.563	1946	1951	1964	rBV2	61609	170737	2.80%	0.368%
26	15.151	2044	2051	2055	rBV	15745	23238	0.38%	0.050%
27	15.339	2076	2083	2098	rBV	2354458	3298274	54.10%	7.107%
28	15.463	2098	2104	2117	rVV	687092	1003486	16.46%	2.162%
29	15.586	2121	2125	2129	rVB6	9333	14936	0.24%	0.032%
30	16.127	2213	2217	2221	rVV5	5564	7990	0.13%	0.017%
31	16.874	2338	2344	2347	rBV7	5586	9068	0.15%	0.020%
32	17.092	2375	2381	2391	rBV	1093245	1605325	26.33%	3.459%
33	17.192	2391	2398	2411	rBV	2348277	3365665	55.21%	7.252%
34	17.398	2428	2433	2436	rBV6	4015	7362	0.12%	0.016%
35	17.768	2493	2496	2501	rBV6	4708	7428	0.12%	0.016%
36	18.004	2531	2536	2542	rBV2	44506	72262	1.19%	0.156%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044672.D
Acq On : 19 Mar 2024 19:59
Operator : MA/JU
Sample : P1779-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	19.056	2711	2715	2720	rBV3	25683	39058	0.64%	0.084%
38	19.133	2724	2728	2732	rVV	22470	26757	0.44%	0.058%
39	19.174	2732	2735	2738	rBV4	5386	8068	0.13%	0.017%
40	19.292	2751	2755	2762	rBV2	46540	66705	1.09%	0.144%
41	19.498	2783	2790	2797	rBV	2720948	3756960	61.63%	8.096%
42	20.739	2998	3001	3004	rBV4	23166	28887	0.47%	0.062%
43	21.292	3090	3095	3104	rBV	1299649	1665895	27.33%	3.590%
44	23.397	3446	3453	3460	rBV	2265047	4092618	67.13%	8.819%
45	23.538	3471	3477	3491	rVB	990463	1912584	31.37%	4.121%




Sum of corrected areas: 46407834

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044672.D
Acq On : 19 Mar 2024 19:59
Operator : MA/JU
Sample : P1779-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

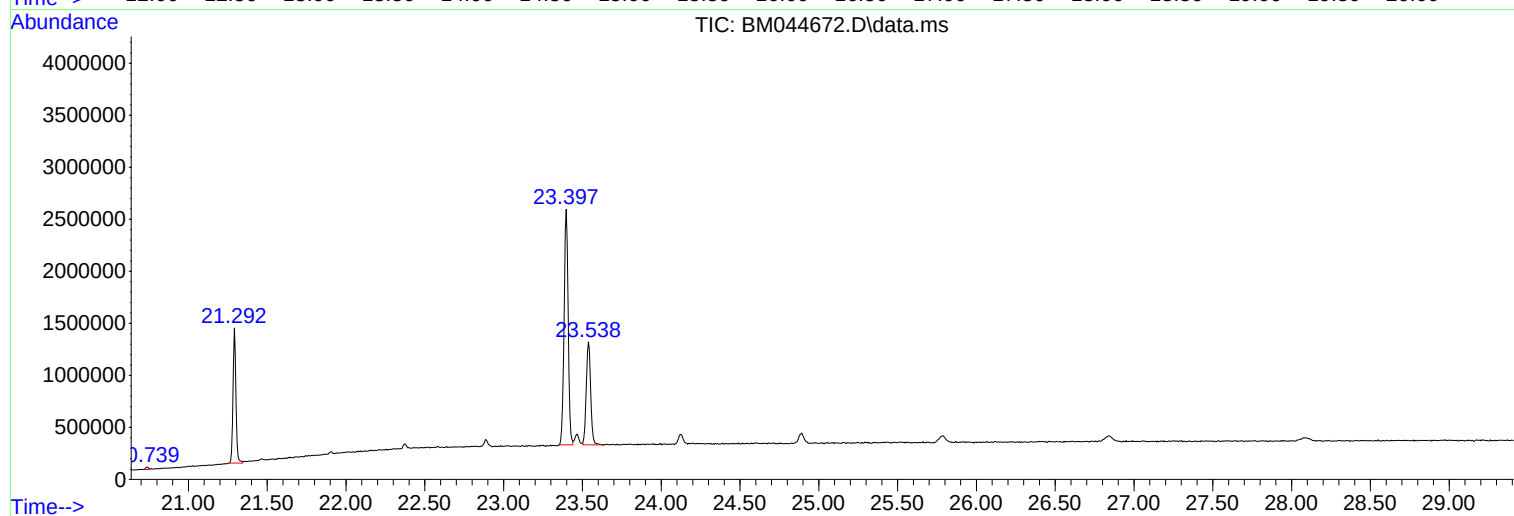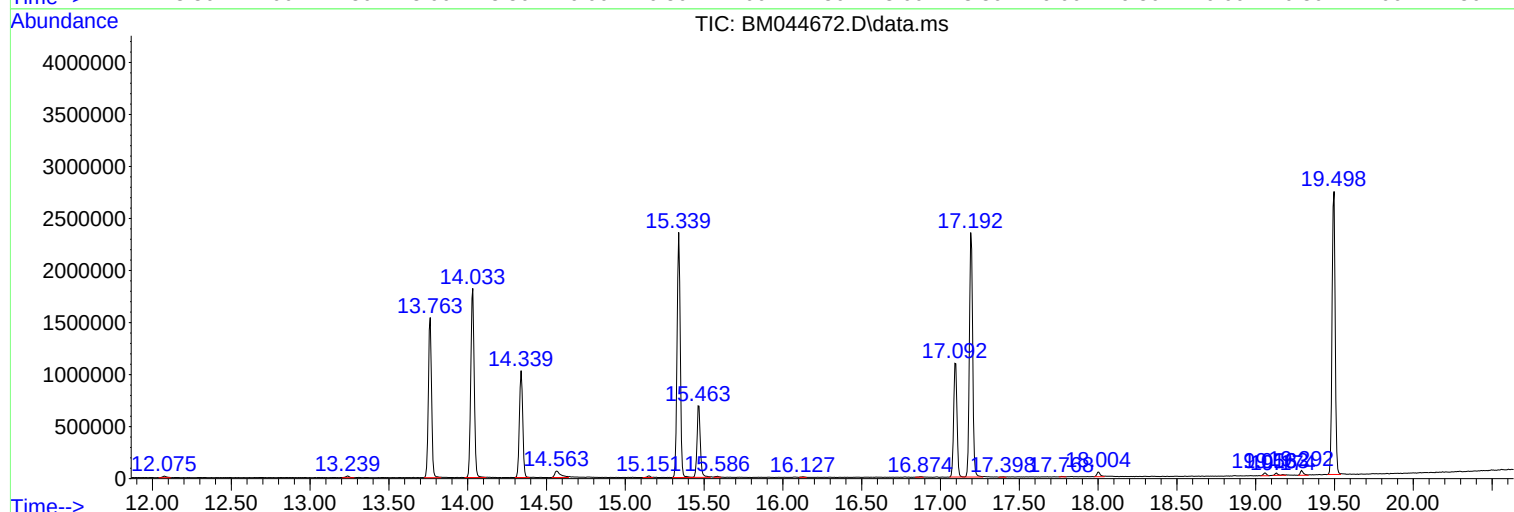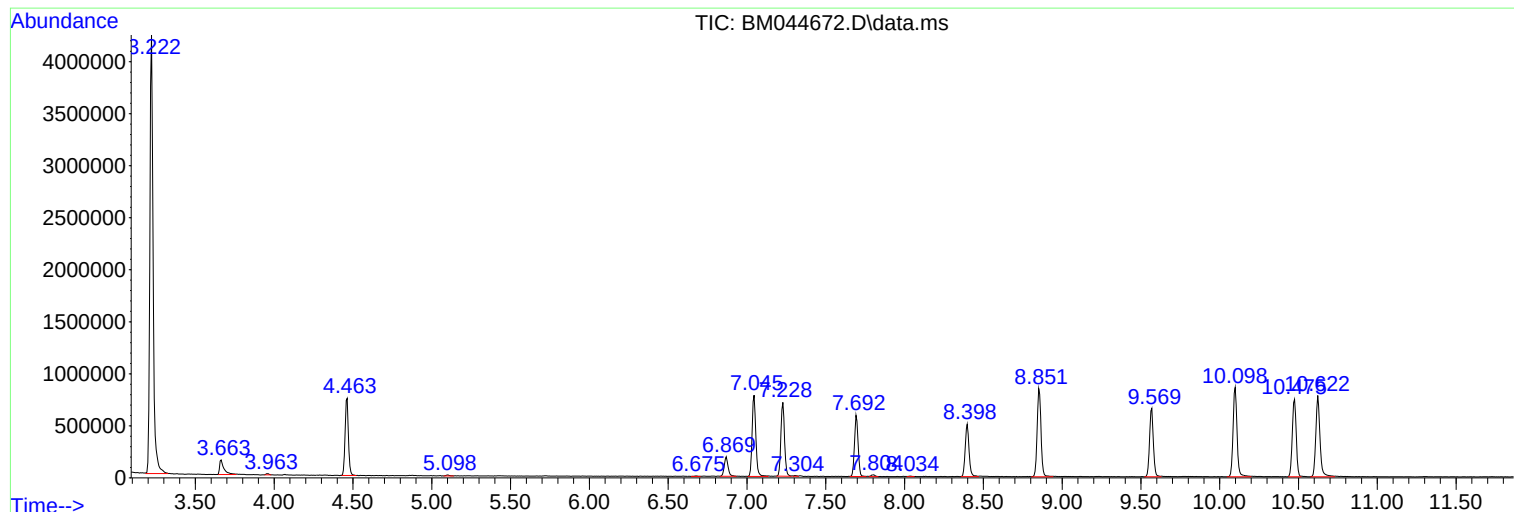

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044672.D
Acq On : 19 Mar 2024 19:59
Operator : MA/JU
Sample : P1779-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM031924\
Data File : BM044672.D
Acq On : 19 Mar 2024 19:59
Operator : MA/JU
Sample : P1779-08
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0AK2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc