


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032015\
Data File : BM000737.D
Acq On : 20 Mar 2015 11:09
Operator : TP/IZ
Sample : DFTPP41
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
DFTPP41

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM031915.M
Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
Last Update : Thu Mar 19 15:39:49 2015

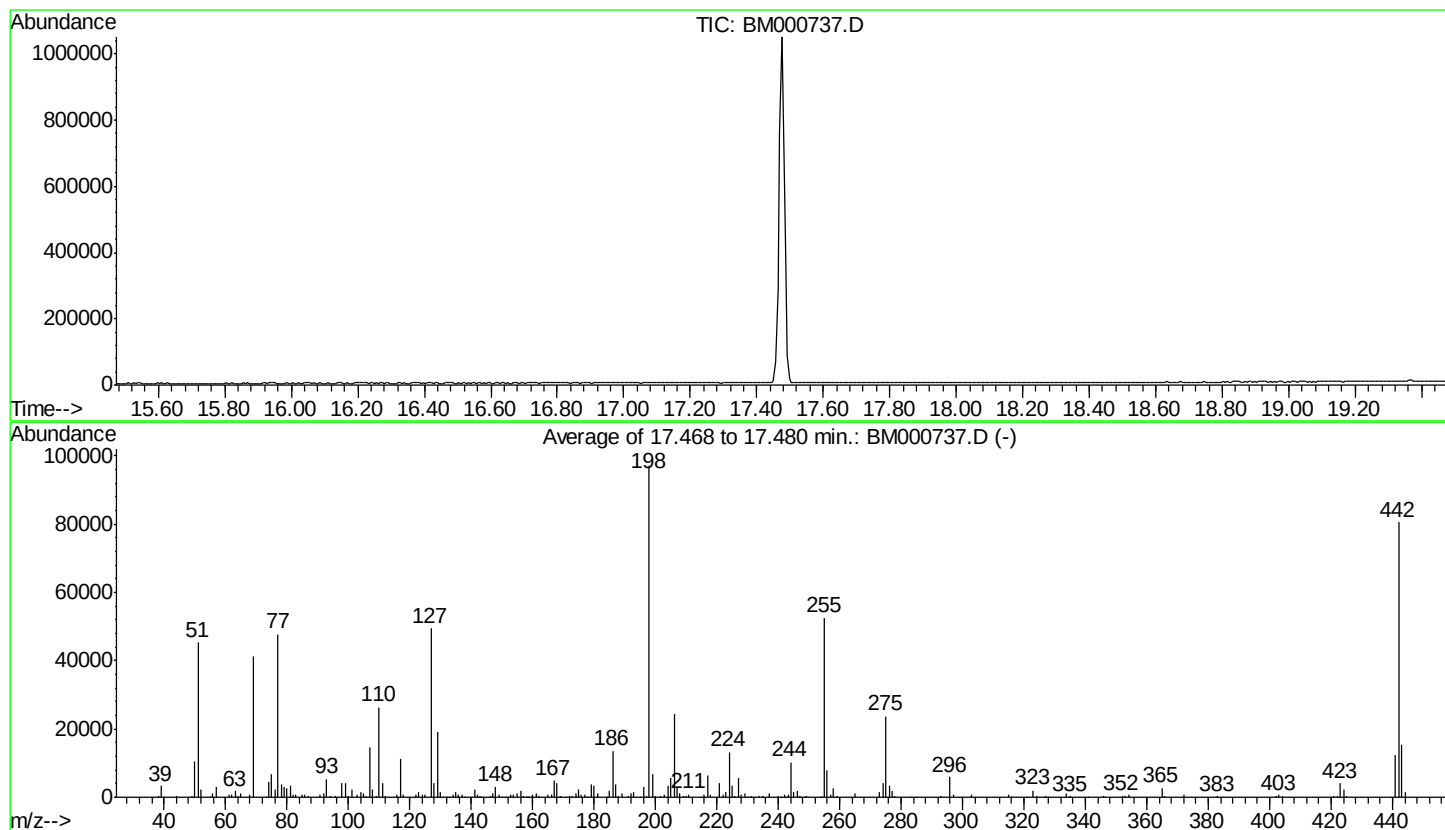

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	45208	PASS
68	69	0.00	2	2.0	811	PASS
69	198	0.00	100	42.6	41346	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	49349	PASS
197	198	0.00	2	0.5	526	PASS
198	198	100	100	100.0	97096	PASS
199	198	5	9	7.0	6758	PASS
275	198	10	60	24.3	23634	PASS
365	198	1	100	2.7	2640	PASS
441	443	0.01	100	80.9	12438	PASS
442	198	50	100	82.9	80520	PASS
443	442	15	24	19.1	15373	PASS