


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032015\
 Data File : BM000737.D
 Acq On : 20 Mar 2015 11:09
 Operator : TP/IZ
 Sample : DFTPP41
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP41

Integration File: RTEINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-SIM-BM031915.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Thu Mar 19 15:39:49 2015

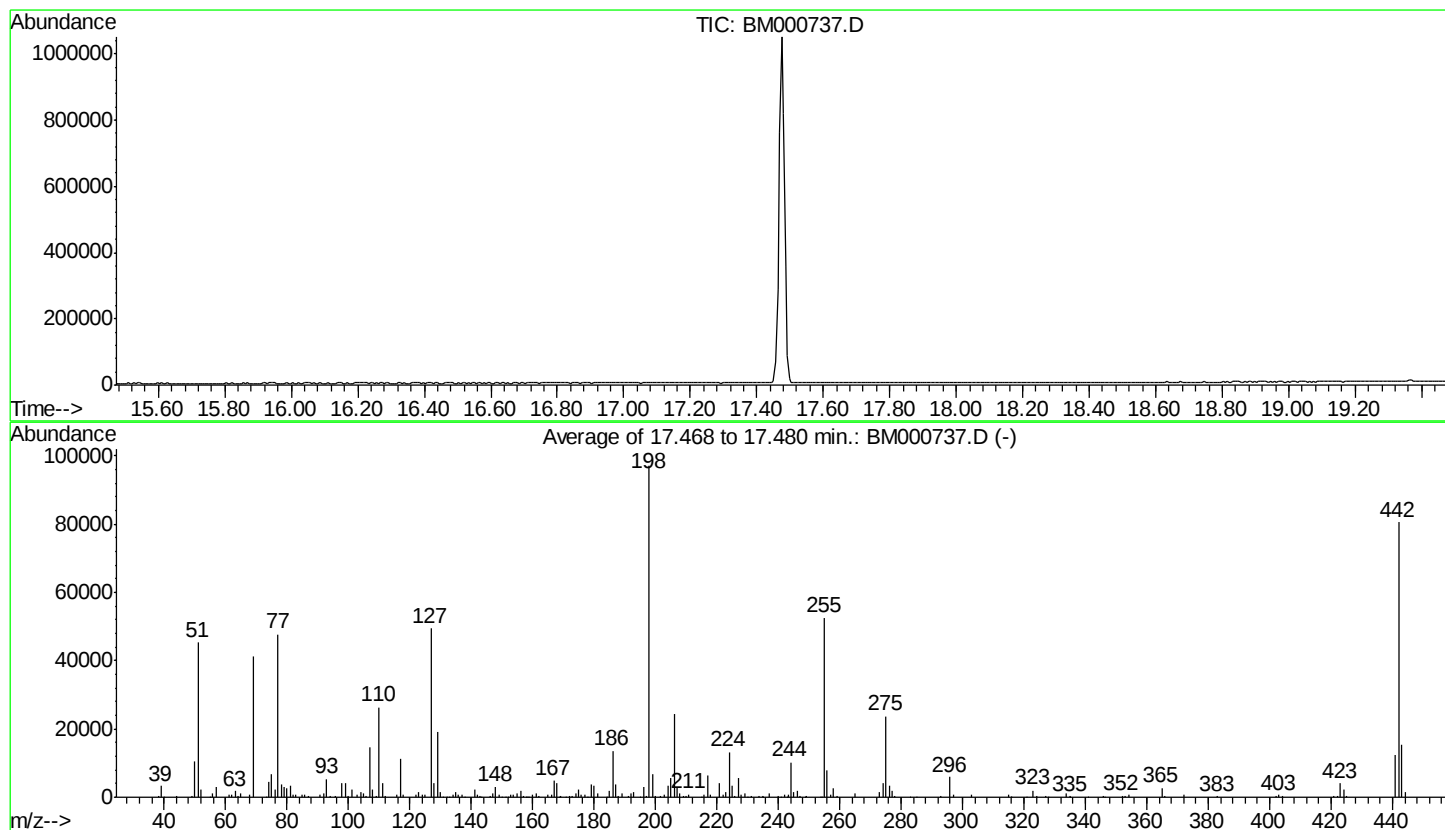

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.6	45208	PASS
68	69	0.00	2	2.0	811	PASS
69	198	0.00	100	42.6	41346	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	50.8	49349	PASS
197	198	0.00	2	0.5	526	PASS
198	198	100	100	100.0	97096	PASS
199	198	5	9	7.0	6758	PASS
275	198	10	60	24.3	23634	PASS
365	198	1	100	2.7	2640	PASS
441	443	0.01	100	80.9	12438	PASS
442	198	50	100	82.9	80520	PASS
443	442	15	24	19.1	15373	PASS

m/z	Abundance
38.10	610.0
39.00	3329.0
40.00	1312.0
44.00	4117.0
48.90	405.0
50.00	10833.0
51.10	46832.0
52.00	2704.0
56.00	909.0
57.00	3371.0
61.00	532.0
61.90	585.0
63.00	1587.0
64.00	338.0
65.10	839.0
67.90	754.0
69.00	41144.0
73.20	575.0
74.00	4467.0
75.00	6804.0
76.00	2358.0
77.10	47656.0
78.10	3712.0
79.00	3129.0
80.00	2533.0
81.00	3194.0
81.90	924.0
83.00	701.0
85.10	449.0
85.90	808.0
87.10	497.0
90.90	623.0
92.00	819.0
93.00	5105.0
93.90	451.0
96.00	463.0
98.00	4068.0
99.00	4079.0
100.10	441.0
101.00	2220.0
103.00	761.0
104.00	1298.0
105.00	1150.0
105.90	446.0
107.00	13982.0
108.10	2016.0
109.10	334.0
110.00	25720.0
111.00	4088.0
112.00	355.0
115.90	869.0
117.00	11591.0
118.00	823.0
122.00	831.0
122.90	1025.0
124.00	780.0
125.00	533.0
127.00	45464.0
128.00	3992.0
129.00	18016.0
130.00	1716.0
132.90	367.0
133.90	475.0
134.90	1505.0
135.90	715.0
137.00	800.0
138.00	305.0
141.00	2241.0
142.00	801.0
142.90	566.0
146.10	460.0
146.90	1242.0
148.00	3059.0
149.00	607.0
153.00	594.0
153.80	470.0
155.00	1102.0
156.00	1867.0
157.20	531.0
158.10	435.0
159.90	775.0
161.00	917.0
161.90	355.0
165.00	945.0
166.00	658.0
167.00	4010.0
168.00	4411.0
168.80	541.0
172.00	346.0
172.90	510.0
174.00	881.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

175.00	1607.0
175.90	524.0
176.80	645.0
179.00	3184.0
180.00	3741.0
181.10	1024.0
184.00	315.0
185.00	1643.0
186.00	12492.0
187.00	3536.0
188.10	471.0
189.00	913.0
191.00	370.0
191.90	920.0
193.00	1355.0
196.00	3164.0
196.90	580.0
198.00	82256.0
198.90	5876.0
200.00	509.0
201.60	458.0
203.00	600.0
204.00	2651.0
205.00	5415.0
206.10	19960.0
207.10	4255.0
208.00	1152.0
209.00	424.0
210.00	528.0
211.00	681.0
216.10	428.0
217.00	4980.0
217.90	524.0
221.00	3770.0
221.90	900.0
223.10	1154.0
224.10	11380.0
225.00	2740.0
225.90	484.0
227.00	5110.0
228.00	719.0
228.90	1089.0
231.00	382.0
233.80	369.0
237.00	891.0
242.10	691.0
242.80	394.0
243.20	461.0
244.10	8750.0
245.10	1160.0
246.10	1592.0
247.00	386.0
249.00	328.0
255.00	41040.0
256.00	6822.0
257.00	611.0
258.00	2378.0
259.00	396.0
265.00	792.0
272.90	902.0
274.00	3211.0
275.00	18584.0
276.00	2748.0
277.00	1350.0
293.00	504.0
296.00	4711.0
296.90	608.0
303.00	456.0
314.90	344.0
323.00	1523.0
328.00	339.0
334.00	697.0
334.90	312.0
345.90	389.0
352.00	526.0
354.00	447.0
365.00	1981.0
372.10	500.0
402.00	525.0
403.10	431.0
421.00	464.0
422.00	402.0
423.10	2376.0
424.10	1503.0
425.00	544.0
441.00	7017.0
442.00	48928.0
443.00	9800.0
444.00	1233.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

m/z	Abundance
38.10	594.0
39.00	3794.0
40.00	1546.0
44.00	4575.0
49.00	442.0
50.00	12576.0
51.10	53968.0
52.00	2500.0
54.90	302.0
55.90	1652.0
57.00	3734.0
61.00	718.0
62.00	642.0
63.00	2365.0
64.00	369.0
65.00	1164.0
68.00	1023.0
69.00	49560.0
72.90	948.0
74.00	5348.0
75.00	8159.0
76.10	2657.0
77.10	57168.0
78.10	4426.0
79.00	3746.0
80.00	3202.0
81.00	4317.0
82.00	1113.0
83.00	952.0
85.00	758.0
85.90	1130.0
87.00	525.0
91.00	1137.0
92.00	1373.0
93.00	6229.0
94.00	380.0
96.00	351.0
98.00	4699.0
99.00	4656.0
101.00	2659.0
102.90	627.0
104.00	1631.0
105.00	1389.0
106.00	409.0
107.00	16856.0
107.90	2623.0
109.00	494.0
110.00	31816.0
111.00	5004.0
112.00	469.0
116.00	841.0
117.00	13009.0
118.00	1345.0
122.00	1084.0
122.90	1880.0
124.00	658.0
124.80	780.0
127.00	58856.0
128.00	5254.0
129.00	22736.0
129.90	1978.0
130.90	350.0
134.00	692.0
135.00	1726.0
135.90	809.0
137.10	1095.0
141.00	2736.0
142.00	1199.0
142.90	733.0
145.90	582.0
146.90	1516.0
148.00	3072.0
148.90	927.0
150.00	358.0
151.00	498.0
152.00	313.0
153.00	858.0
153.90	769.0
155.10	1368.0
156.00	2670.0
157.10	541.0
157.80	525.0
158.90	410.0
159.90	862.0
161.00	1387.0
162.00	481.0
165.10	1112.0
166.10	834.0
167.00	5495.0
168.00	4136.0
169.00	664.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

170.80	310.0
172.00	517.0
172.90	583.0
173.90	1303.0
175.00	2723.0
176.00	864.0
176.90	1292.0
177.90	422.0
178.90	4270.0
180.00	3963.0
181.00	1331.0
185.00	2244.0
186.10	15150.0
187.10	4638.0
188.10	789.0
188.90	1035.0
191.00	618.0
192.00	1589.0
193.00	1448.0
196.00	2831.0
197.00	535.0
198.00	118056.0
199.00	8273.0
200.10	669.0
201.60	625.0
203.00	870.0
204.00	4027.0
205.10	6521.0
206.10	29552.0
207.00	5192.0
208.00	1292.0
209.00	616.0
210.10	784.0
211.00	1225.0
214.90	308.0
215.90	420.0
216.10	410.0
217.00	7259.0
218.00	901.0
221.00	5328.0
221.90	1351.0
223.00	1618.0
224.00	15561.0
225.10	5273.0
225.90	669.0
227.00	6425.0
228.00	890.0
229.00	1433.0
231.10	613.0
233.90	406.0
234.90	615.0
236.90	1177.0
240.10	423.0
241.00	331.0
242.00	1118.0
243.10	869.0
244.10	12653.0
245.10	1628.0
246.00	2003.0
246.90	452.0
248.70	335.0
254.10	374.0
255.10	63664.0
256.00	9889.0
257.00	980.0
258.00	3584.0
259.00	695.0
265.00	1772.0
273.00	1742.0
274.00	4660.0
275.00	28144.0
276.10	3730.0
277.00	2061.0
277.90	673.0
285.10	530.0
293.00	550.0
296.00	6924.0
296.90	1111.0
303.00	968.0
315.00	773.0
315.80	435.0
323.10	2528.0
324.10	431.0
327.00	424.0
333.90	1335.0
335.10	400.0
341.00	341.0
346.10	300.0
351.90	555.0
353.00	589.0
354.10	1131.0
365.00	3233.0
366.00	477.0
372.10	1056.0
383.10	554.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

402.00	468.0
403.00	1039.0
404.10	471.0
421.00	697.0
422.00	527.0
423.00	5399.0
424.00	2934.0
424.90	560.0
441.00	14976.0
442.00	94920.0
443.00	18464.0
444.10	1494.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

m/z	Abundance
38.00	408.0
39.00	2558.0
40.00	1169.0
44.00	3903.0
49.00	452.0
50.10	8597.0
51.10	34824.0
52.10	1668.0
56.00	1275.0
57.00	2405.0
61.00	515.0
61.90	618.0
63.10	1392.0
65.10	860.0
68.10	656.0
69.00	33336.0
73.00	702.0
74.00	3255.0
75.00	5772.0
76.00	1673.0
77.10	38232.0
78.00	2856.0
79.00	2374.0
80.00	1895.0
81.00	2855.0
82.00	513.0
83.00	638.0
84.90	594.0
86.00	717.0
87.00	431.0
91.00	675.0
91.90	918.0
93.00	4921.0
93.90	343.0
95.90	401.0
98.00	3740.0
99.00	3825.0
99.90	300.0
101.00	1628.0
103.10	383.0
103.90	1141.0
105.00	901.0
106.00	363.0
107.00	13168.0
108.00	1611.0
109.00	544.0
110.00	21456.0
111.00	3386.0
112.00	662.0
116.00	641.0
117.00	8739.0
118.00	598.0
121.90	743.0
123.00	1178.0
124.00	475.0
125.00	533.0
127.00	43728.0
128.00	3549.0
129.00	16086.0
130.00	1332.0
132.20	300.0
133.90	572.0
135.00	1119.0
136.00	450.0
137.10	903.0
141.00	1965.0
142.10	699.0
143.10	521.0
146.00	346.0
147.00	1140.0
148.00	2950.0
149.10	438.0
152.90	725.0
154.00	625.0
154.90	1335.0
156.00	1649.0
157.00	482.0
159.90	658.0
161.00	875.0
162.10	313.0
165.10	662.0
166.00	570.0
167.00	4765.0
168.00	3460.0
169.00	448.0
172.00	365.0
172.80	503.0
174.00	815.0
175.00	1914.0
176.00	396.0
176.80	593.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

179.00	3767.0
180.00	2678.0
181.00	1091.0
185.00	1553.0
186.00	13312.0
187.00	3550.0
188.00	439.0
189.00	1007.0
191.10	617.0
192.10	949.0
193.10	1708.0
195.10	362.0
196.00	3106.0
196.80	465.0
198.00	90976.0
199.00	6127.0
200.00	445.0
201.50	436.0
203.00	567.0
204.10	3207.0
205.00	5205.0
206.10	23928.0
207.10	3897.0
208.00	999.0
209.00	520.0
210.20	357.0
211.00	798.0
215.90	540.0
217.00	6654.0
218.00	751.0
221.00	3712.0
222.90	1290.0
224.10	12879.0
225.00	2690.0
226.00	345.0
227.00	4896.0
228.00	672.0
229.00	1169.0
229.90	313.0
231.00	462.0
235.10	335.0
237.10	973.0
239.90	329.0
242.00	548.0
243.10	800.0
244.10	9512.0
245.00	1325.0
246.00	2065.0
247.00	364.0
249.00	376.0
253.80	339.0
255.00	53304.0
256.00	6969.0
257.10	668.0
257.90	2391.0
259.00	573.0
265.00	1255.0
273.00	1974.0
274.00	4607.0
275.00	24176.0
276.10	3351.0
277.00	1884.0
278.00	308.0
282.90	388.0
293.00	457.0
296.00	6326.0
296.80	478.0
297.00	473.0
302.90	606.0
315.00	918.0
316.00	338.0
320.90	383.0
323.00	1922.0
324.00	404.0
327.10	347.0
334.00	1910.0
335.10	371.0
345.80	518.0
352.00	613.0
352.80	441.0
353.10	410.0
354.00	685.0
365.00	2708.0
366.00	367.0
371.90	1065.0
382.90	307.0
401.90	454.0
402.90	770.0
404.00	371.0
421.10	370.0
422.10	404.0
423.10	4309.0
424.10	2662.0
425.00	373.0
441.10	15321.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

442.00	97712.0
443.00	17856.0
444.00	1755.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41

Scan 2507 (17.433 min): BM000737.D
DFTPP41

m/z	Abundance
40.00	1195.0
44.00	3902.0
73.00	570.0
207.00	1255.0

Instrument :
BNA_M
ClientSampleId :
DFTPP41