

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032016\
 Data File : BM004708.D
 Acq On : 20 Mar 2016 16:16
 Operator : UM/SJ
 Sample : MDL-BL-W
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 MDL-BL-W

Quant Time: Mar 21 02:47:57 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM031816.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Sat Mar 19 07:50:46 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	36194	5.00	ng	0.00
6) Naphthalene-d8	10.61	136	141667	5.00	ng	-0.02
10) Acenaphthene-d10	14.46	164	71733	5.00	ng	0.00
16) Phenanthrene-d10	17.19	188	137639	5.00	ng	-0.03
22) Chrysene-d12	21.39	240	149272	5.00	ng	0.00
28) Perylene-d12	23.69	264	125409	5.00	ng	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
4) 2-Fluorophenol	5.42	112	55658	6.66	ng	0.00
5) Phenol-d6	6.99	99	66433	6.49	ng	0.00
7) Nitrobenzene-d5	8.99	82	22180	3.25	ng	0.00
11) 2,4,6-Tribromophenol	15.95	330	12171	5.12	ng	0.00
12) 2-Fluorobiphenyl	13.09	172	94277	4.59	ng	0.00
24) Terphenyl-d14	19.84	244	76641	4.06	ng	0.00


Target Compounds	Qvalue
------------------	--------


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032016\
Data File : BM004708.D
Acq On : 20 Mar 2016 16:16
Operator : UM/SJ
Sample : MDL-BL-W
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
MDL-BL-W

Quant Time: Mar 21 02:47:57 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM031816.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Sat Mar 19 07:50:46 2016
Response via : Initial Calibration

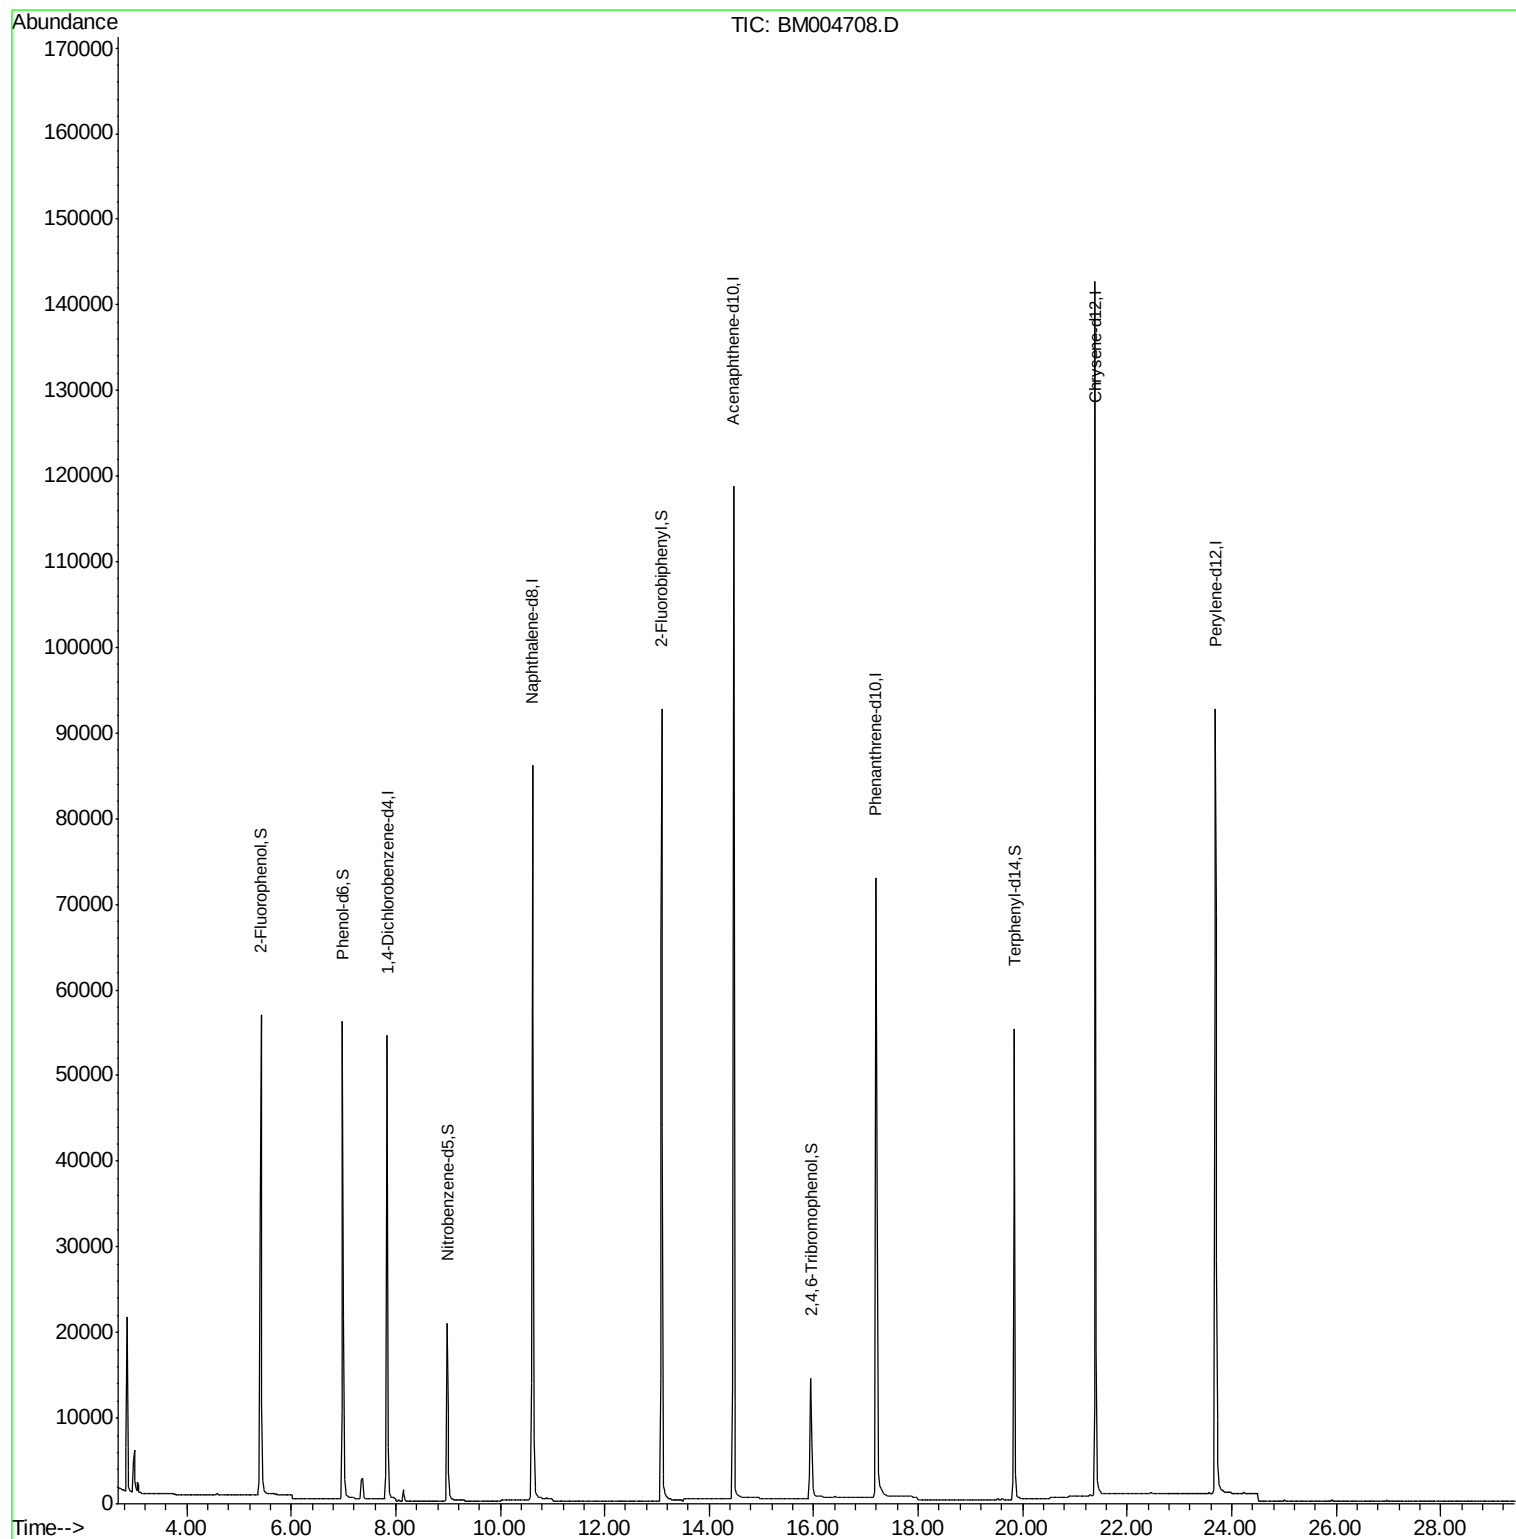


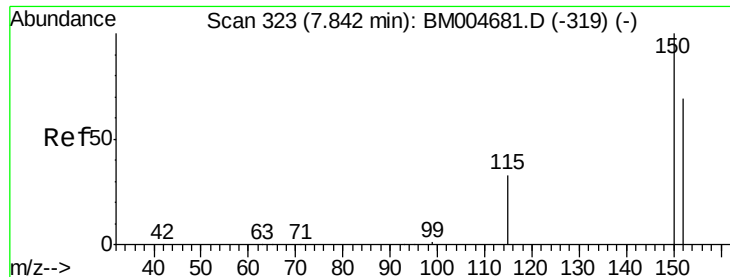




#1
 1,4-Dichlorobenzene-d4
 Concen: 5.00 ng
 RT: 7.84 min Scan# 323
 Delta R.T. 0.00 min
 Lab File: BM004708.D
 Acq: 20 Mar 2016 16:16

Instrument :
 BNA_M
 ClientSampleId :
 MDL-BL-W

Tgt Ion:152 Resp: 36194
 Ion Ratio Lower Upper
 152 100
 150 139.9 115.9 173.9
 115 44.8 38.4 57.6

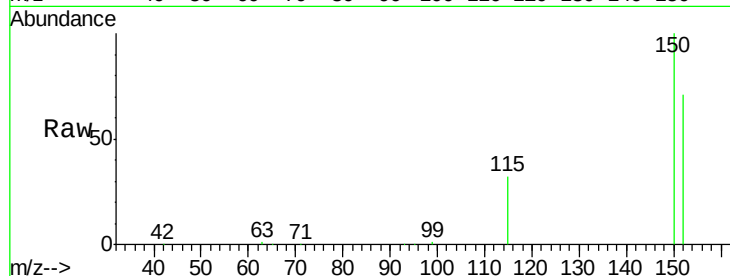


Abundance Ion 152.00 (151.70 to 152.70): E
 Ion 150.00 (149.70 to 150.70): E
 Ion 115.00 (114.70 to 115.70): E

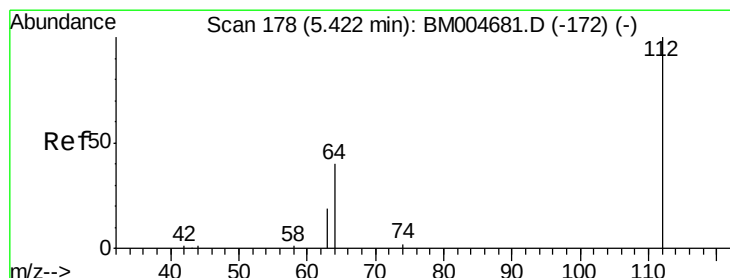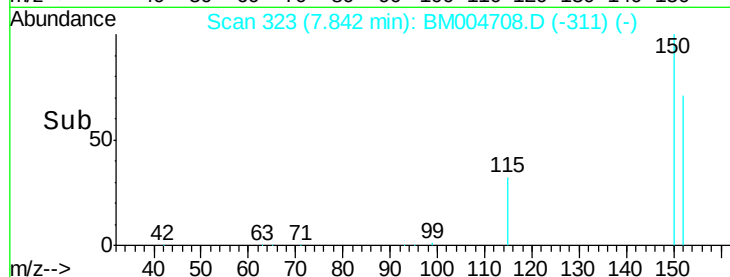
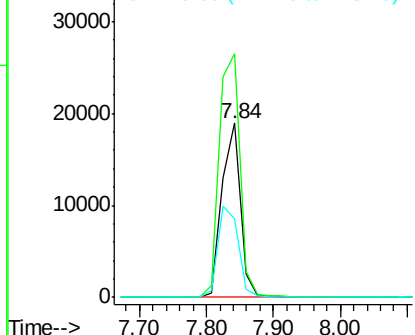



#4
 2-Fluorophenol
 Concen: 6.66 ng
 RT: 5.42 min Scan# 178
 Delta R.T. 0.00 min
 Lab File: BM004708.D
 Acq: 20 Mar 2016 16:16

Tgt Ion:112 Resp: 55658
 Ion Ratio Lower Upper
 112 100
 64 46.4 37.0 55.6
 63 23.7 19.3 28.9

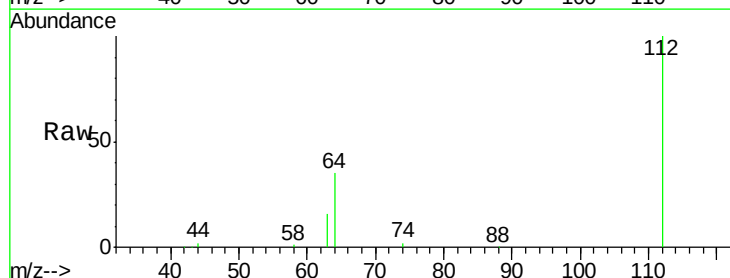

Abundance Ion 112.00 (111.70 to 112.70): E
 Ion 64.00 (63.70 to 64.70): BM0
 Ion 63.00 (62.70 to 63.70): BM0

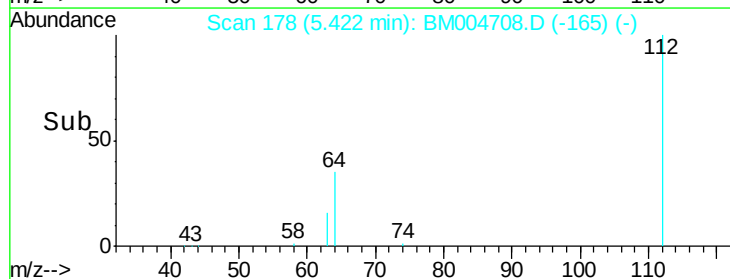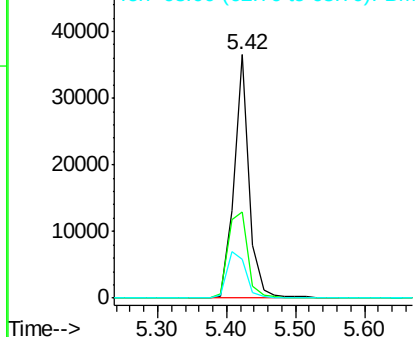

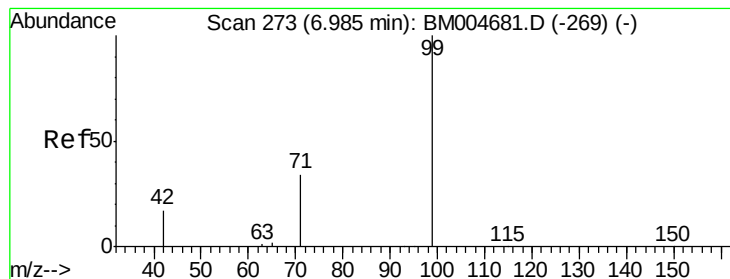

#5

Phenol-d6

Concen: 6.49 ng

RT: 6.99 min Scan# 273

Delta R.T. 0.00 min

Lab File: BM004708.D

Acq: 20 Mar 2016 16:16

Instrument :

BNA_M

ClientSampleId :

MDL-BL-W


Tgt Ion: 99 Resp: 66433

Ion Ratio Lower Upper

99 100

42 13.9 12.7 19.1




71 27.6 22.9 34.3

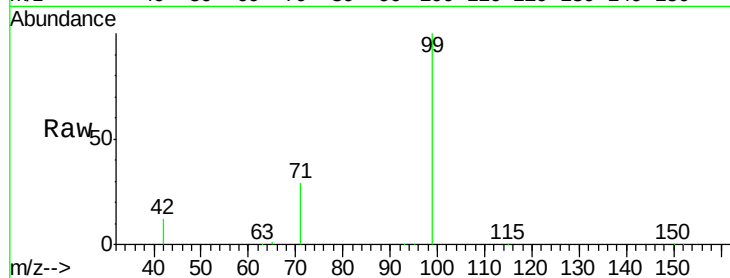

Abundance Ion 99.00 (98.70 to 99.70): BM004708.D (-269) (-)

Ion 42.00 (41.70 to 42.70): BM004708.D (-269) (-)

Ion 71.00 (70.70 to 71.70): BM004708.D (-269) (-)

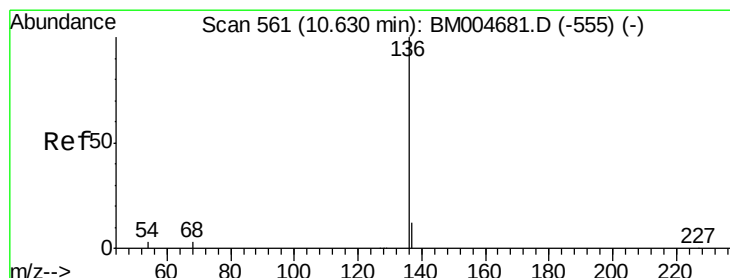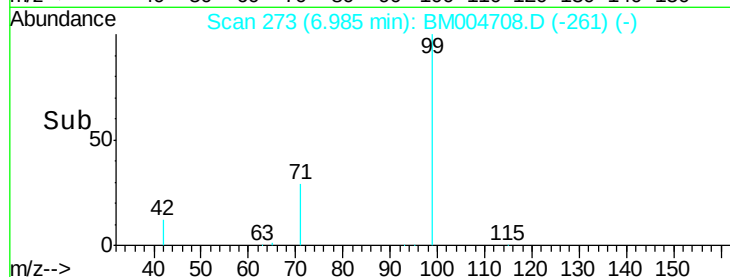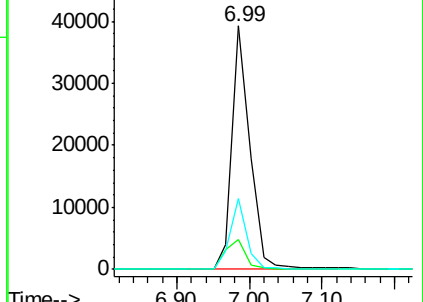

#6

Naphthalene-d8

Concen: 5.00 ng

RT: 10.61 min Scan# 560

Delta R.T. -0.02 min

Lab File: BM004708.D

Acq: 20 Mar 2016 16:16

Tgt Ion: 136 Resp: 141667


Ion Ratio Lower Upper

136 100

137 10.2 9.4 14.2

54 6.8 2.2 3.4#

68 5.8 2.2 3.4#


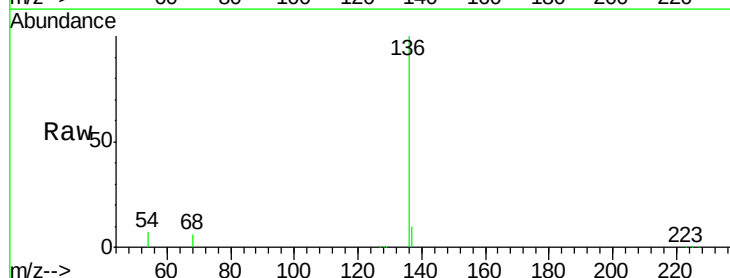



Abundance Ion 136.00 (135.70 to 136.70): BM004708.D (-549) (-)

Ion 137.00 (136.70 to 137.70): BM004708.D (-549) (-)

Ion 54.00 (53.70 to 54.70): BM004708.D (-549) (-)

Ion 68.00 (67.70 to 68.70): BM004708.D (-549) (-)

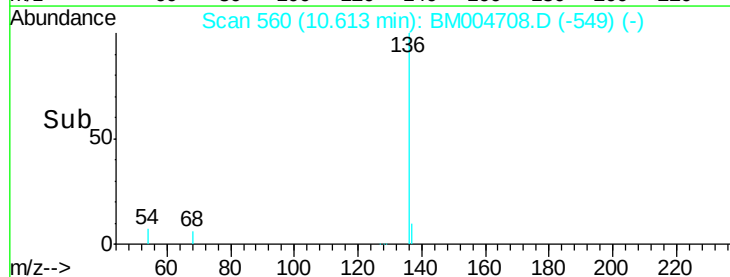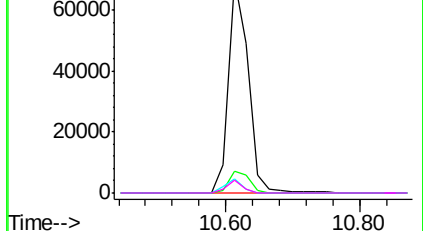

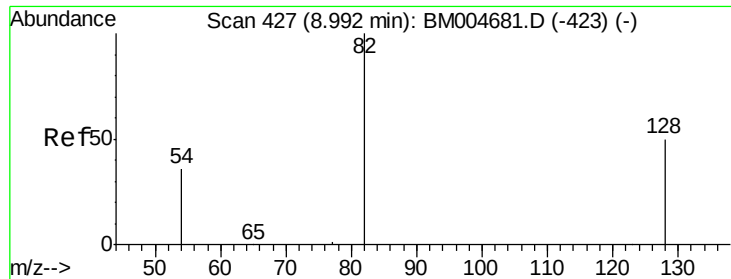

#7

Nitrobenzene-d5

Concen: 3.25 ng

RT: 8.99 min Scan# 427

Delta R.T. 0.00 min

Lab File: BM004708.D

Acq: 20 Mar 2016 16:16

Instrument :

BNA_M

ClientSampleId :

MDL-BL-W


Tgt Ion: 82 Resp: 22180

Ion Ratio Lower Upper

82 100

128 52.1 41.8 62.8




54 34.9 32.9 49.3



Abundance Ion 82.00 (81.70 to 82.70): BM004708.D (-408) (-)

Ion 128.00 (127.70 to 128.70): BM004708.D (-408) (-)

Ion 54.00 (53.70 to 54.70): BM004708.D (-408) (-)

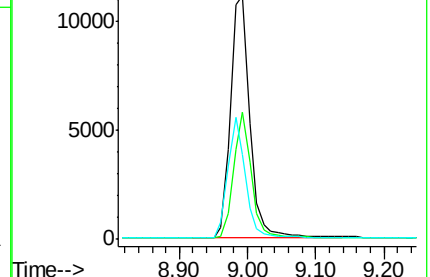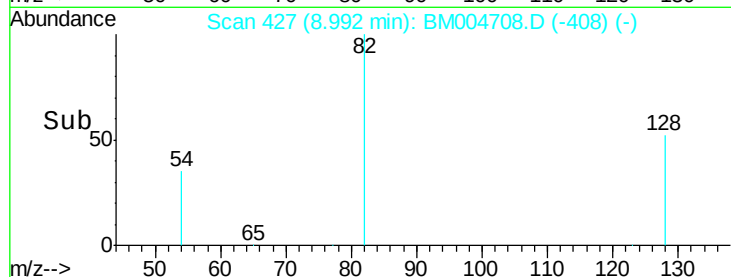

#10

Acenaphthene-d10

Concen: 5.00 ng

RT: 14.46 min Scan# 866

Delta R.T. 0.00 min

Lab File: BM004708.D

Acq: 20 Mar 2016 16:16


Tgt Ion: 164 Resp: 71733

Ion Ratio Lower Upper

164 100

162 102.3 85.4 128.0



160 46.0 40.2 60.2




Abundance Ion 164.00 (163.70 to 164.70): BM004708.D (-857) (-)

Ion 162.00 (161.70 to 162.70): BM004708.D (-857) (-)

Ion 160.00 (159.70 to 160.70): BM004708.D (-857) (-)

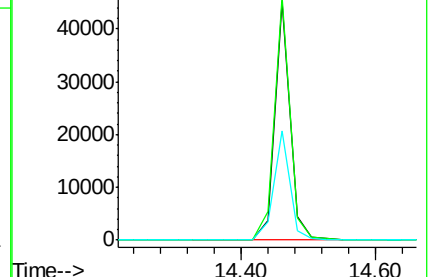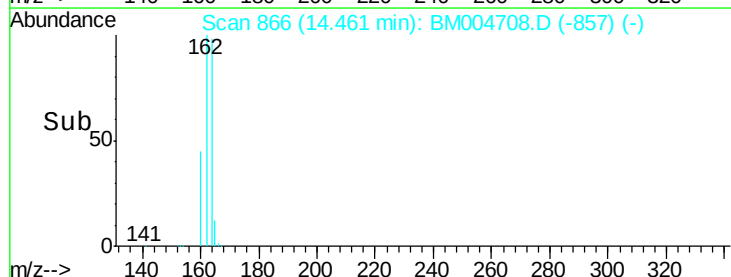


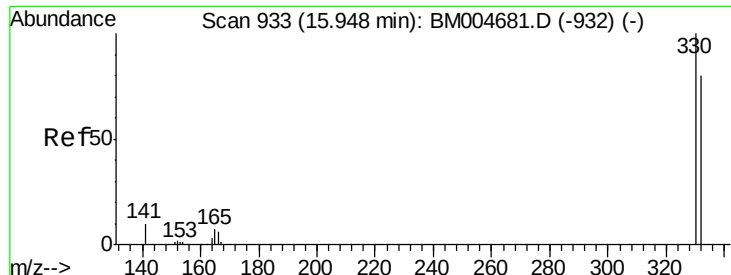




#11
 2,4,6-Tribromophenol
 Concen: 5.12 ng
 RT: 15.95 min Scan# 933
 Delta R.T. 0.00 min
 Lab File: BM004708.D
 Acq: 20 Mar 2016 16:16

Instrument :
 BNA_M
 ClientSampleId :
 MDL-BL-W

Tgt Ion:330 Resp: 12171
 Ion Ratio Lower Upper
 330 100
 332 94.0 93.9 140.9
 141 0.0 42.2 63.2#

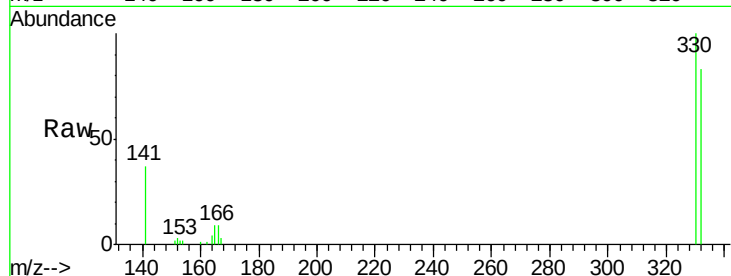


Abundance Ion 329.80 (329.50 to 330.50): E
 Ion 331.80 (331.50 to 332.50): E
 Ion 141.00 (140.70 to 141.70): E

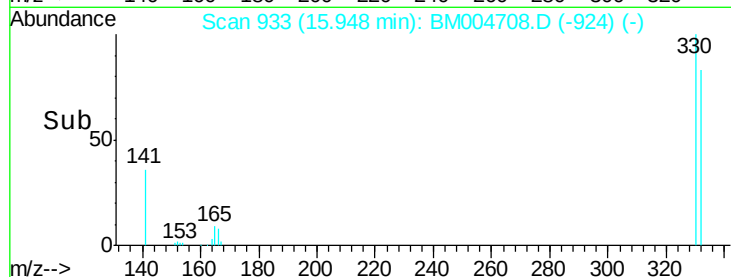
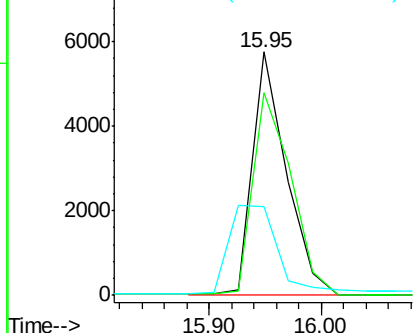



#12
 2-Fluorobiphenyl
 Concen: 4.59 ng
 RT: 13.09 min Scan# 783
 Delta R.T. 0.00 min
 Lab File: BM004708.D
 Acq: 20 Mar 2016 16:16

Tgt Ion:172 Resp: 94277
 Ion Ratio Lower Upper
 172 100
 171 33.0 28.2 42.2
 170 21.2 19.4 29.2



Abundance Ion 172.00 (171.70 to 172.70): E
 Ion 171.00 (170.70 to 171.70): E
 Ion 170.00 (169.70 to 170.70): E

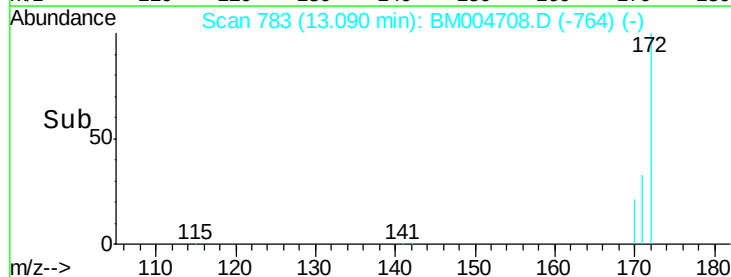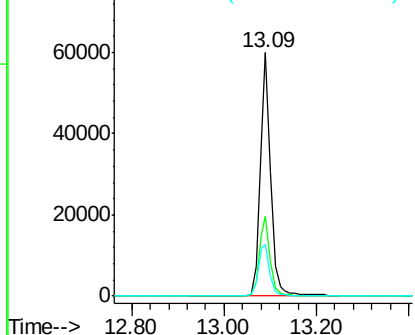

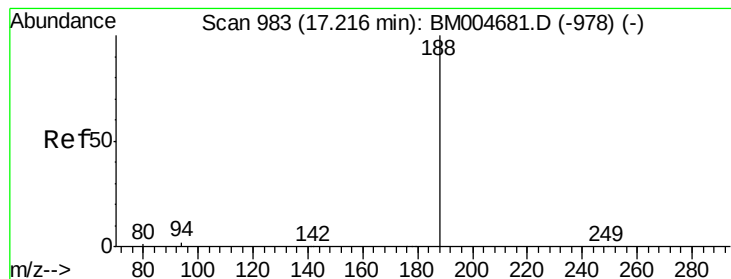

#16

Phenanthrene-d10

Concen: 5.00 ng

RT: 17.19 min Scan# 982

Delta R.T. -0.03 min

Lab File: BM004708.D

Acq: 20 Mar 2016 16:16

Instrument :

BNA_M

ClientSampleId :

MDL-BL-W


Tgt Ion:188 Resp: 137639

Ion Ratio Lower Upper

188 100

94 18.9 1.4 2.0#




80 19.6 1.0 1.6#



Abundance Ion 188.00 (187.70 to 188.70): E

Ion 94.00 (93.70 to 94.70): BM0

Ion 80.00 (79.70 to 80.70): BM0

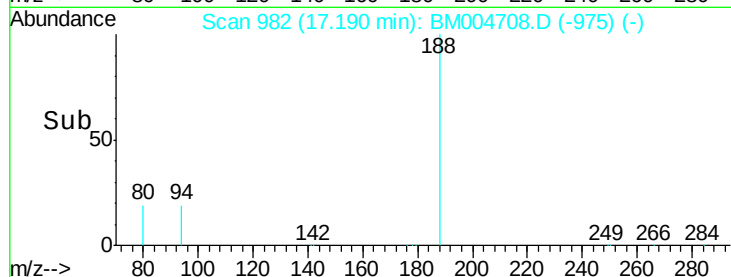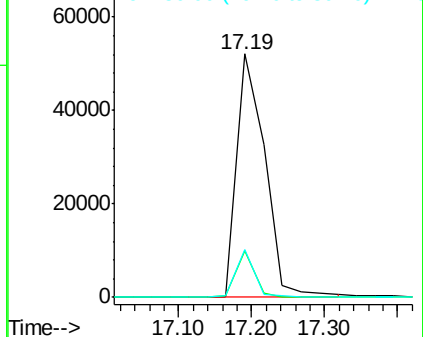

#22

Chrysene-d12

Concen: 5.00 ng

RT: 21.39 min Scan# 1203

Delta R.T. 0.00 min

Lab File: BM004708.D

Acq: 20 Mar 2016 16:16


Tgt Ion:240 Resp: 149272

Ion Ratio Lower Upper

240 100

120 7.2 7.4 11.2#



236 29.1 24.5 36.7




Abundance Ion 240.00 (239.70 to 240.70): E

Ion 120.00 (119.70 to 120.70): E

Ion 236.00 (235.70 to 236.70): E

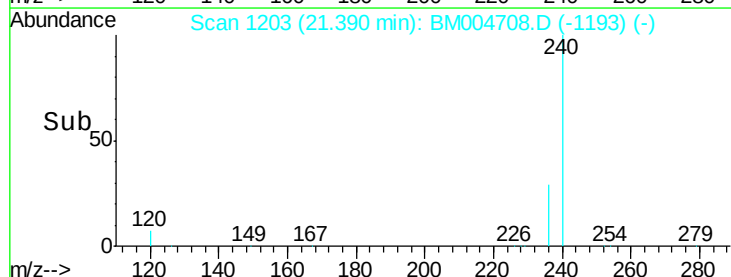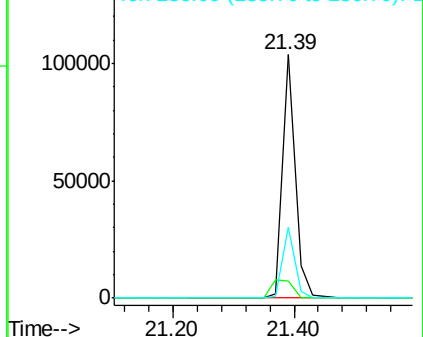

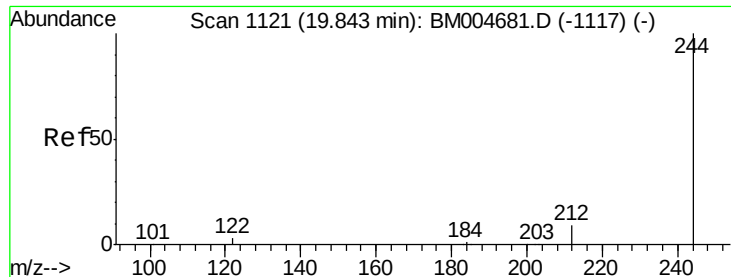

#24

Terphenyl-d14

Concen: 4.06 ng

RT: 19.84 min Scan# 1121

Delta R.T. 0.00 min

Lab File: BM004708.D

Acq: 20 Mar 2016 16:16

Instrument :

BNA_M

ClientSampleId :

MDL-BL-W


Tgt Ion:244 Resp: 76641

Ion Ratio Lower Upper




244 100

212 8.6 7.7 11.5

122 2.0 3.4 5.0#

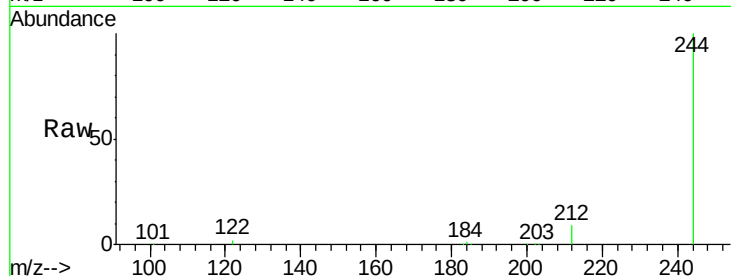

Abundance Ion 244.00 (243.70 to 244.70): E
Ion 212.00 (211.70 to 212.70): E
Ion 122.00 (121.70 to 122.70): E

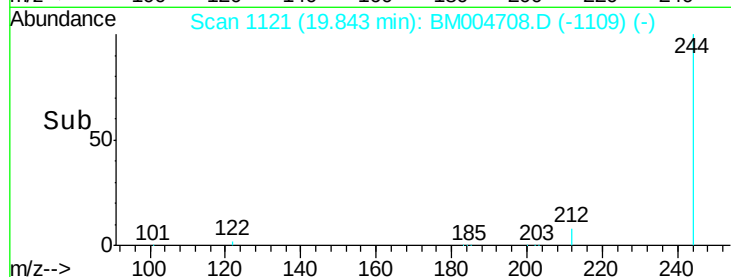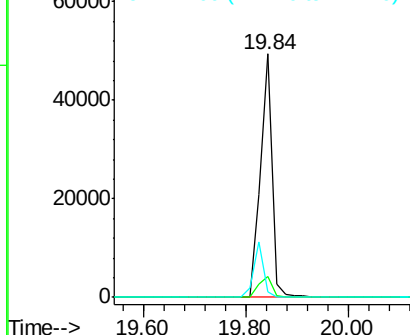

#28

Perylene-d12

Concen: 5.00 ng

RT: 23.69 min Scan# 1361

Delta R.T. 0.00 min

Lab File: BM004708.D

Acq: 20 Mar 2016 16:16


Tgt Ion:264 Resp: 125409

Ion Ratio Lower Upper

264 100

260 25.6 21.0 31.4

265 21.8 17.5 26.3



Abundance Ion 264.00 (263.70 to 264.70): E
Ion 260.00 (259.70 to 260.70): E
Ion 265.00 (264.70 to 265.70): E

