


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032016\
 Data File : BM004699.D
 Acq On : 20 Mar 2016 09:43
 Operator : UM/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-SIM-BM031816.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Sat Mar 19 07:50:46 2016

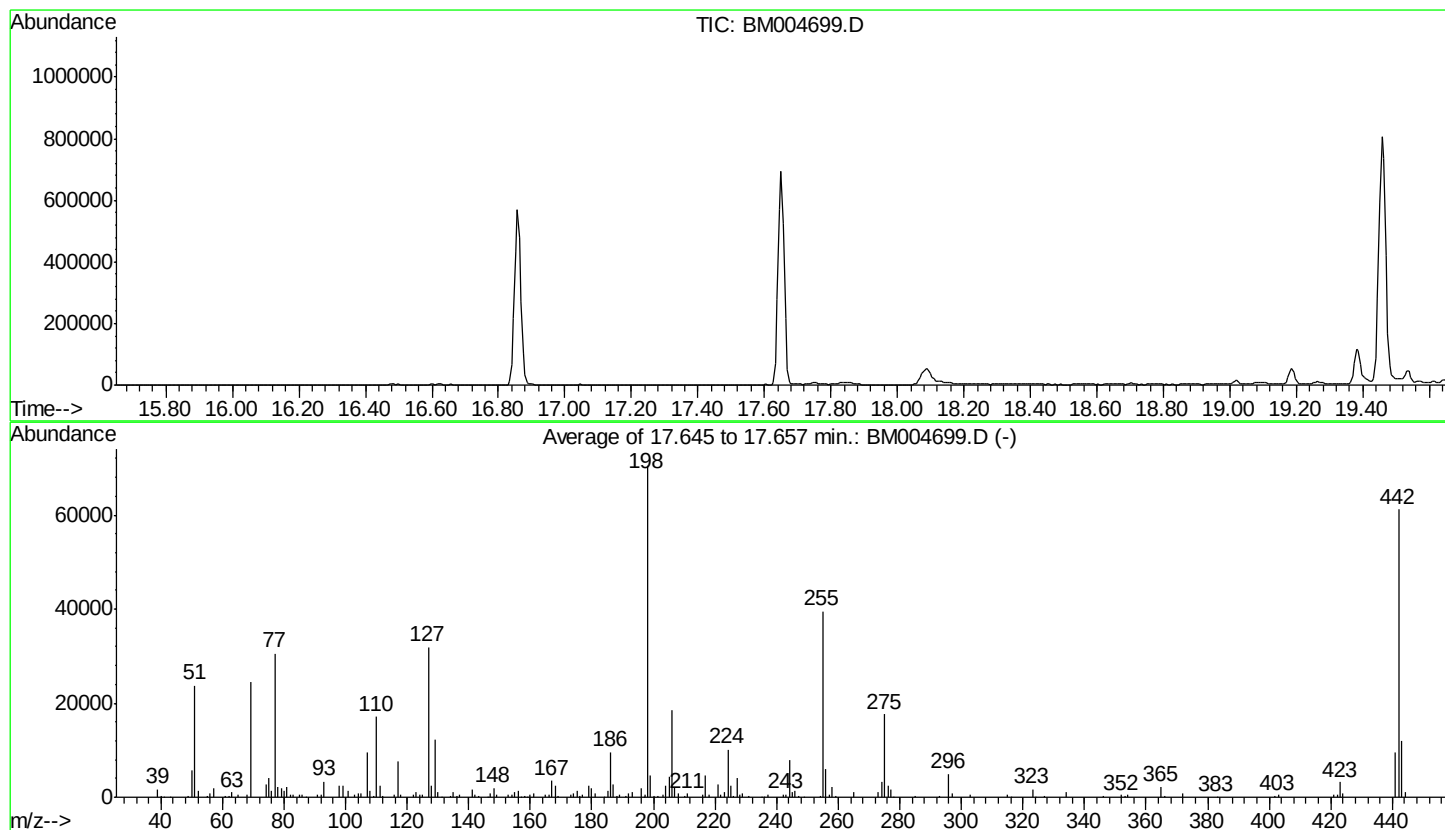

AutoFind: Scans 2543, 2544, 2545; Background Corrected with Scan 2537

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	33.8	23800	PASS
68	69	0.00	2	1.8	431	PASS
69	198	0.00	100	34.7	24448	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	45.3	31912	PASS
197	198	0.00	2	0.6	434	PASS
198	198	100	100	100.0	70498	PASS
199	198	5	9	6.6	4678	PASS
275	198	10	60	24.9	17581	PASS
365	198	1	100	3.1	2186	PASS
441	442	0.01	24	15.5	9496	PASS
442	198	50	100	86.8	61165	PASS
443	442	15	24	19.4	11894	PASS