

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032017\
 Data File : BM009292.D
 Acq On : 20 Mar 2017 13:21
 Operator : SJ/MA
 Sample : I2303-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BD3

Quant Time: Mar 20 13:56:06 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031317MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Mon Mar 20 13:19:54 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	79959	20.00	ng/ul	0.00
18) Naphthalene-d8	10.67	136	358800	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.52	164	261359	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.26	188	698529	20.00	ng/ul	0.00
77) Chrysene-d12	21.43	240	1147483	20.00	ng/ul	0.00
85) Perylene-d12	23.77	264	1236207	20.00	ng/ul	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
3) 1,4-Dioxane-d8	3.34	96	10968	6.04	ng/uL	0.00
5) Phenol-d5	7.03	99	45821	5.30	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.20	67	178726	31.72	ng/ul	0.00
9) 2-Chlorophenol-d4	7.40	132	130625	24.71	ng/ul	0.00
13) 4-Methylphenol-d8	8.57	113	97181	14.08	ng/ul	0.00
19) Nitrobenzene-d5	9.04	128	94251	36.78	ng/ul	0.00
22) 2-Nitrophenol-d4	9.76	143	101254	35.60	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.29	165	188276	30.99	ng/ul	0.00
29) 4-Chloroaniline-d4	10.82	131	9905	1.37	ng/ul	0.00
43) Dimethylphthalate-d6	13.92	166	768447	38.71	ng/ul	0.00
46) Acenaphthylene-d8	14.21	160	919825	40.30	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	20432	5.18	ng/ul	0.00
57) Fluorene-d10	15.51	176	739891	41.77	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	127305	30.46	ng/ul	0.00
70) Anthracene-d10	17.36	188	1305833	39.50	ng/ul	0.00
78) Pyrene-d10	19.65	212	1681610	36.31	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.62	264	2181505	38.57	ng/ul	0.00


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
56) Diethylphthalate	15.33	149	27159	1.30	ng/ul#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032017\
Data File : BM009292.D
Acq On : 20 Mar 2017 13:21
Operator : SJ/MA
Sample : I2303-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BD3

Quant Time: Mar 20 13:56:06 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031317MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Mon Mar 20 13:19:54 2017
Response via : Initial Calibration

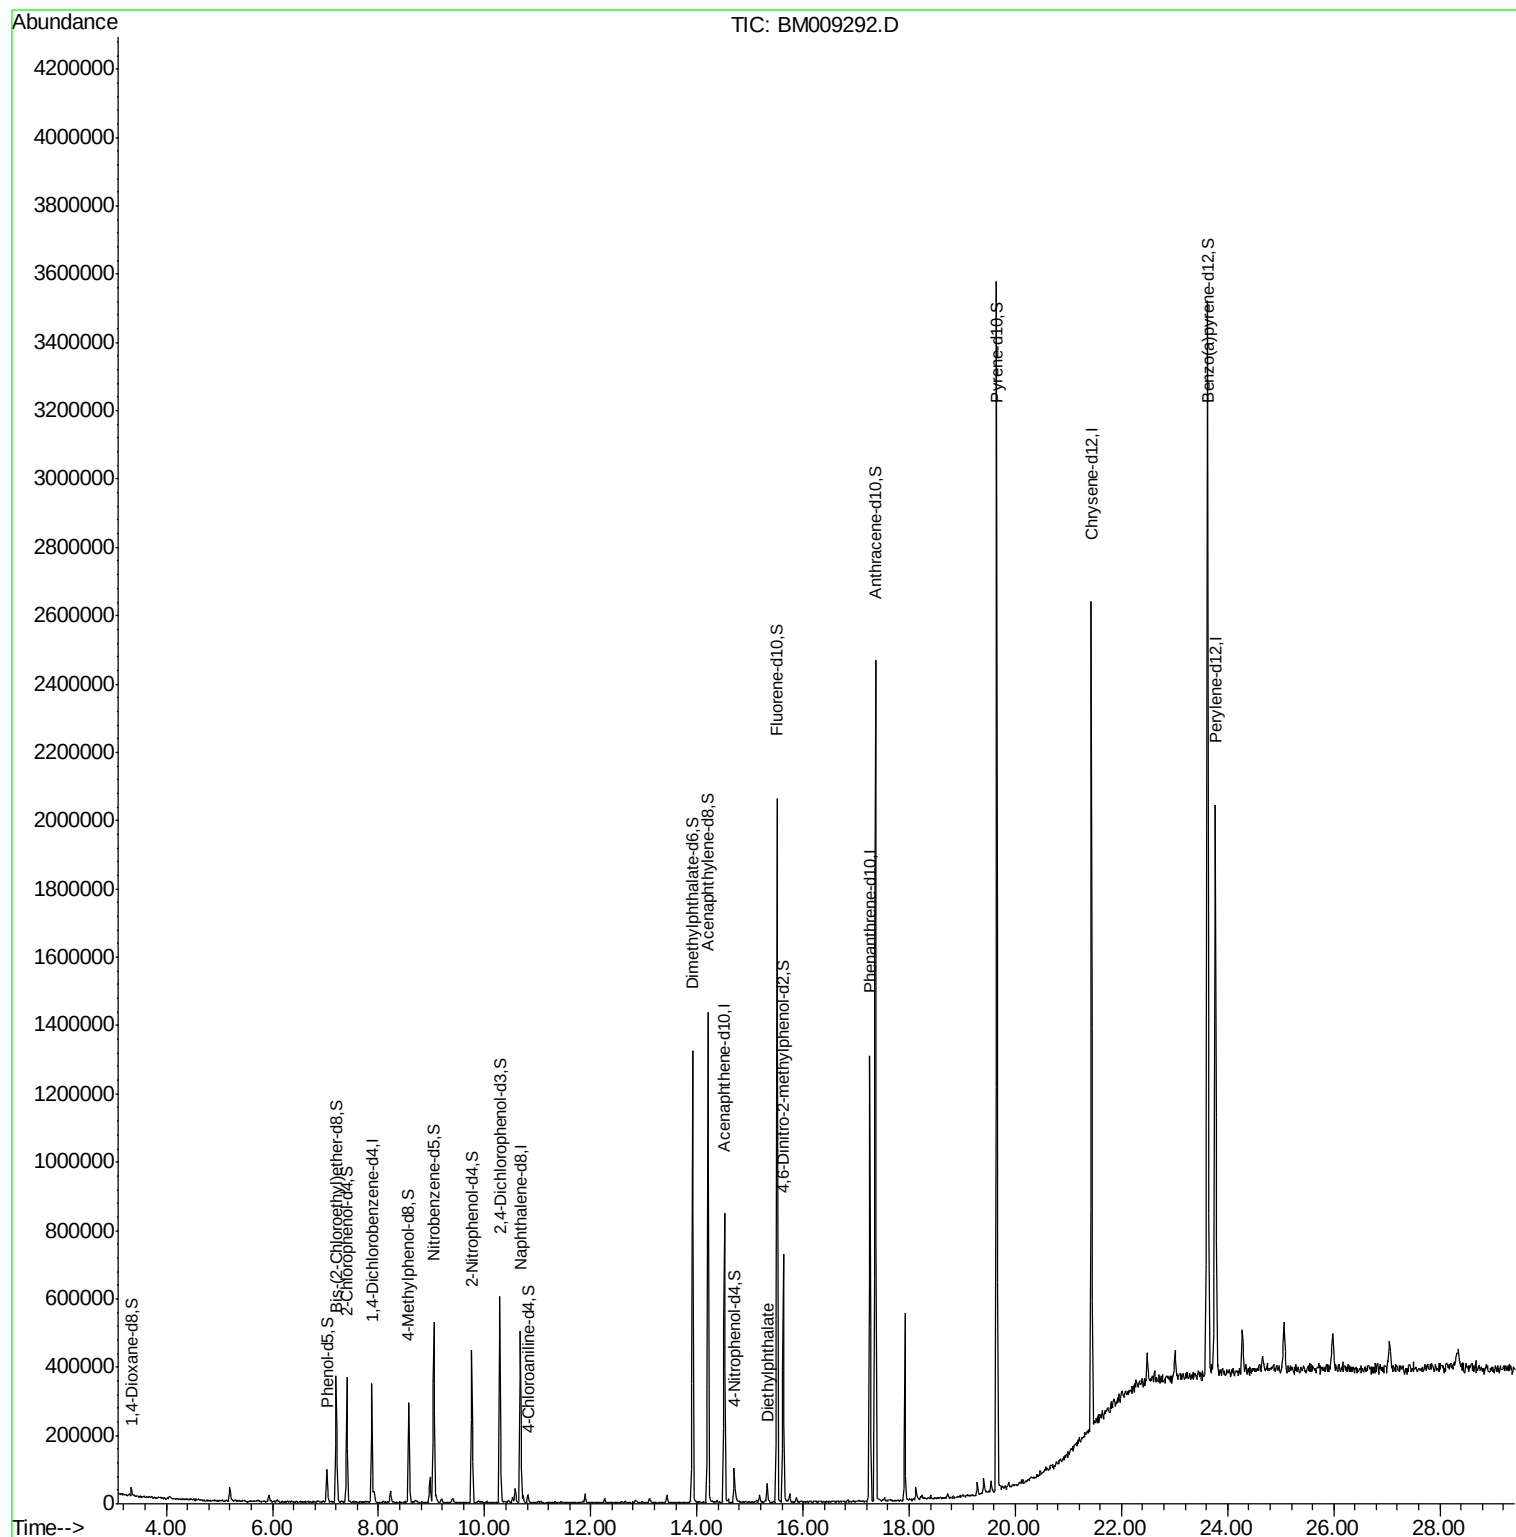


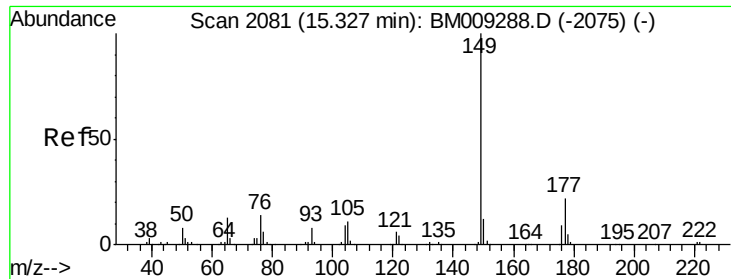

#56
 Diethylphthalate
 Concen: 1.30 ng/ul
 RT: 15.33 min Scan# 2081
 Delta R.T. -0.00 min
 Lab File: BM009292.D
 Acq: 20 Mar 2017 13:21

Instrument :
 BNA_M
 ClientSampleId :
 C0BD3

Tgt Ion	Ratio	Lower	Upper
149	100		
177	26.8	17.4	26.2#
150	11.9	10.0	15.0

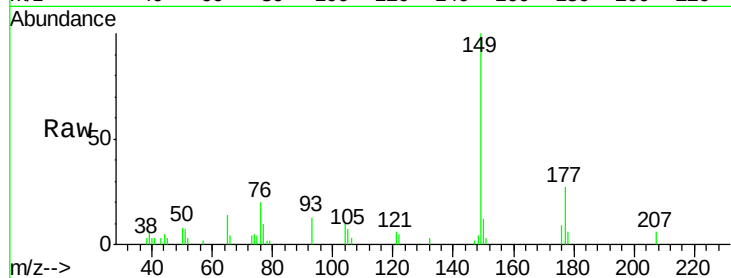

Abundance Ion 149.00 (148.70 to 149.70): E
 Ion 177.00 (176.70 to 177.70): E
 Ion 150.00 (149.70 to 150.70): E

