

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032017\
 Data File : BM009305.D
 Acq On : 20 Mar 2017 21:11
 Operator : SJ/MA
 Sample : I2303-11
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C0BH7

Quant Time: Mar 21 03:23:56 2017
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031317MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Tue Mar 21 03:09:49 2017
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.87	152	123608	20.00	ng/ul	0.00
18) Naphthalene-d8	10.67	136	541123	20.00	ng/ul	0.00
35) Acenaphthene-d10	14.52	164	354088	20.00	ng/ul	0.00
61) Phenanthrene-d10	17.26	188	924815	20.00	ng/ul	0.00
77) Chrysene-d12	21.43	240	1436598	20.00	ng/ul	0.00
85) Perylene-d12	23.77	264	1505875	20.00	ng/ul	0.00

System Monitoring Compounds

3) 1,4-Dioxane-d8	3.34	96	12630	4.50	ng/uL	0.00
5) Phenol-d5	7.03	99	65450	4.89	ng/ul	0.00
7) Bis-(2-Chloroethyl)ether-d	7.20	67	242501	27.84	ng/ul	0.00
9) 2-Chlorophenol-d4	7.40	132	187806	22.98	ng/ul	0.00
13) 4-Methylphenol-d8	8.57	113	132367	12.41	ng/ul	0.00
19) Nitrobenzene-d5	9.04	128	127675	33.04	ng/ul	0.00
22) 2-Nitrophenol-d4	9.76	143	144304	33.64	ng/ul	0.00
26) 2,4-Dichlorophenol-d3	10.29	165	251379	27.44	ng/ul	0.00
29) 4-Chloroaniline-d4	0.00	131	0d	0.00	ng/ul	
43) Dimethylphthalate-d6	13.92	166	1003576	37.32	ng/ul	0.00
46) Acenaphthylene-d8	14.21	160	1199408	38.78	ng/ul	0.00
51) 4-Nitrophenol-d4	14.70	143	30902	5.79	ng/ul	0.00
57) Fluorene-d10	15.50	176	932075	38.84	ng/ul	0.00
62) 4,6-Dinitro-2-methylphenol	15.63	200	172992	31.27	ng/ul	0.00
70) Anthracene-d10	17.36	188	1649126	37.68	ng/ul	0.00
78) Pyrene-d10	19.65	212	2130186	36.74	ng/ul	0.00
89) Benzo(a)pyrene-d12	23.62	264	2557289	37.12	ng/ul	0.00


Target Compounds						Qvalue
20) Nitrobenzene	9.08	77	376947	29.25	ng/ul#	84
36) 1,2,4,5-Tetrachlorobenzene	12.70	216	167575	15.74	ng/ul	96
72) 1,2,3,4-Tetrachlorobenzene	13.31	216	821392	75.60	ng/uL	99
73) Pentachlorobenzene	14.83	250	40859	3.50	ng/uL	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032017\
Data File : BM009305.D
Acq On : 20 Mar 2017 21:11
Operator : SJ/MA
Sample : I2303-11
Misc :
ALS Vial : 18 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C0BH7

Quant Time: Mar 21 03:23:56 2017
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-BM031317MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Tue Mar 21 03:09:49 2017
Response via : Initial Calibration

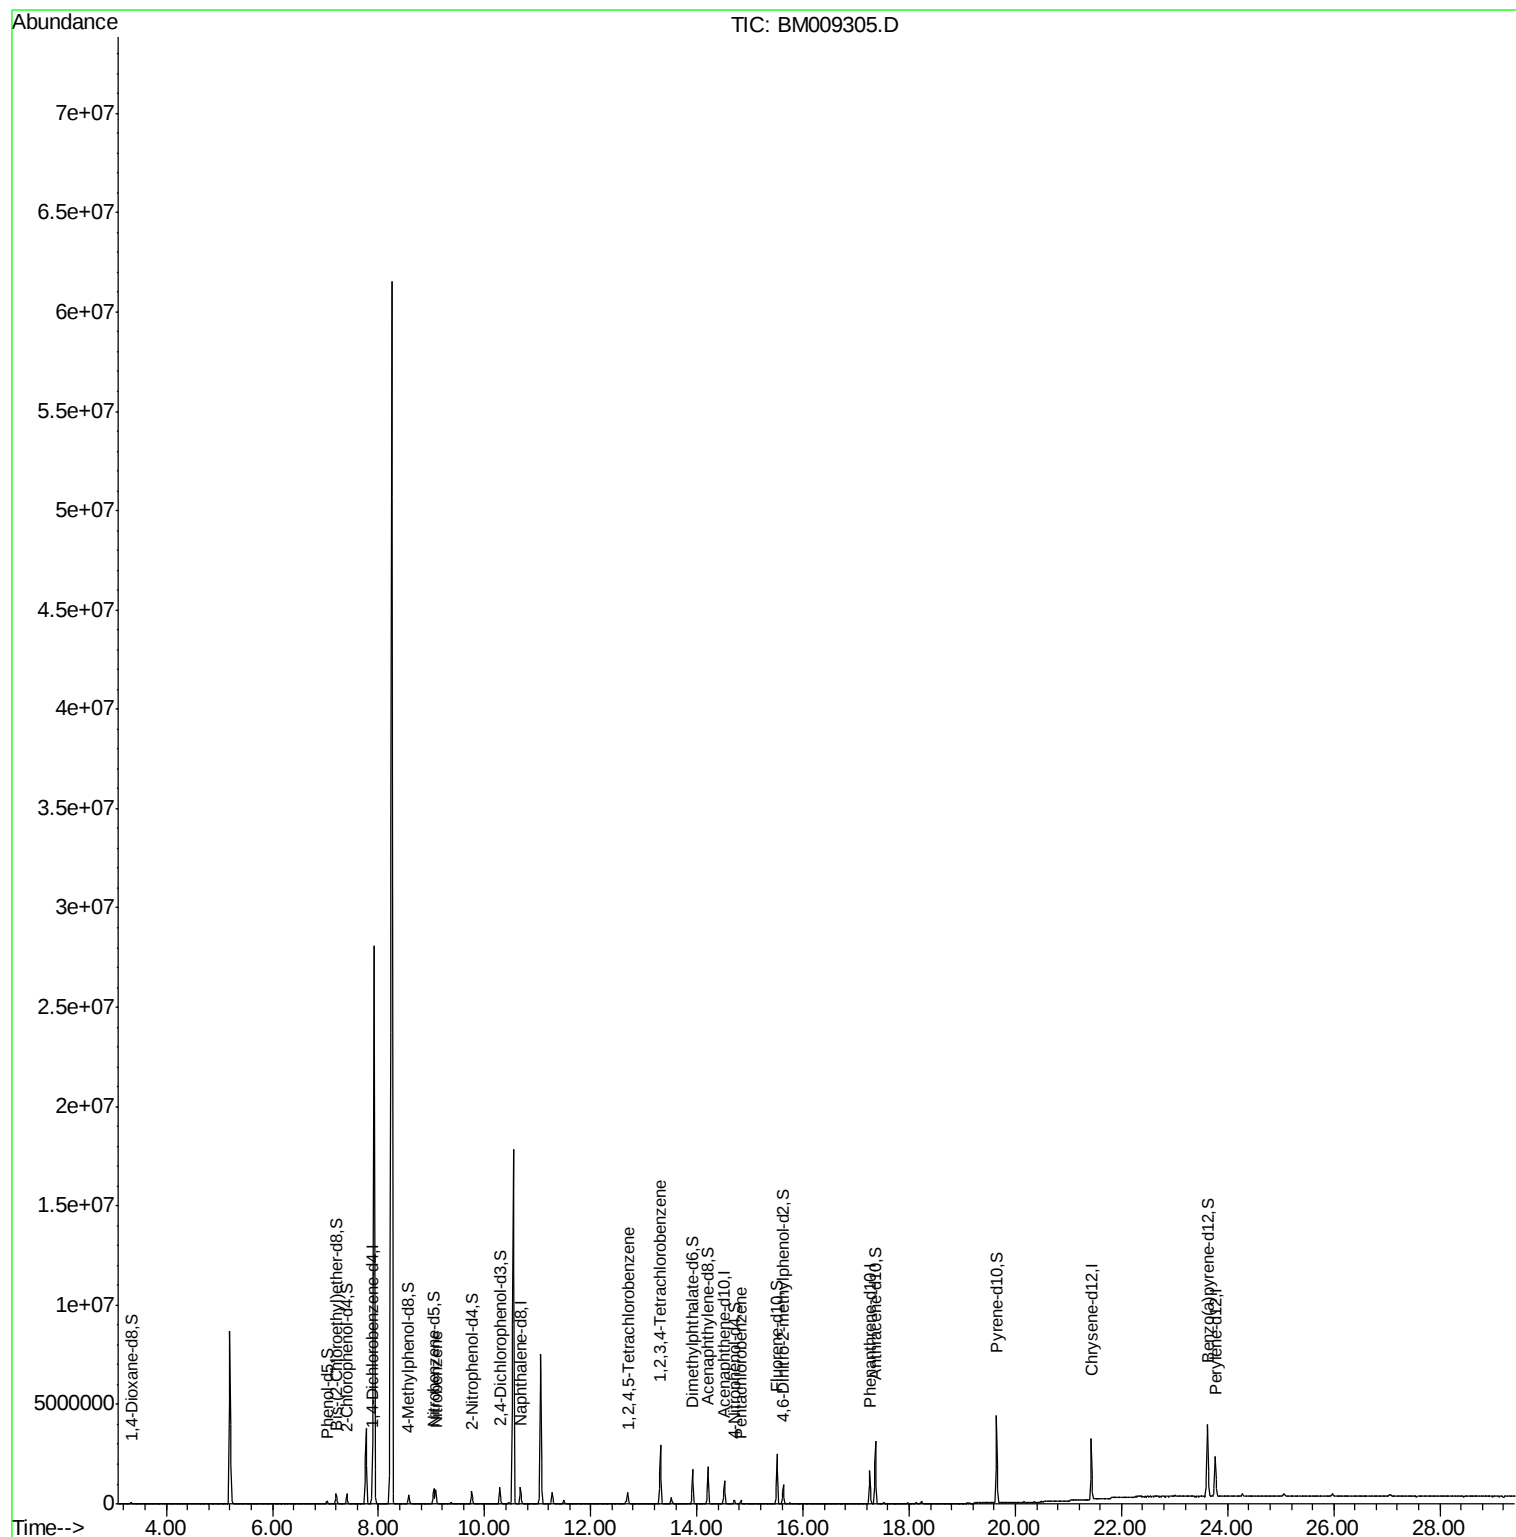

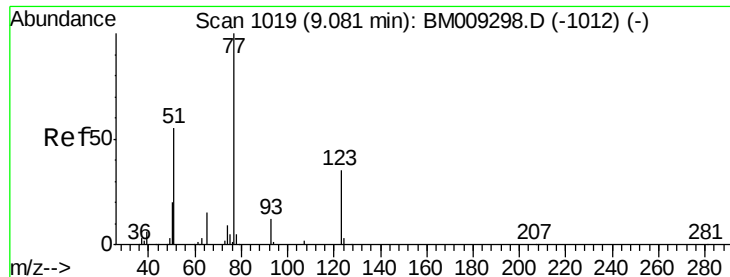

#20

Nitrobenzene

Concen: 29.25 ng/ul

RT: 9.08 min Scan# 1019

Delta R.T. -0.00 min

Lab File: BM009305.D

Acq: 20 Mar 2017 21:11

Instrument :

BNA_M

ClientSampleId :

C0BH7


Tgt Ion: 77 Resp: 376947

Ion Ratio Lower Upper

77 100

123 35.6 39.0 58.4#




65 15.3 10.4 15.6

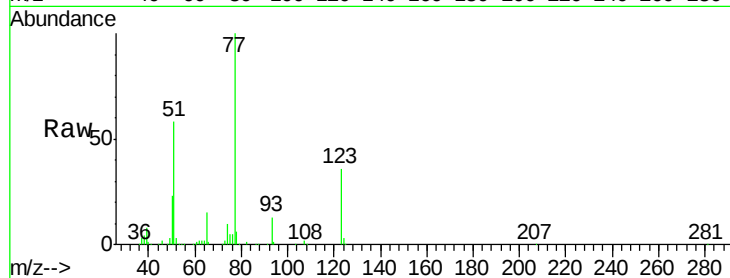

Abundance Ion 77.00 (76.70 to 77.70): BM009305.D (-985) (-)

Ion 123.00 (122.70 to 123.70): BM009305.D (-985) (-)

Ion 65.00 (64.70 to 65.70): BM009305.D (-985) (-)

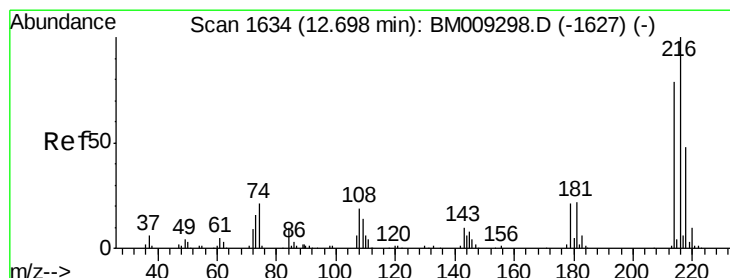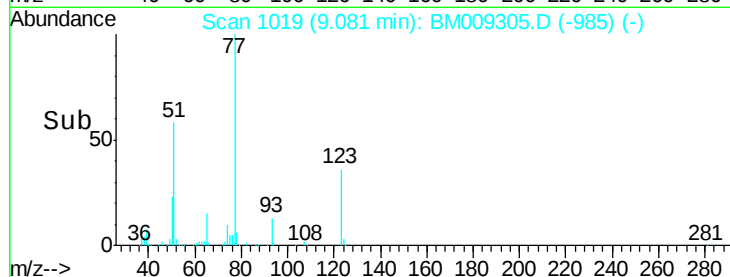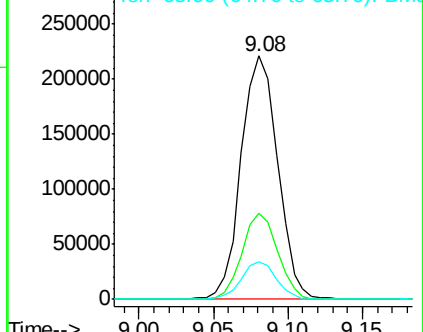

#36

1,2,4,5-Tetrachlorobenzene

Concen: 15.74 ng/ul

RT: 12.70 min Scan# 1634

Delta R.T. -0.00 min

Lab File: BM009305.D

Acq: 20 Mar 2017 21:11

Tgt Ion: 216 Resp: 167575


Ion Ratio Lower Upper

216 100

214 73.4 62.5 93.7

179 22.6 18.2 27.2

108 17.7 14.2 21.2


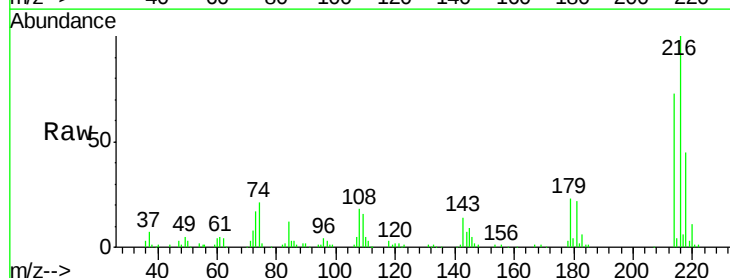



Abundance Ion 216.00 (215.70 to 216.70): BM009305.D (-1600) (-)

Ion 214.00 (213.70 to 214.70): BM009305.D (-1600) (-)

Ion 179.00 (178.70 to 179.70): BM009305.D (-1600) (-)

Ion 108.00 (107.70 to 108.70): BM009305.D (-1600) (-)

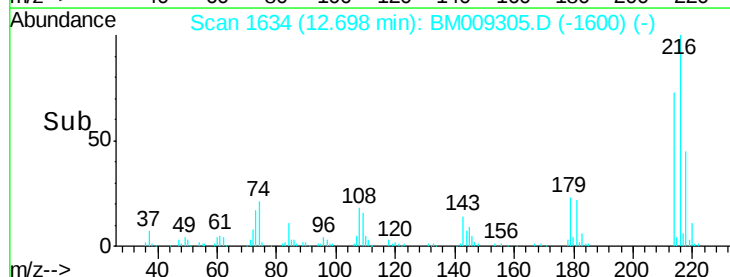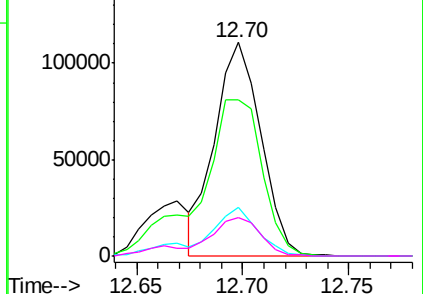

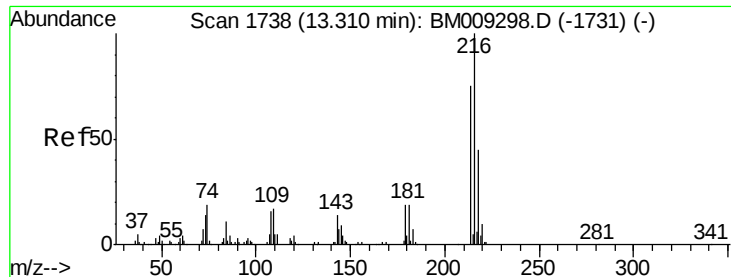

#72

1,2,3,4-Tetrachlorobenzene

Concen: 75.60 ng/uL

RT: 13.31 min Scan# 1738

Delta R.T. -0.00 min

Lab File: BM009305.D

Acq: 20 Mar 2017 21:11

Instrument :

BNA_M

ClientSampleId :

C0BH7


Tgt Ion:216 Resp: 821392

Ion Ratio Lower Upper

216 100

214 77.8 62.5 93.7




218 48.8 38.4 57.6

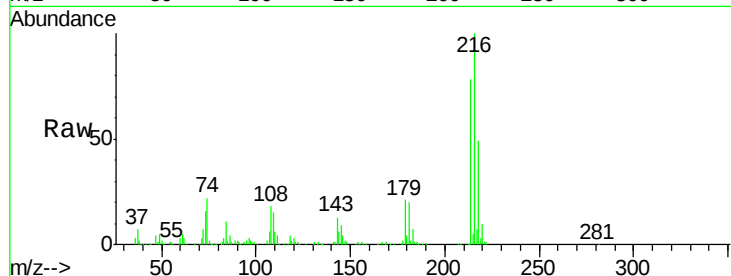

Abundance Ion 216.00 (215.70 to 216.70): E

Ion 214.00 (213.70 to 214.70): E

Ion 218.00 (217.70 to 218.70): E

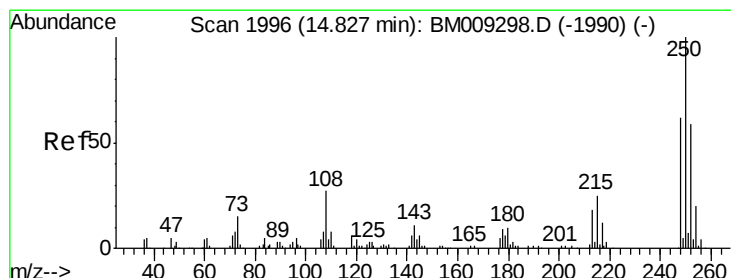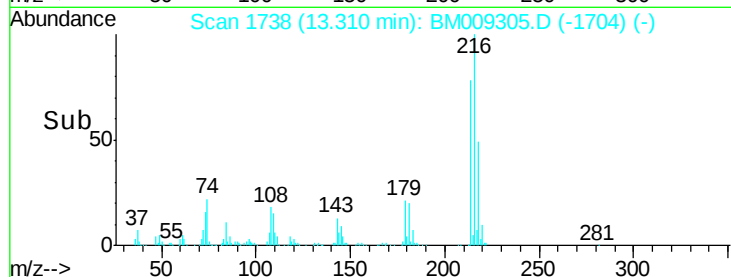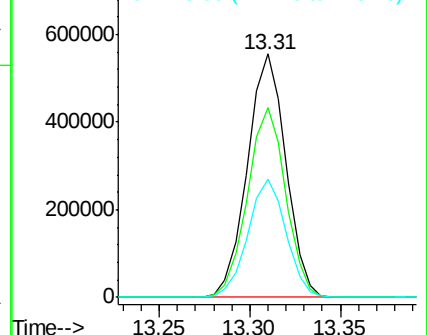

#73

Pentachlorobenzene

Concen: 3.50 ng/uL

RT: 14.83 min Scan# 1996

Delta R.T. -0.00 min

Lab File: BM009305.D

Acq: 20 Mar 2017 21:11


Tgt Ion:250 Resp: 40859

Ion Ratio Lower Upper

250 100

248 62.5 50.6 75.8

252 61.6 51.4 77.0

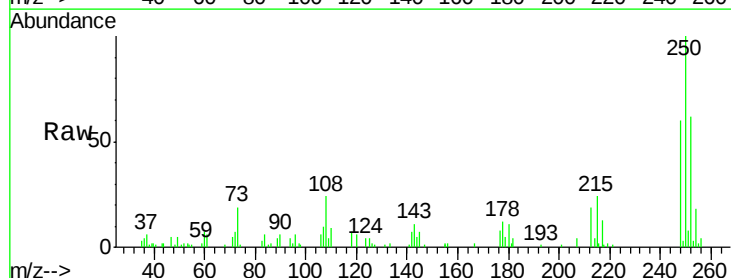

Abundance Ion 250.00 (249.70 to 250.70): E

Ion 248.00 (247.70 to 248.70): E

Ion 252.00 (251.70 to 252.70): E

