


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032115\
 Data File : BM000744.D
 Acq On : 20 Mar 2015 17:52
 Operator : TP/IZ
 Sample : DFTPP42
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP42

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM032115.M
 Title : SVOA CALIBRATION
 Last Update : Sat Mar 21 02:15:30 2015

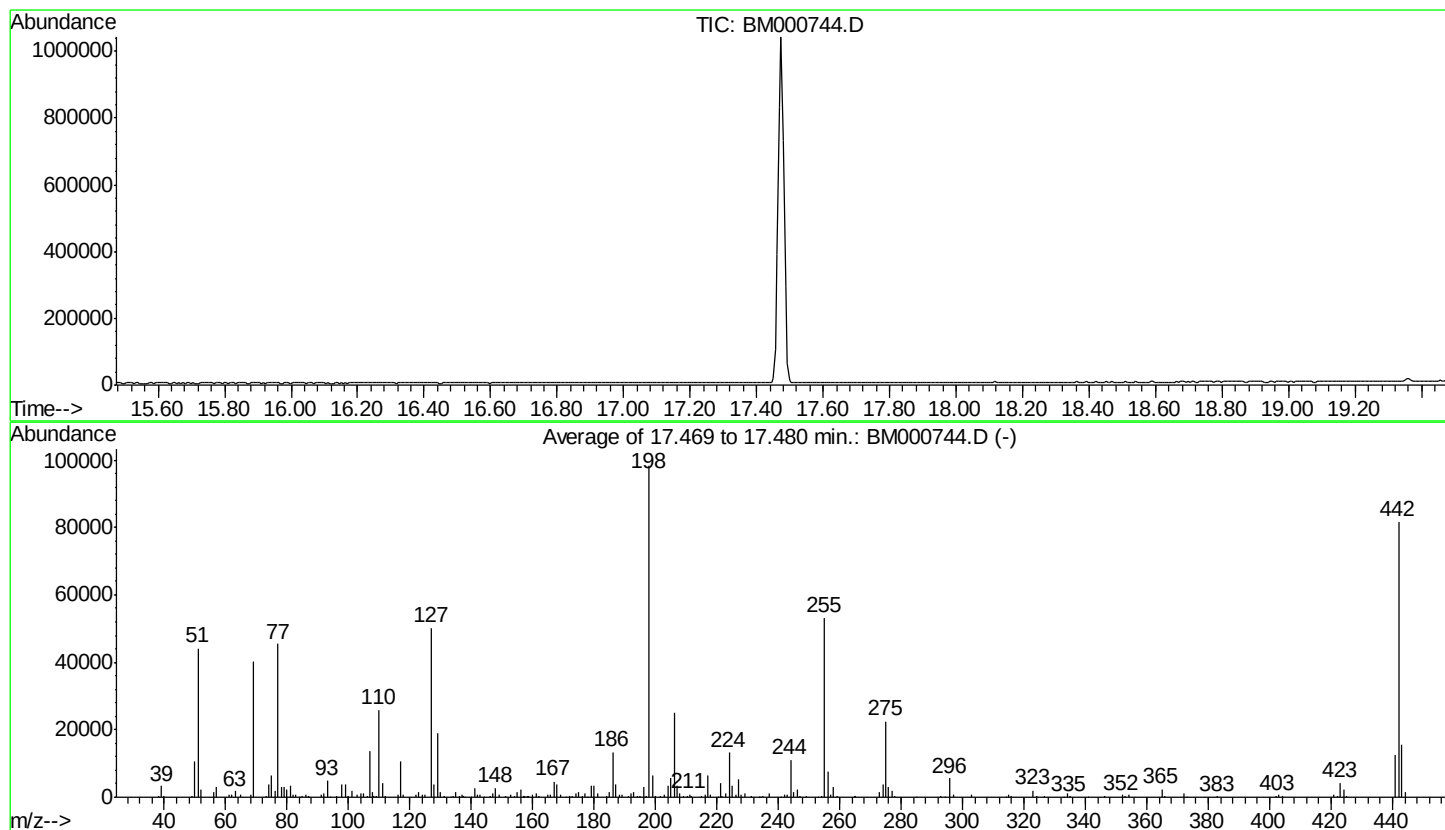

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	44210	PASS
68	69	0.00	2	1.6	635	PASS
69	198	0.00	100	40.7	40064	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.1	50264	PASS
197	198	0.00	2	0.5	490	PASS
198	198	100	100	100.0	98328	PASS
199	198	5	9	6.7	6553	PASS
275	198	10	60	22.9	22549	PASS
365	198	1	100	2.4	2382	PASS
441	443	0.01	100	80.2	12506	PASS
442	198	50	100	83.0	81648	PASS
443	442	15	24	19.1	15586	PASS