


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032115\
 Data File : BM000744.D
 Acq On : 20 Mar 2015 17:52
 Operator : TP/IZ
 Sample : DFTPP42
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP42

Integration File: LSCINT.P

Method : Z:\HPCHEM1\BNA_M\METHODS\SOM02.2-EPA-BM032115.M
 Title : SVOA CALIBRATION
 Last Update : Mon Mar 23 13:57:52 2015

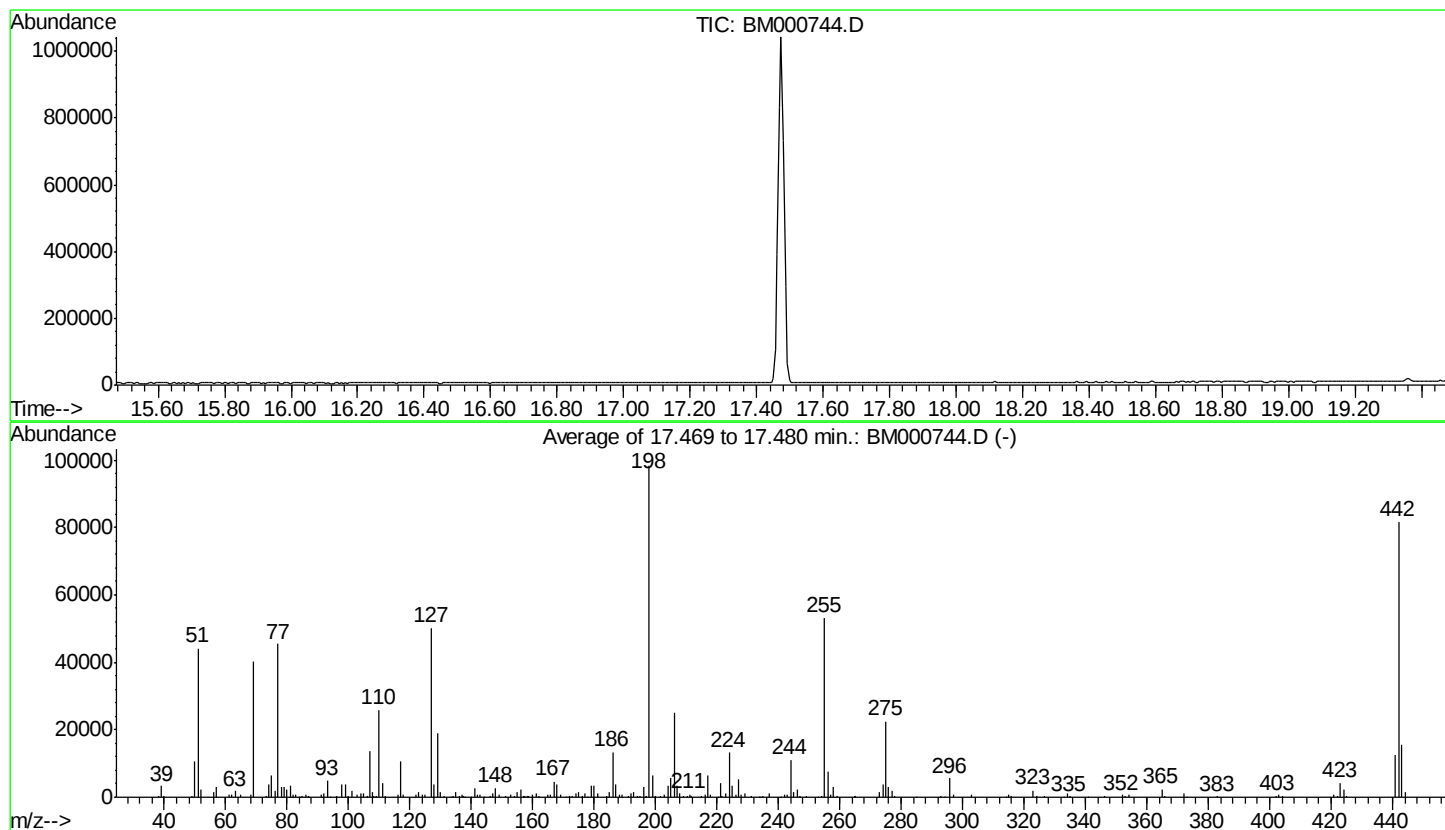

AutoFind: Scans 2513, 2514, 2515; Background Corrected with Scan 2507

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	45.0	44210	PASS
68	69	0.00	2	1.6	635	PASS
69	198	0.00	100	40.7	40064	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	51.1	50264	PASS
197	198	0.00	2	0.5	490	PASS
198	198	100	100	100.0	98328	PASS
199	198	5	9	6.7	6553	PASS
275	198	10	60	22.9	22549	PASS
365	198	1	100	2.4	2382	PASS
441	443	0.01	100	80.2	12506	PASS
442	198	50	100	83.0	81648	PASS
443	442	15	24	19.1	15586	PASS

m/z	Abundance
38.00	509.0
39.10	3828.0
40.00	2034.0
44.00	3763.0
49.00	751.0
50.10	11563.0
51.00	49024.0
52.10	2504.0
56.00	1774.0
57.00	3623.0
61.00	800.0
62.00	886.0
63.00	2057.0
65.10	1073.0
68.00	634.0
69.00	43600.0
73.00	923.0
74.00	3822.0
75.10	7020.0
76.00	2404.0
77.10	49904.0
78.10	3583.0
79.00	3238.0
80.00	2567.0
81.00	3438.0
82.00	862.0
82.90	942.0
85.00	570.0
86.00	995.0
86.90	475.0
91.00	836.0
91.90	1271.0
93.10	4827.0
96.00	495.0
98.00	3845.0
99.00	4255.0
101.00	1918.0
102.80	585.0
103.90	1236.0
105.00	1045.0
106.00	373.0
107.00	14480.0
107.90	1909.0
109.10	382.0
110.00	25720.0
111.00	4536.0
112.00	508.0
115.90	733.0
117.00	10805.0
117.90	1065.0
122.00	752.0
123.00	2042.0
124.00	572.0
124.80	608.0
127.00	52272.0
128.00	3785.0
129.00	18744.0
129.90	1556.0
131.10	385.0
133.90	330.0
135.00	1586.0
135.90	584.0
137.00	1063.0
137.90	388.0
139.90	307.0
141.00	2455.0
142.00	985.0
142.90	480.0
144.10	332.0
145.90	450.0
146.90	1341.0
148.00	2593.0
148.90	603.0
151.00	453.0
152.90	799.0
153.90	560.0
155.00	1361.0
156.00	2113.0
156.80	608.0
157.30	348.0
158.00	582.0
158.80	334.0
160.00	631.0
161.00	1293.0
162.00	408.0
165.00	443.0
166.00	648.0
167.00	4726.0
168.00	4706.0
169.10	829.0
171.90	418.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

172.90	611.0
174.00	945.0
175.10	1675.0
176.00	480.0
177.00	1085.0
179.00	3299.0
180.00	3814.0
181.00	1068.0
183.90	333.0
184.90	1500.0
186.10	12243.0
187.00	4022.0
188.00	602.0
189.00	786.0
191.00	469.0
192.00	987.0
193.10	1586.0
194.00	359.0
196.10	2496.0
197.00	603.0
198.00	93088.0
199.00	6532.0
200.00	381.0
201.50	801.0
202.90	663.0
204.00	3415.0
205.10	5353.0
206.00	24120.0
207.00	4269.0
208.00	844.0
209.00	488.0
210.30	411.0
211.10	789.0
211.80	330.0
216.00	512.0
217.00	6017.0
218.10	774.0
221.00	3676.0
223.00	1406.0
224.10	12474.0
225.10	3310.0
226.00	828.0
227.00	4877.0
228.00	681.0
229.00	1036.0
231.00	425.0
237.00	822.0
240.90	437.0
242.00	663.0
242.90	605.0
244.00	9585.0
245.00	1470.0
246.00	2242.0
247.00	539.0
248.90	593.0
255.00	48904.0
256.00	7155.0
257.00	688.0
258.00	2703.0
259.10	474.0
264.90	901.0
272.90	1332.0
274.00	2874.0
275.00	19568.0
276.00	2681.0
277.00	1465.0
277.90	330.0
292.90	695.0
296.00	4642.0
297.00	849.0
303.10	854.0
314.90	436.0
315.90	477.0
323.00	1756.0
324.10	324.0
326.80	349.0
333.00	312.0
334.10	1121.0
346.00	392.0
351.90	619.0
353.00	336.0
354.10	713.0
364.90	2049.0
365.90	305.0
372.00	964.0
403.00	734.0
404.00	438.0
421.00	615.0
422.00	332.0
423.00	2951.0
424.00	1965.0
441.00	9167.0
442.00	57808.0
443.00	11688.0
444.10	1083.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

m/z	Abundance
38.00	704.0
39.00	4228.0
40.00	2022.0
44.00	3806.0
48.90	483.0
50.00	11943.0
51.10	52536.0
52.00	2773.0
56.00	1671.0
57.00	3673.0
61.00	547.0
62.10	719.0
63.00	2069.0
65.00	1132.0
68.00	795.0
69.00	47616.0
73.00	856.0
74.10	4306.0
75.00	7610.0
76.00	2167.0
77.10	53312.0
78.10	4064.0
79.00	3978.0
80.00	2888.0
81.00	4385.0
82.00	1004.0
83.00	1035.0
85.00	643.0
86.00	1109.0
86.90	640.0
91.00	970.0
92.00	1259.0
93.00	5808.0
94.00	431.0
96.00	527.0
98.00	4595.0
98.90	4528.0
100.10	333.0
101.10	2114.0
102.90	939.0
103.90	1161.0
105.10	1376.0
106.00	524.0
107.00	16281.0
107.90	2302.0
109.00	388.0
110.00	31744.0
111.00	4487.0
112.00	668.0
116.00	932.0
117.00	12494.0
117.90	1135.0
121.90	1002.0
123.00	1552.0
123.90	743.0
124.90	840.0
127.00	62160.0
128.00	5207.0
129.00	23304.0
130.00	1778.0
131.00	481.0
133.90	773.0
135.10	1640.0
136.00	565.0
137.20	1058.0
141.00	2782.0
142.00	1004.0
143.00	870.0
146.00	450.0
147.00	1542.0
148.00	3216.0
149.00	827.0
151.10	357.0
153.00	911.0
153.90	668.0
154.90	1649.0
156.00	2593.0
156.80	520.0
157.20	459.0
158.10	583.0
158.90	424.0
160.10	866.0
161.00	1307.0
162.00	426.0
164.90	1080.0
166.00	799.0
167.00	5449.0
168.00	4605.0
169.00	760.0
170.80	312.0
172.00	457.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

173.00	641.0
174.00	1259.0
175.10	2066.0
175.90	538.0
177.00	1086.0
178.00	342.0
179.00	3867.0
180.00	4117.0
181.00	1294.0
183.90	406.0
184.90	1763.0
186.00	16196.0
187.00	4838.0
188.10	785.0
189.00	902.0
190.90	603.0
192.00	1236.0
193.00	1577.0
193.90	503.0
196.00	3201.0
197.00	521.0
198.00	120000.0
199.00	7953.0
199.90	470.0
201.40	622.0
203.00	717.0
204.00	3492.0
205.00	7055.0
206.00	30552.0
207.10	5572.0
208.00	1315.0
209.10	384.0
210.10	474.0
211.10	1193.0
211.80	352.0
214.80	379.0
216.00	810.0
217.00	7526.0
218.00	1038.0
221.00	4785.0
221.70	1501.0
223.00	1562.0
224.10	16035.0
225.00	4245.0
226.10	686.0
227.00	6772.0
228.10	811.0
229.00	1107.0
231.00	596.0
234.10	517.0
234.90	328.0
237.00	1356.0
242.10	1134.0
243.00	761.0
244.00	13660.0
245.00	1862.0
246.00	2632.0
247.00	303.0
249.00	361.0
253.00	347.0
254.10	501.0
255.00	63104.0
256.00	9021.0
257.10	892.0
258.00	3336.0
265.10	1585.0
273.00	1839.0
274.00	4222.0
275.00	27392.0
276.00	3871.0
277.00	2186.0
278.00	537.0
285.10	379.0
293.00	604.0
294.00	398.0
296.00	6871.0
296.90	987.0
303.00	758.0
314.00	383.0
314.90	678.0
323.00	2252.0
324.10	420.0
326.80	495.0
334.00	1469.0
334.90	618.0
341.00	367.0
346.00	530.0
352.00	699.0
353.10	320.0
354.00	1167.0
365.00	2800.0
365.90	375.0
371.90	1247.0
383.00	448.0
401.90	510.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

402.90	549.0
404.00	559.0
421.00	743.0
422.10	591.0
423.00	5687.0
424.00	2874.0
425.10	465.0
441.10	14518.0
442.00	98736.0
443.00	18688.0
444.00	1747.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

m/z	Abundance
39.10	2101.0
40.00	1554.0
44.00	3650.0
49.00	462.0
50.00	7942.0
51.00	31072.0
52.00	1697.0
56.00	891.0
57.00	2420.0
61.00	477.0
61.90	493.0
63.10	1223.0
64.90	578.0
68.10	476.0
69.00	28976.0
73.10	578.0
74.00	3054.0
75.00	4932.0
76.00	1440.0
77.10	33120.0
78.10	2065.0
79.00	2295.0
79.90	1762.0
81.00	2408.0
82.00	831.0
83.00	512.0
84.00	331.0
85.10	418.0
86.00	503.0
87.10	491.0
91.00	477.0
92.00	723.0
93.00	3828.0
98.00	2577.0
99.00	2809.0
100.00	312.0
101.00	1442.0
103.00	637.0
103.80	1157.0
104.90	1032.0
107.00	10357.0
108.10	1731.0
110.00	20384.0
111.10	3115.0
111.90	555.0
116.00	416.0
117.00	8114.0
117.90	660.0
122.00	877.0
123.00	1256.0
124.00	613.0
125.00	593.0
127.00	36360.0
128.10	2627.0
129.00	15293.0
129.90	1386.0
131.00	321.0
133.10	306.0
133.90	466.0
135.00	1366.0
136.10	419.0
136.90	698.0
141.00	2277.0
142.00	470.0
143.00	551.0
147.00	1054.0
147.90	2274.0
148.90	671.0
153.00	840.0
154.00	460.0
155.00	1265.0
156.00	1750.0
157.00	339.0
158.00	472.0
160.00	683.0
161.00	985.0
164.90	804.0
165.80	554.0
167.00	4093.0
168.00	2670.0
169.00	376.0
173.10	406.0
174.00	1137.0
175.00	1385.0
176.10	386.0
177.00	840.0
178.90	2767.0
180.00	2607.0
181.00	1094.0
184.00	309.0
185.00	1428.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

186.00	11471.0
187.00	2898.0
188.00	600.0
189.00	756.0
191.10	359.0
192.00	995.0
193.00	1249.0
194.00	350.0
195.10	685.0
196.00	2984.0
196.70	379.0
197.00	347.0
198.00	81896.0
199.00	5174.0
200.00	438.0
203.10	590.0
204.00	3635.0
205.00	5102.0
206.00	20840.0
207.00	3840.0
208.00	1182.0
209.10	388.0
210.30	397.0
210.90	897.0
214.90	357.0
216.00	560.0
217.00	6062.0
218.10	883.0
220.20	324.0
221.00	3796.0
223.10	1007.0
224.10	10884.0
225.00	3086.0
226.00	432.0
227.00	4488.0
227.90	540.0
229.00	1068.0
231.10	514.0
233.80	359.0
234.90	477.0
237.00	882.0
242.00	646.0
243.10	793.0
244.10	10005.0
245.00	1083.0
246.00	1927.0
248.90	315.0
253.90	333.0
255.00	47552.0
256.00	6904.0
256.90	542.0
258.00	2550.0
259.00	494.0
264.90	807.0
273.00	1292.0
274.10	4126.0
275.00	20688.0
276.00	2570.0
276.90	1643.0
278.00	337.0
293.10	396.0
296.00	5196.0
297.00	699.0
303.00	657.0
314.90	837.0
316.00	541.0
323.10	1981.0
324.00	425.0
326.90	520.0
334.10	1372.0
334.90	383.0
346.10	344.0
352.10	574.0
352.90	512.0
354.00	481.0
365.00	2297.0
365.90	367.0
372.00	949.0
373.00	313.0
382.90	370.0
401.90	525.0
402.80	630.0
420.90	699.0
422.00	622.0
423.00	4414.0
424.00	2381.0
425.10	377.0
441.00	13834.0
442.00	88400.0
443.00	16384.0
444.00	1261.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42

Scan 2507 (17.433 min): BM000744.D
DFTPP42

m/z	Abundance
40.00	1405.0
44.00	4428.0
73.10	446.0
207.00	1260.0

Instrument :
BNA_M
ClientSampleId :
DFTPP42