

Data Path : \\74.0.250.170\SV0ASRV\HPCHEM1\BNA M\DATA\BM032118\
 Data File : BM014643.D
 Acq On : 21 Mar 2018 16:20
 Operator : SJ/JU
 Sample : J1935-12
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 BEEL8

Manual Integrations
 APPROVED

Sohil
 3/22/2018 6:50:30 PM

Quant Time: Mar 22 03:14:43 2018
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM031518-PAH.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Thu Mar 22 01:49:10 2018
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.45	152	136537	20.00	ng/ul	0.00
2) Naphthalene-d8	10.22	136	500598	20.00	ng/ul	0.00
6) Acenaphthene-d10	14.12	164	243827	20.00	ng/ul	0.00
12) Phenanthrene-d10	16.88	188	512287	20.00	ng/ul	0.00
18) Chrysene-d12	21.11	240	417672	20.00	ng/ul	0.00
23) Perylene-d12	23.27	264	369775	20.00	ng/ul	0.00
System Monitoring Compounds						
3) 2,4-Dichlorophenol-d3	9.88	165	161190m	20.83	ng/ul	0.00
7) Acenaphthylene-d8	13.80	160	706552	27.11	ng/ul	0.00
10) Fluorene-d10	15.12	176	438428	25.68	ng/ul	0.00
15) Anthracene-d10	16.99	188	616889	25.15	ng/ul	0.00
19) Pyrene-d10	19.30	212	664640	26.47	ng/ul	0.00
26) Benzo(a)pyrene-d12	23.14	264	469749m	26.26	ng/ul	0.00
Target Compounds						
17) Fluoranthene	18.96	202	61202	1.879	ng/ul#	97
20) Pyrene	19.33	202	52389	1.668	ng/ul#	94

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : \\74.0.250.170\SVOASRV\HPCHEM1\BNA M\DATA\BM032118\
Data File : BM014643.D
Acq On : 21 Mar 2018 16:20
Operator : SJ/JU
Sample : J1935-12
Misc :
ALS Vial : 12 Sample Multiplier: 1


Instrument :
BNA_M
ClientSampleId :
BEEL8

Quant Time: Mar 22 03:14:43 2018
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-BM031518-PAH.M
Quant Title : SVOA CALIBRATION
QLast Update : Thu Mar 22 01:49:10 2018
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
3/22/2018 6:50:30 PM

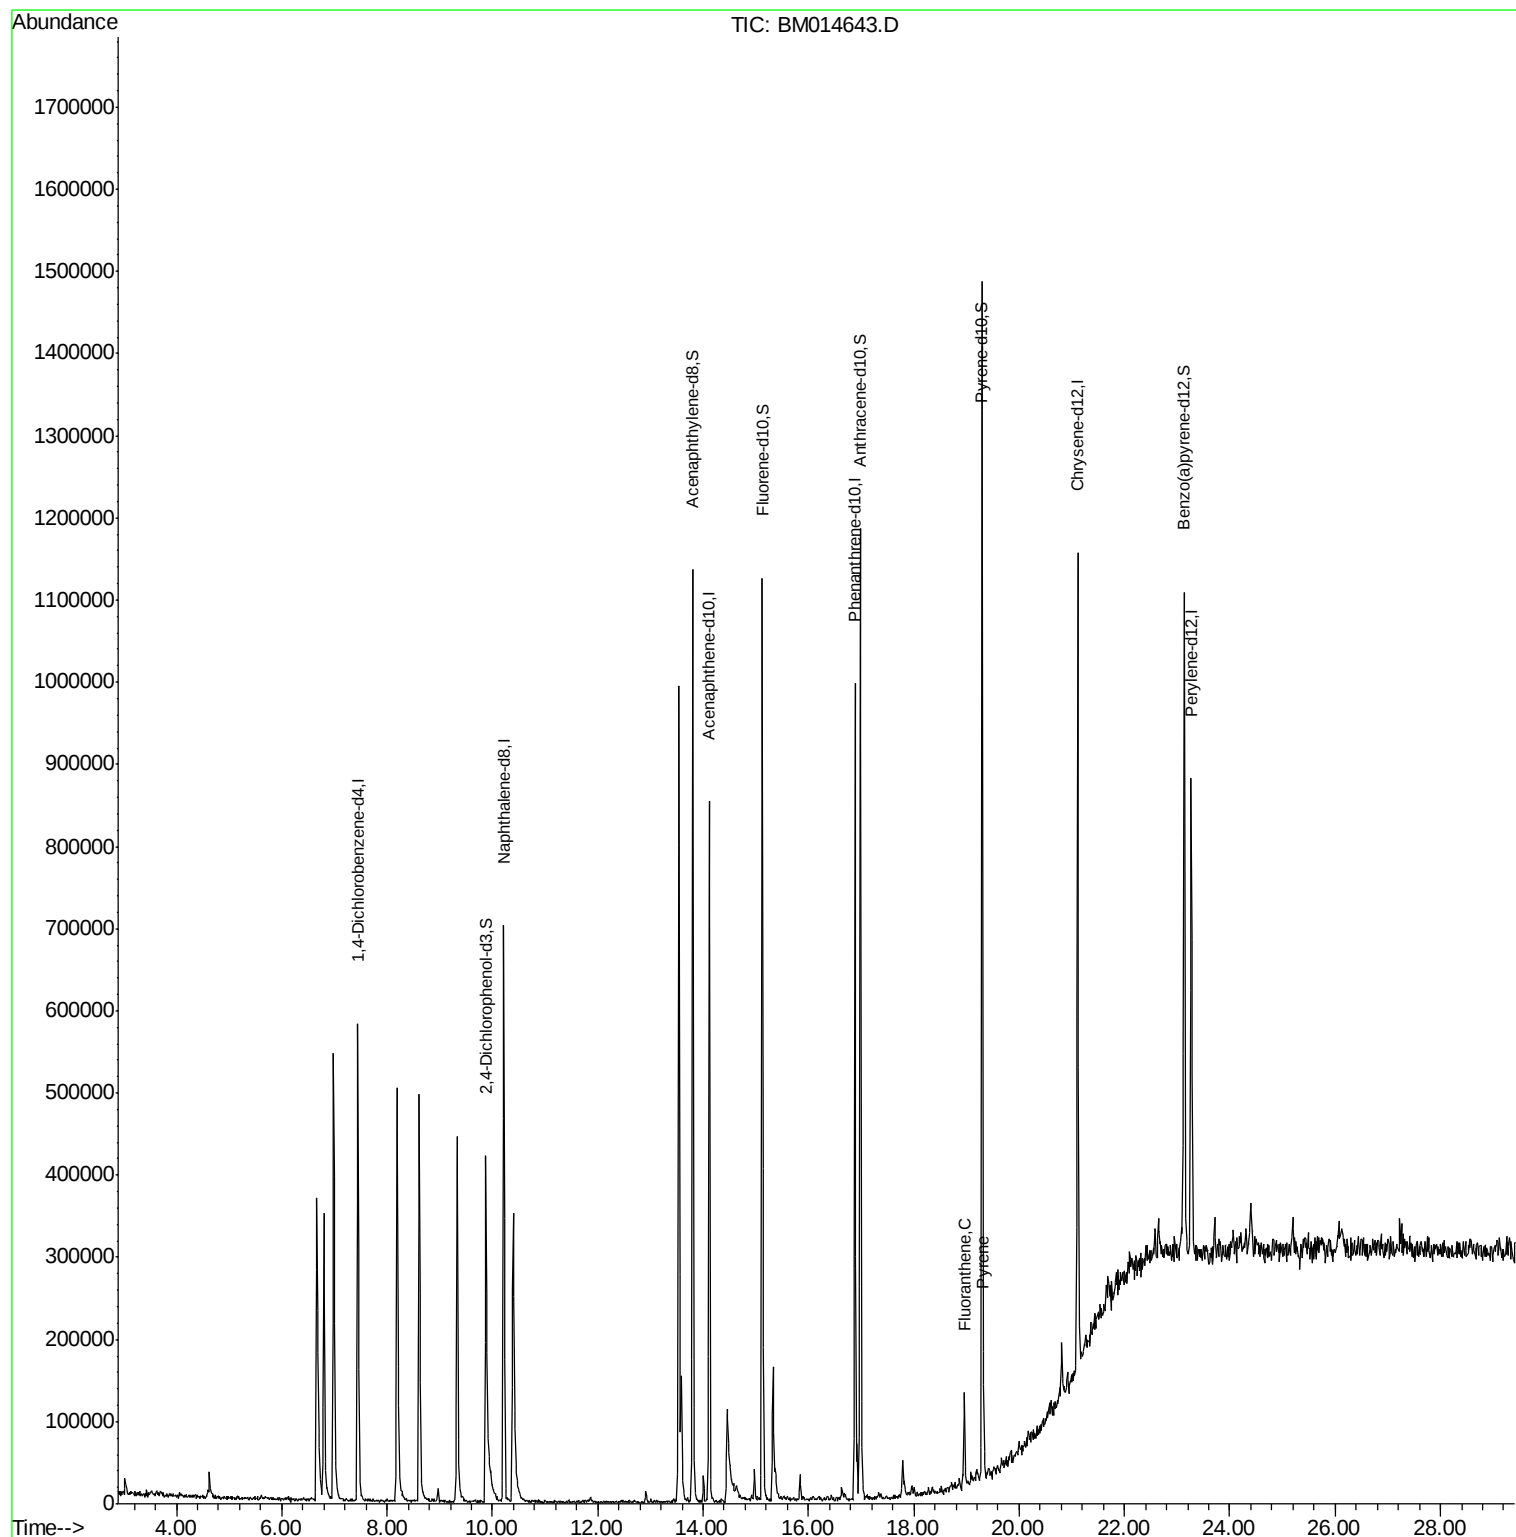

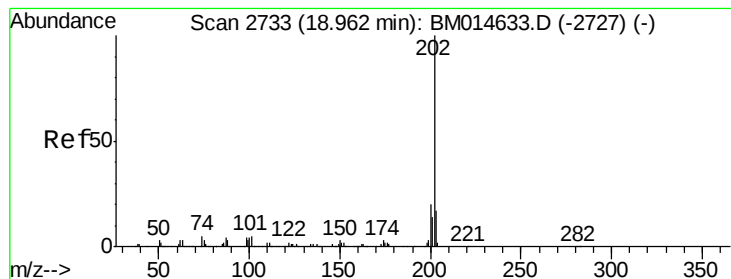

#17

Fluoranthene

Concen: 1.879 ng/ul

RT: 18.96 min Scan# 2733

Delta R.T. 0.00 min

Lab File: BM014643.D

Acq: 21 Mar 2018 16:20

Instrument :

BNA_M





ClientSampleId :

BEEL8

Tot Ion:	202	Resp:	61202
Ion Ratio	Lower	Upper	
202	100		
101	5.3	4.6	7.0
100	6.2	3.4	5.2#

Manual Integrations
APPROVED

Sohil
3/22/2018 6:50:30 PM

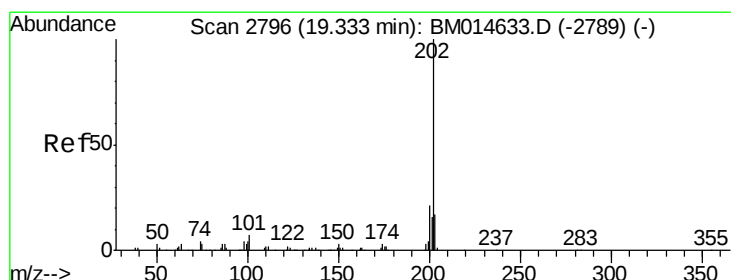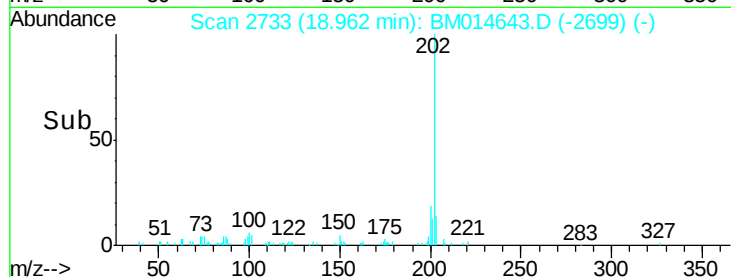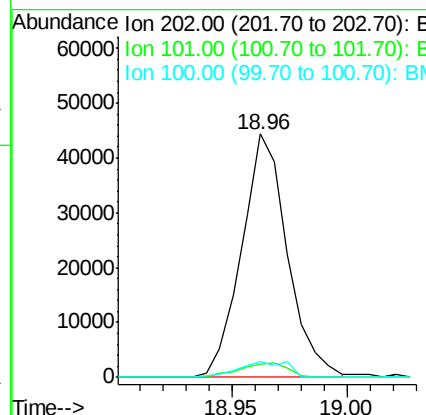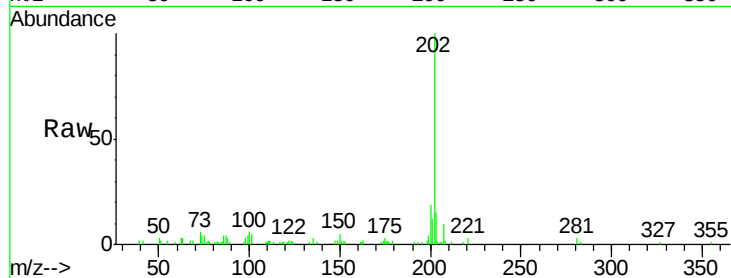

#20

Pyrene

Concen: 1.668 ng/ul

RT: 19.33 min Scan# 2795

Delta R.T. -0.01 min

Lab File: BM014643.D

Acq: 21 Mar 2018 16:20

Tgt Ion:	202	Resp:	52389
Ion Ratio	Lower	Upper	
202	100		
101	8.8	5.1	7.7#
100	7.9	4.9	7.3#

