
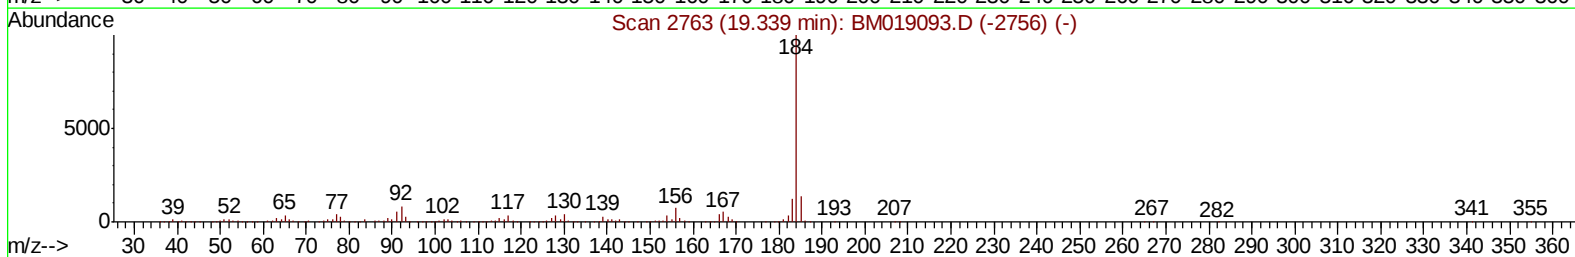
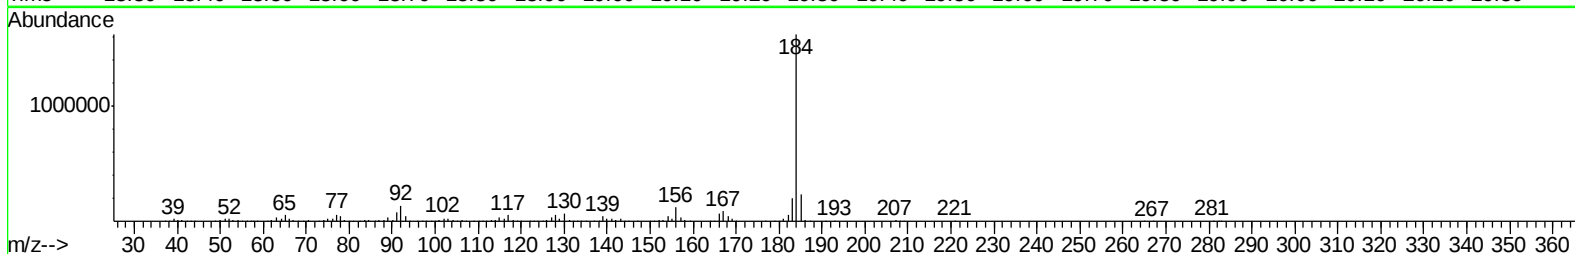


Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032119\
Data File : BM019289.D
Acq On : 21 Mar 2019 14:18
Operator : JU/SJ
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 05:13:05 2019
Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Mon Mar 11 17:30:46 2019
Response via : Initial Calibration

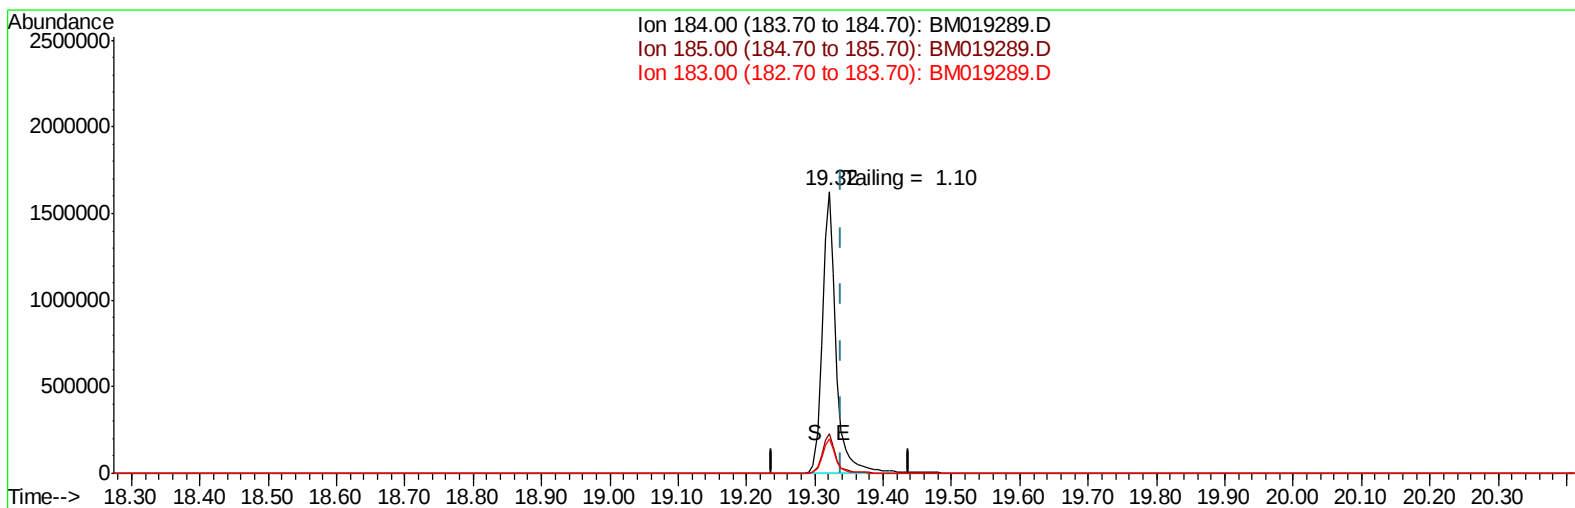

TIC: BM019289.D

(77) Benzidine




19.321min (-0.018) 30884.59ng

response 2292245

Ion	Exp%	Act%
184.00	100	100
185.00	13.70	14.23
183.00	12.20	12.14
0.00	0.00	0.00

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032119\
 Data File : BM019289.D
 Acq On : 21 Mar 2019 14:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 22 05:13:05 2019
 Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Mon Mar 11 17:30:46 2019
 Response via : Initial Calibration

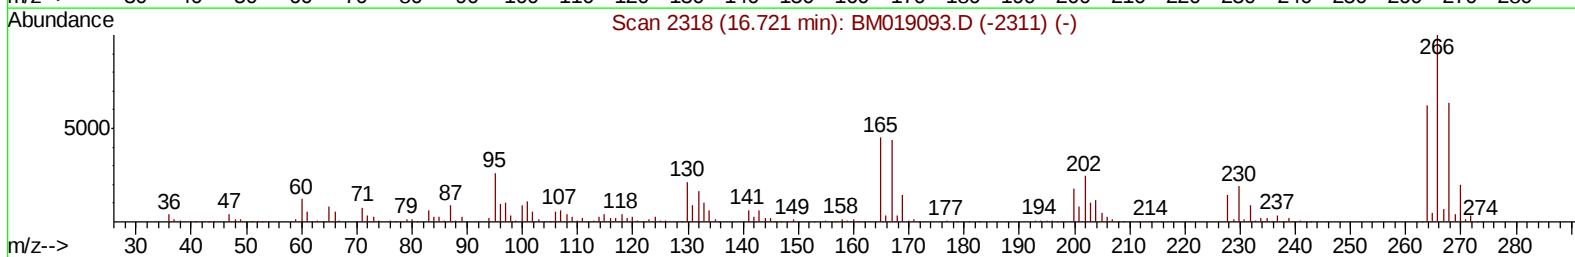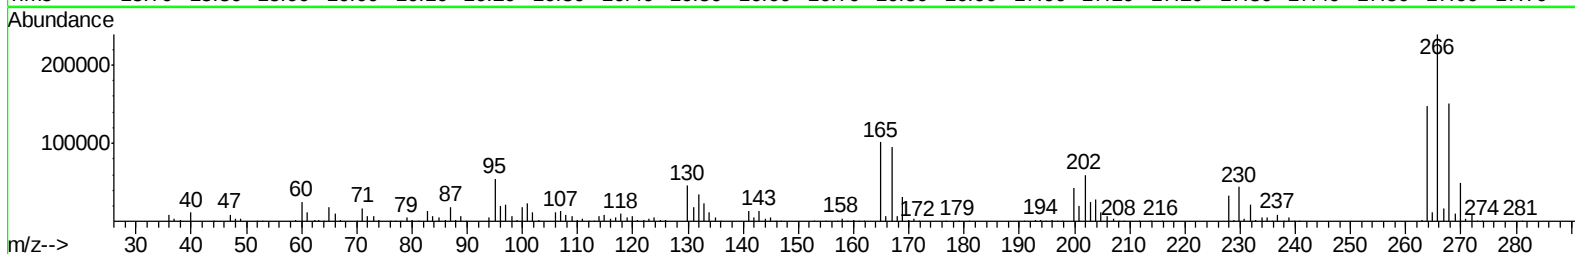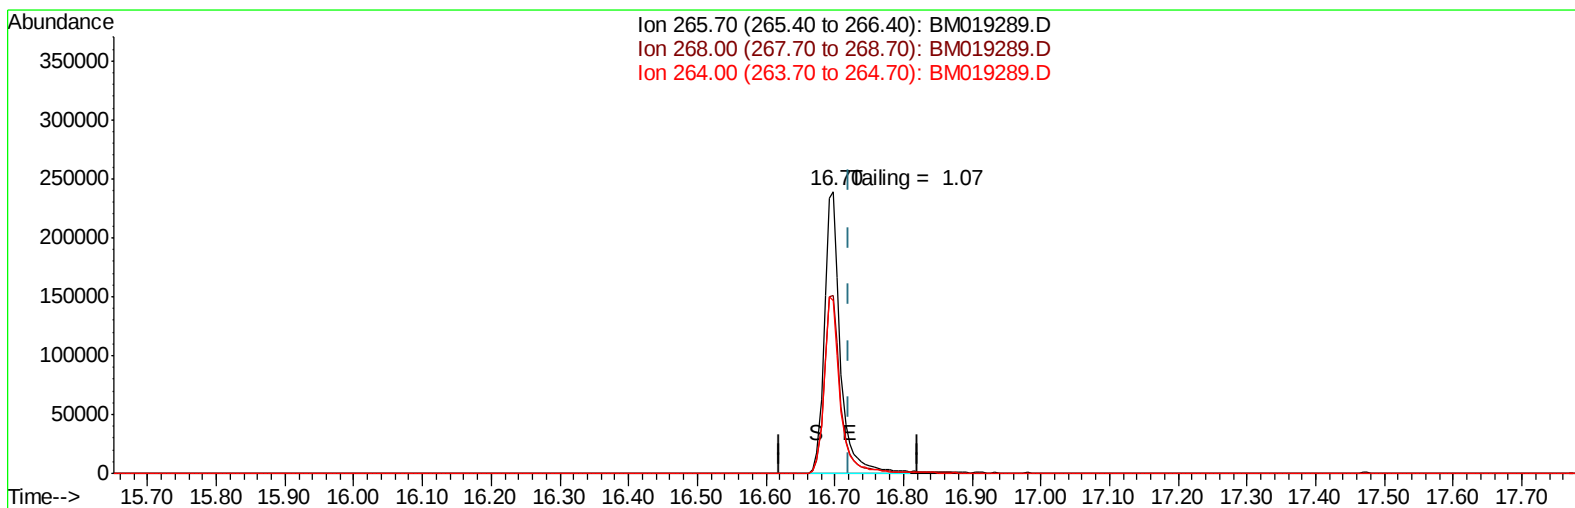

TIC: BM019289.D

(70) Pentachlorophenol (C)

16.698min (-0.024) 342359.38ng

response 386708

Ion	Exp%	Act%
265.70	100	100
268.00	64.10	63.20
264.00	62.50	61.60
0.00	0.00	0.00