

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032119\
 Data File : BM019292.D
 Acq On : 21 Mar 2019 16:06
 Operator : JU/SJ
 Sample : PB118124BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB118124BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	376	382	401	rBV	2756301	4010692	44.83%	8.212%
2	6.816	644	651	670	rBV	2363803	3891826	43.50%	7.968%
3	7.163	703	710	726	rBV	2789106	4344044	48.55%	8.894%
4	7.628	783	789	801	rVB	619051	952820	10.65%	1.951%
5	7.946	836	843	856	rBV	2057203	3218821	35.98%	6.591%
6	8.798	980	988	1006	rBV	1439885	2529785	28.27%	5.180%
7	10.416	1256	1263	1283	rBV	708065	1353315	15.13%	2.771%
8	12.898	1678	1685	1697	rBV	4861210	6985126	78.07%	14.302%
9	14.286	1915	1921	1933	rBV2	1197447	1964638	21.96%	4.023%
10	15.786	2170	2176	2197	rBV	2975922	4592189	51.33%	9.402%
11	17.045	2383	2390	2399	rBV	1415075	2176135	24.32%	4.456%
12	19.686	2833	2839	2855	rBV	7095558	8947168	100.00%	18.319%
13	21.245	3099	3104	3115	rBV2	1381630	2047876	22.89%	4.193%
14	23.474	3477	3483	3494	rBV	906581	1825852	20.41%	3.738%


Sum of corrected areas: 48840287

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032119\
Data File : BM019292.D
Acq On : 21 Mar 2019 16:06
Operator : JU/SJ
Sample : PB118124BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118124BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

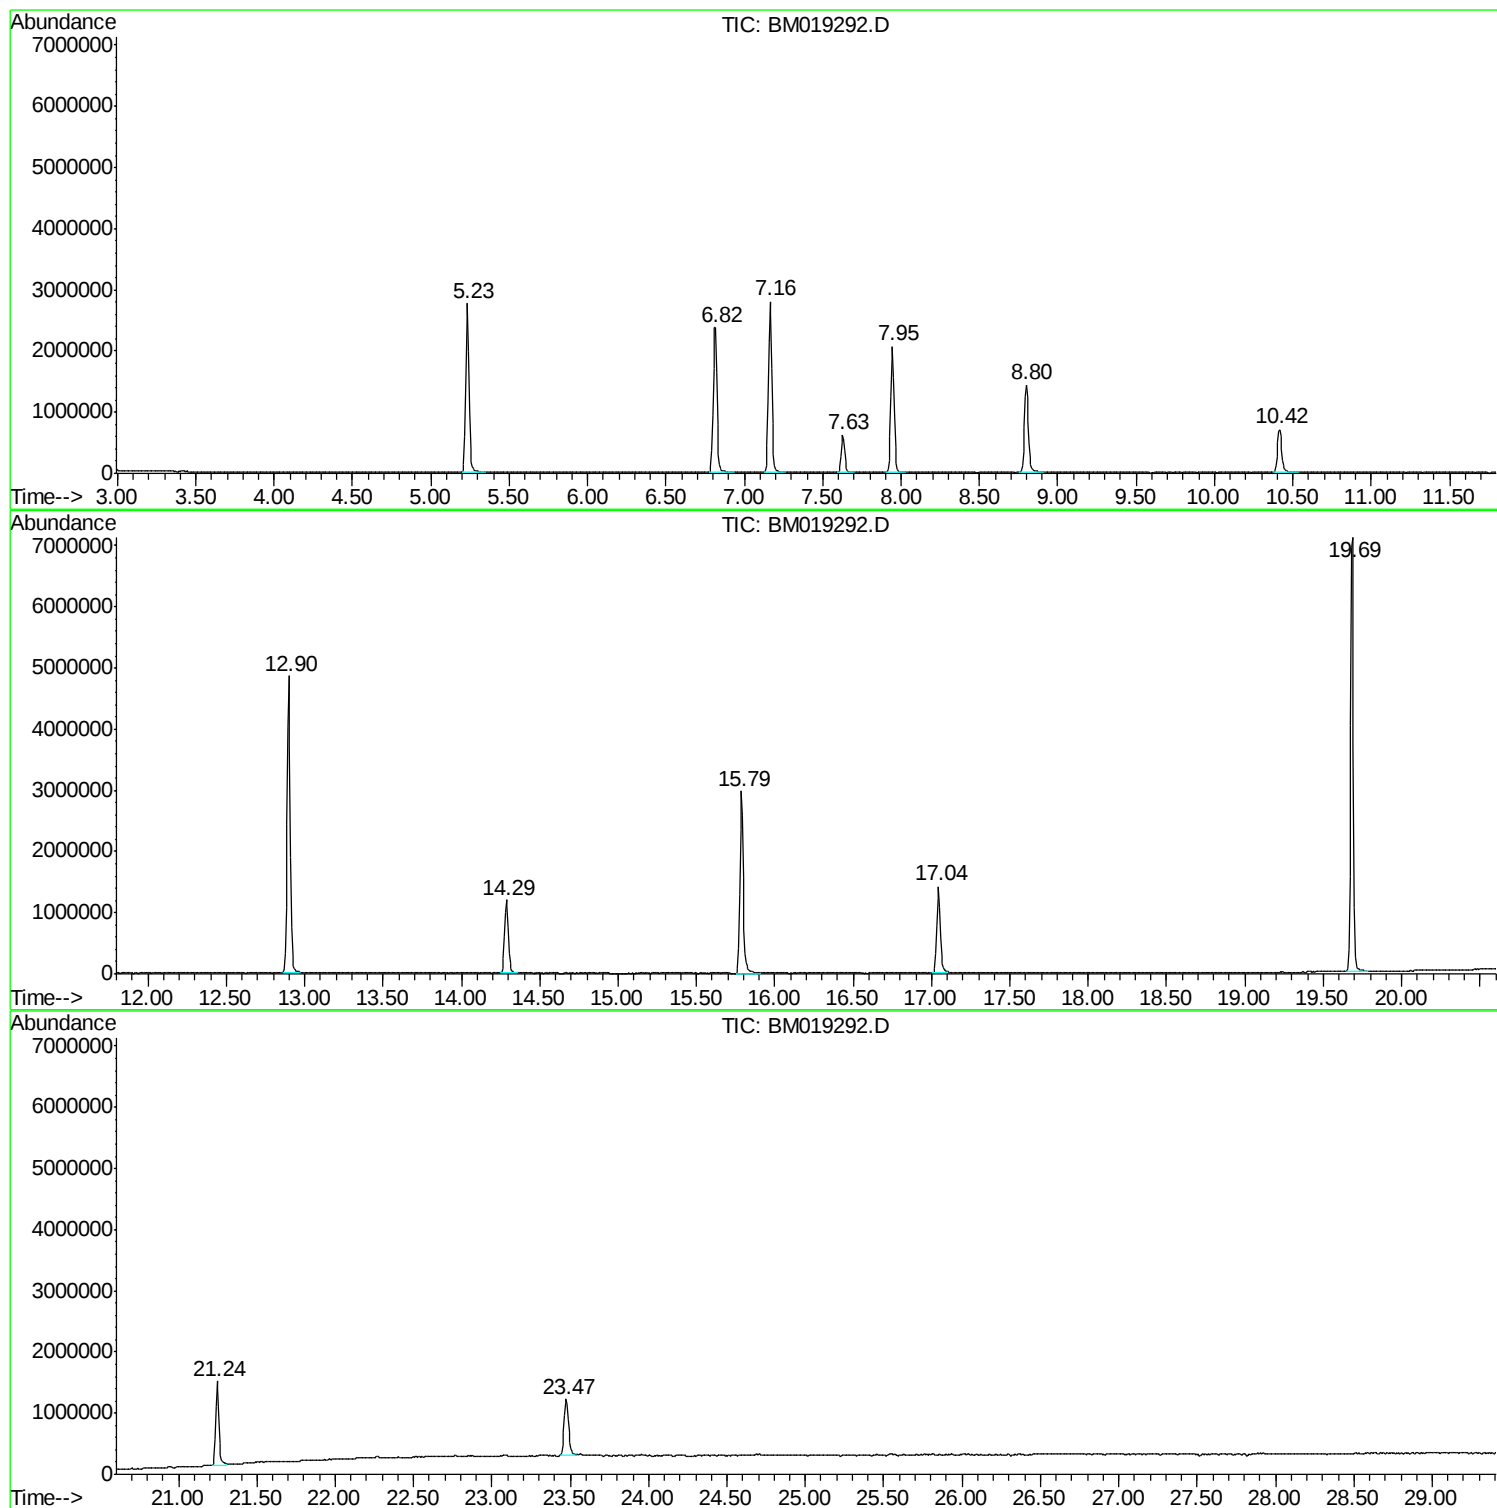

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032119\
Data File : BM019292.D
Acq On : 21 Mar 2019 16:06
Operator : JU/SJ
Sample : PB118124BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118124BL










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.16 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.16	91.18 ng	4344040	1,4-Dichlorobenzene-d4	7.63

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	5-Aminoindole	132	C8H8N2	005192-03-0	12
2		Benzene, 1,2,4-trifluoro-	132	C6H3F3	000367-23-7	9
3		Benzene, 1,3,5-trifluoro-	132	C6H3F3	000372-38-3	9
4		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9
5		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9

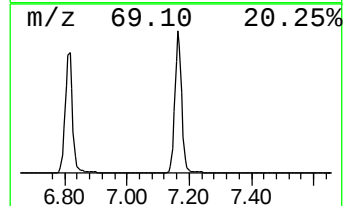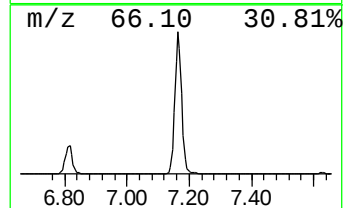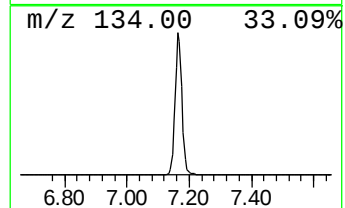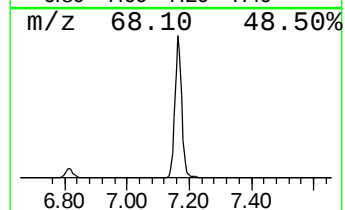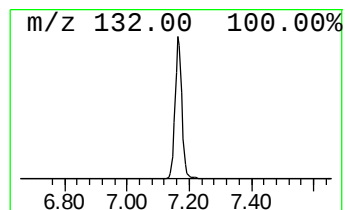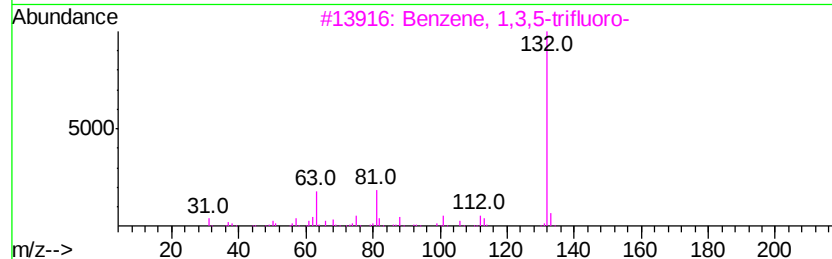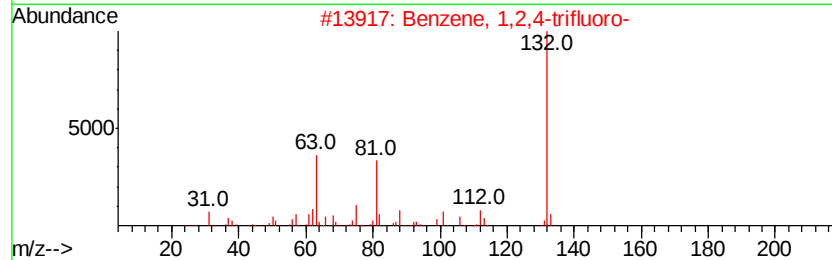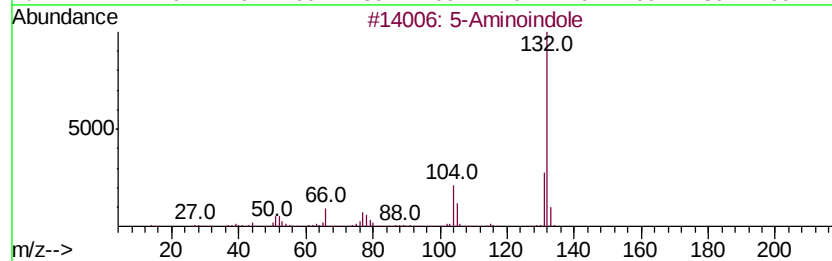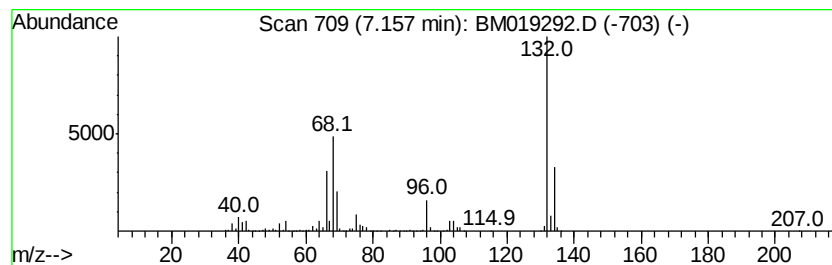

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032119\
Data File : BM019292.D
Acq On : 21 Mar 2019 16:06
Operator : JU/SJ
Sample : PB118124BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB118124BL

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.16	7.16	91.2	ng	4344040	1	7.63	952820	20.0