

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032119\
 Data File : BM019298.D
 Acq On : 21 Mar 2019 19:44
 Operator : JU/SJ
 Sample : K2003-01
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 S4A(5-30)COMP

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON
 Sampling : 1
 Start Thrs: 0.2
 Stop Thrs : 0
 Filtering: 5
 Min Area: 3 % of largest Peak
 Max Peaks: 100
 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.234	375	382	397	rBV	3111347	4486164	40.17%	7.246%
2	6.816	643	651	668	rBV	3328251	5345935	47.87%	8.634%
3	7.163	703	710	730	rBV	3349837	5308092	47.53%	8.573%
4	7.628	782	789	799	rBV	546409	857863	7.68%	1.386%
5	7.945	835	843	855	rBV	2296358	3570211	31.97%	5.766%
6	8.798	981	988	1001	rBV	1799322	3013277	26.98%	4.867%
7	10.416	1255	1263	1281	rBV	781816	1424784	12.76%	2.301%
8	12.898	1678	1685	1700	rBV	6015306	8694764	77.85%	14.043%
9	13.757	1825	1831	1844	rBV	282444	480371	4.30%	0.776%
10	14.286	1914	1921	1936	rBV2	1452933	2282385	20.44%	3.686%
11	15.786	2170	2176	2194	rBV	4692890	6745476	60.40%	10.895%
12	17.045	2383	2390	2396	rBV2	1872421	2722619	24.38%	4.397%
13	17.933	2536	2541	2552	rBV3	83321	180691	1.62%	0.292%
14	19.115	2737	2742	2747	rVB	115217	158119	1.42%	0.255%
15	19.480	2800	2804	2809	rVB	93099	126999	1.14%	0.205%
16	19.686	2833	2839	2849	rBV	9334281	11167950	100.00%	18.037%
17	20.950	3050	3054	3067	rBV2	218392	501014	4.49%	0.809%
18	21.244	3099	3104	3110	rBV	1852702	2587287	23.17%	4.179%
19	22.268	3275	3278	3282	rVB	93845	113679	1.02%	0.184%
20	23.474	3477	3483	3496	rVB	1155372	2147663	19.23%	3.469%


Sum of corrected areas: 61915343

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032119\
Data File : BM019298.D
Acq On : 21 Mar 2019 19:44
Operator : JU/SJ
Sample : K2003-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
S4A(5-30)COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

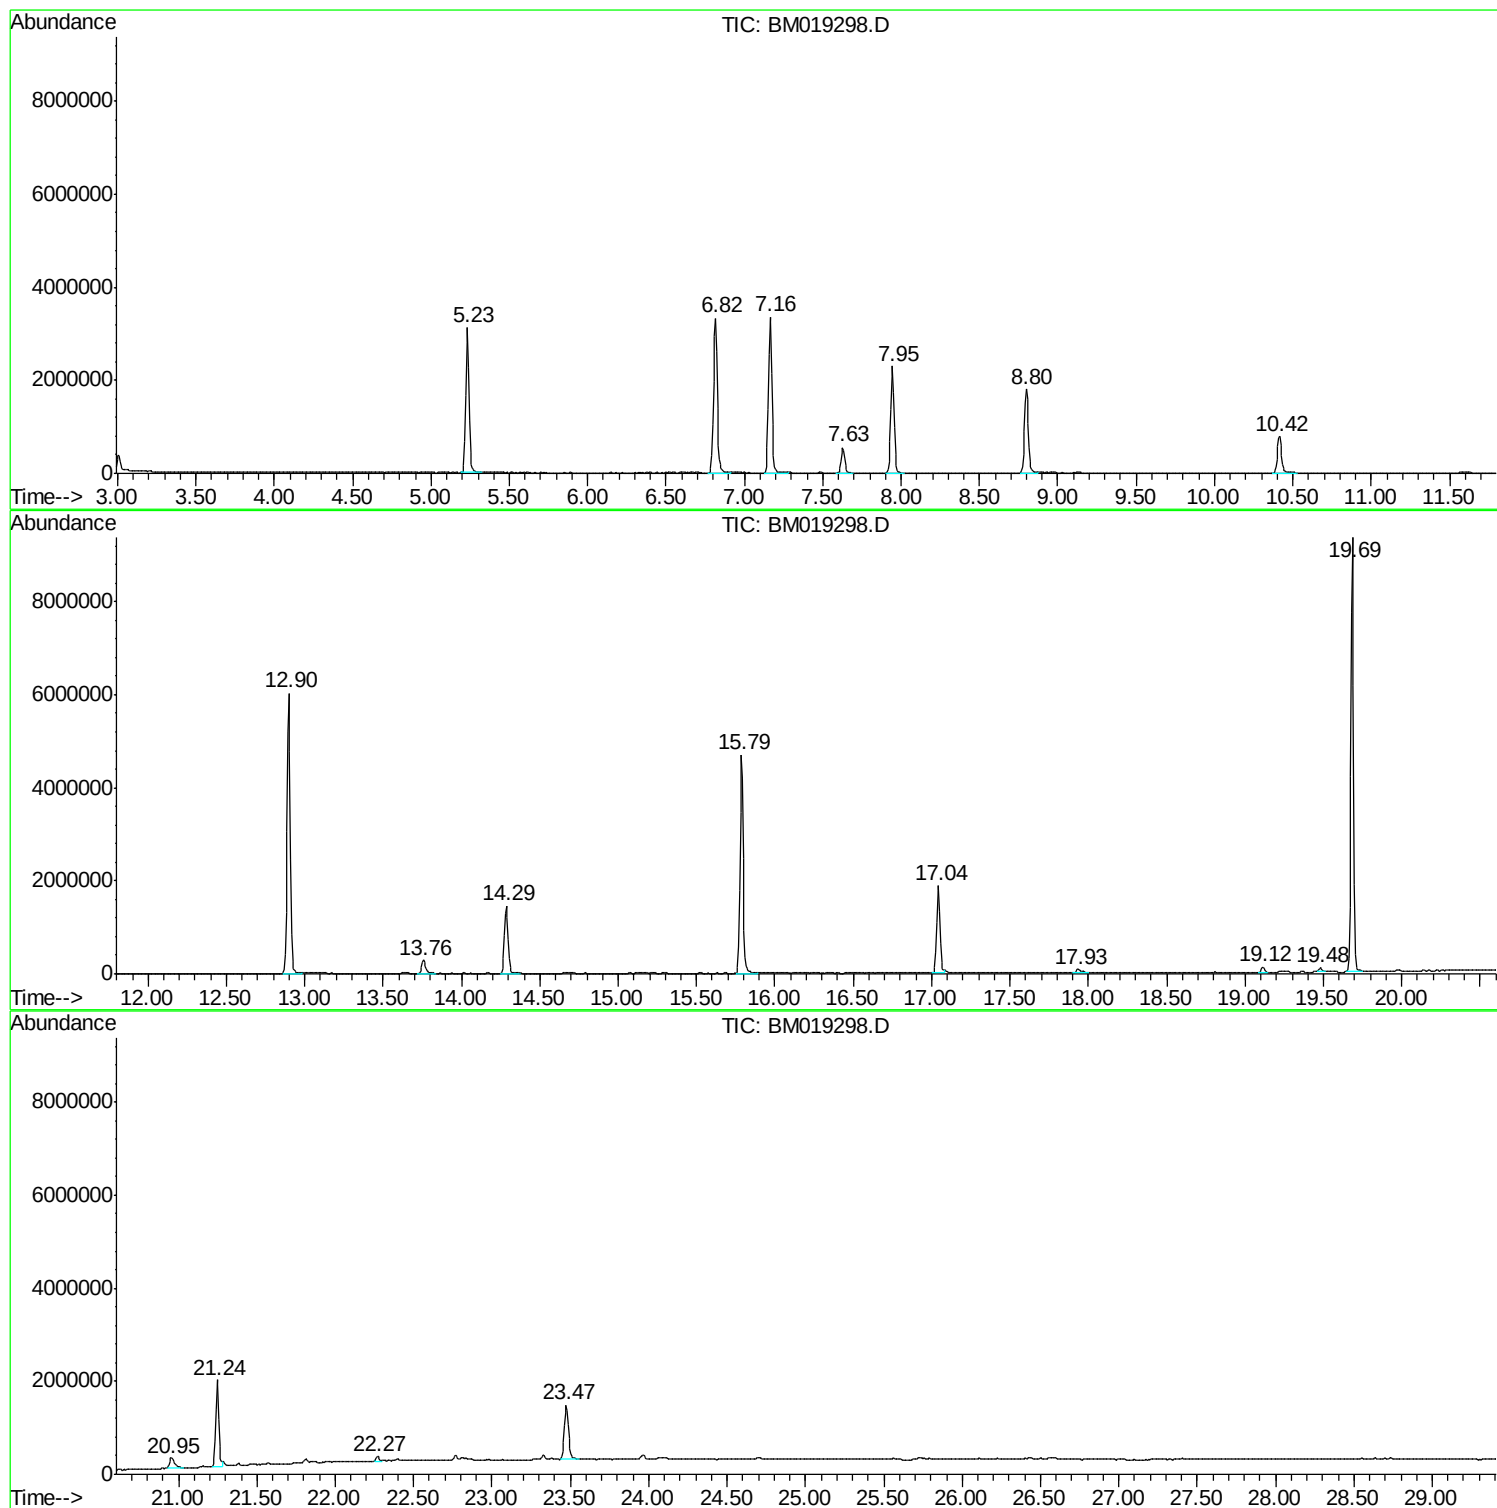

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032119\
Data File : BM019298.D
Acq On : 21 Mar 2019 19:44
Operator : JU/SJ
Sample : K2003-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
S4A(5-30)COMP










Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 unknown7.16 Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
7.16	123.75 ng	5308090	1,4-Dichlorobenzene-d4	7.63

Hit#	of	Tentative ID	MW	MolForm	CAS#	Qual
1	5	Tranlylcypromine-propionyl	189	C12H15NO	1000123-86-3	10
2		Bicyclo[4.2.0]octa-1,3,5-triene,...	132	C10H12	028749-81-7	9
3		Benzene, 1-ethenyl-3,5-dimethyl-	132	C10H12	005379-20-4	9
4		Xenon	132	Xe	007440-63-3	9
5		(E)-3-Chloro-2-methyl-2-pentenal	132	C6H9ClO	031357-76-3	9

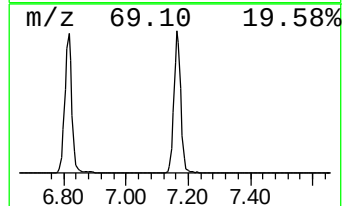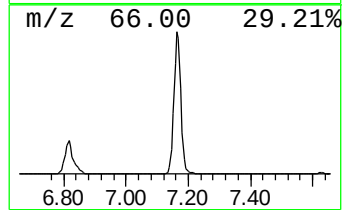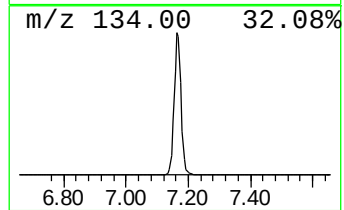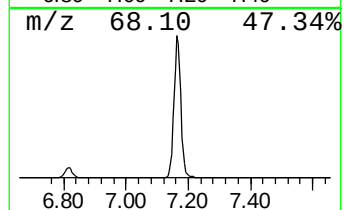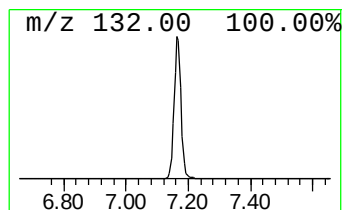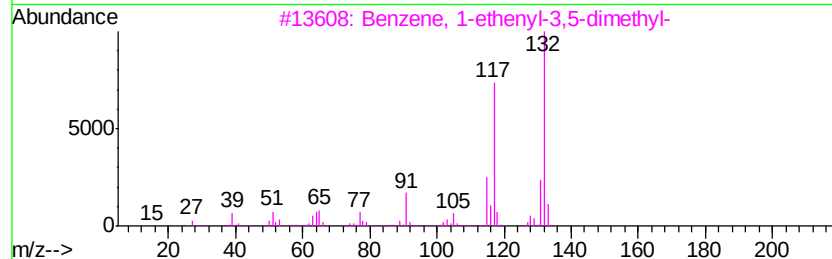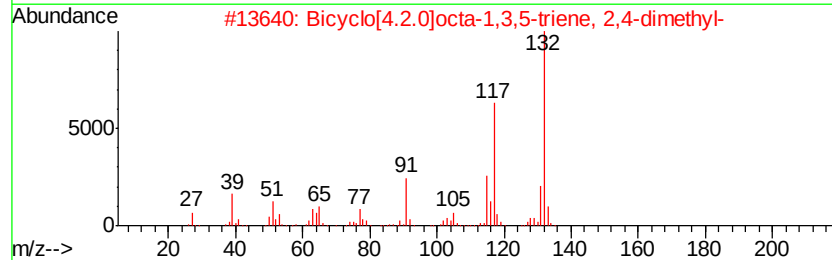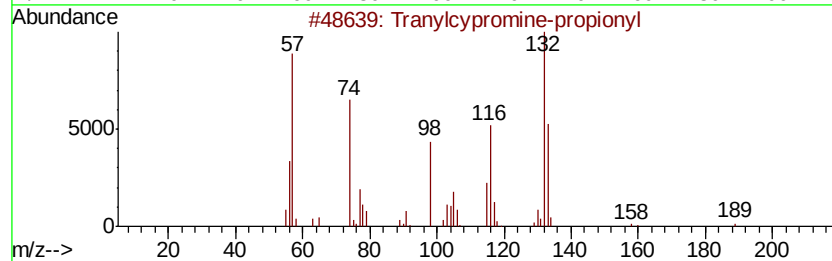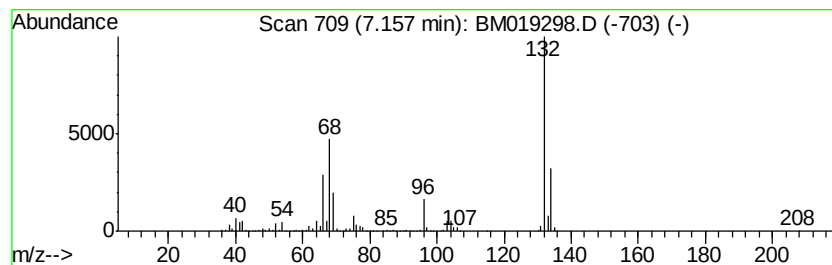

Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032119\
Data File : BM019298.D
Acq On : 21 Mar 2019 19:44
Operator : JU/SJ
Sample : K2003-01
Misc :
ALS Vial : 10 Sample Multiplier: 1










Instrument :
BNA_M
ClientSampleId :
S4A(5-30)COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

Peak Number 3 1-Nonadecene Concentration Rank 3

R.T.	EstConc	Area	Relative to ISTD	R.T.
20.95	3.87 ng	501014	Chrysene-d12	21.24
Hit# of	5	Tentative ID	MW MolForm	CAS# Qual
1	1-Nonadecene	266 C19H38	018435-45-5	96
2	3-Eicosene, (E)-	280 C20H40	074685-33-9	91
3	Trichloroacetic acid, hexadecyl ...	386 C18H33Cl3O2	074339-54-1	91
4	Heptafluorobutanoic acid, heptad...	452 C21H35F7O2	1000282-97-3	91
5	Trichloroacetic acid, pentadecyl...	372 C17H31Cl3O2	074339-53-0	91

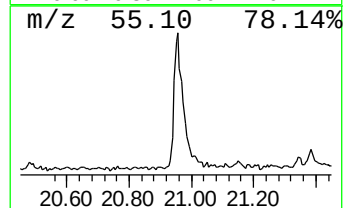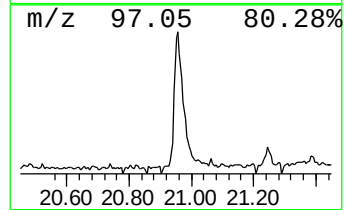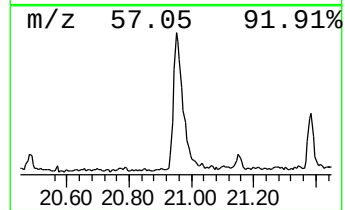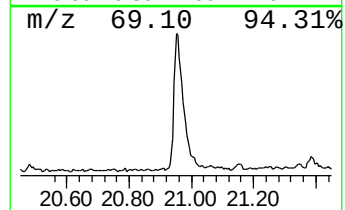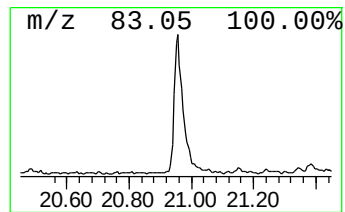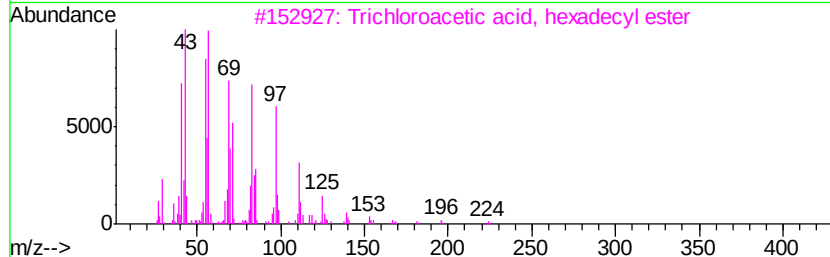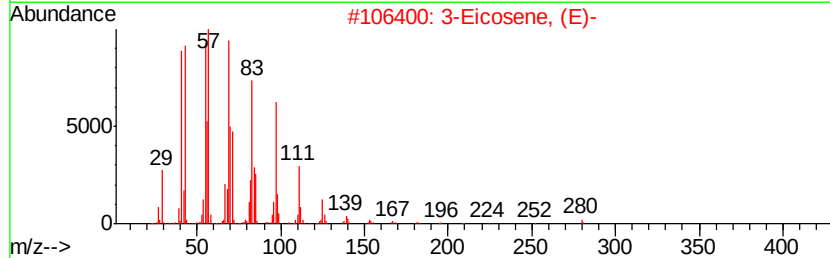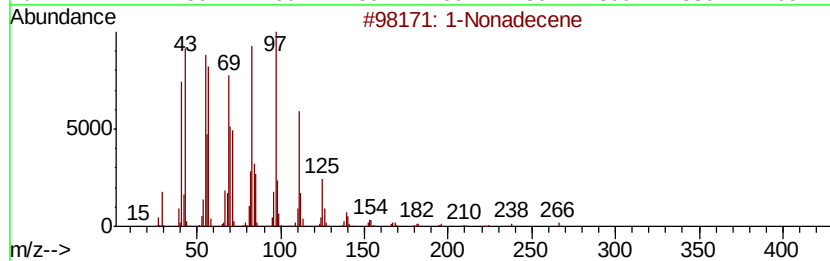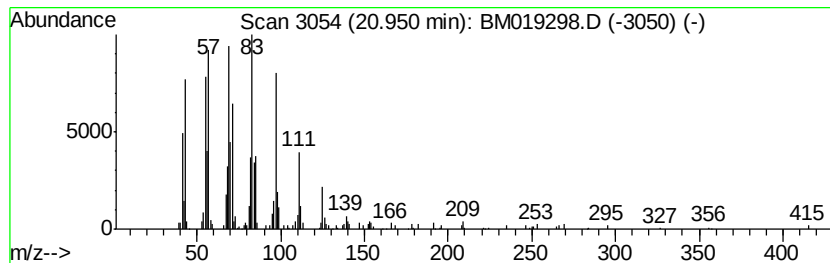

Data Path : Z:\SVOASRV\HPCHEM1\BNA_M\DATA\BM032119\
Data File : BM019298.D
Acq On : 21 Mar 2019 19:44
Operator : JU/SJ
Sample : K2003-01
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
S4A(5-30)COMP

Quant Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\DATABASE\NIST02.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	---Internal Standard---			
					#	RT	Resp	Conc
unknown7.16	7.16	123.8	ng	5308090	1	7.63	857863	20.0
1-Nonadecene	20.95	3.9	ng	501014	5	21.24	2587290	20.0