


Data Path : Z:\SVOASRV\HPCHEM1\BNA M\DATA\BM032119\
 Data File : BM019289.D
 Acq On : 21 Mar 2019 14:18
 Operator : JU/SJ
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\SVOASRV\HPCHEM1\BNA_M\METHODS\8270-BM031119.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Mon Mar 11 17:30:46 2019

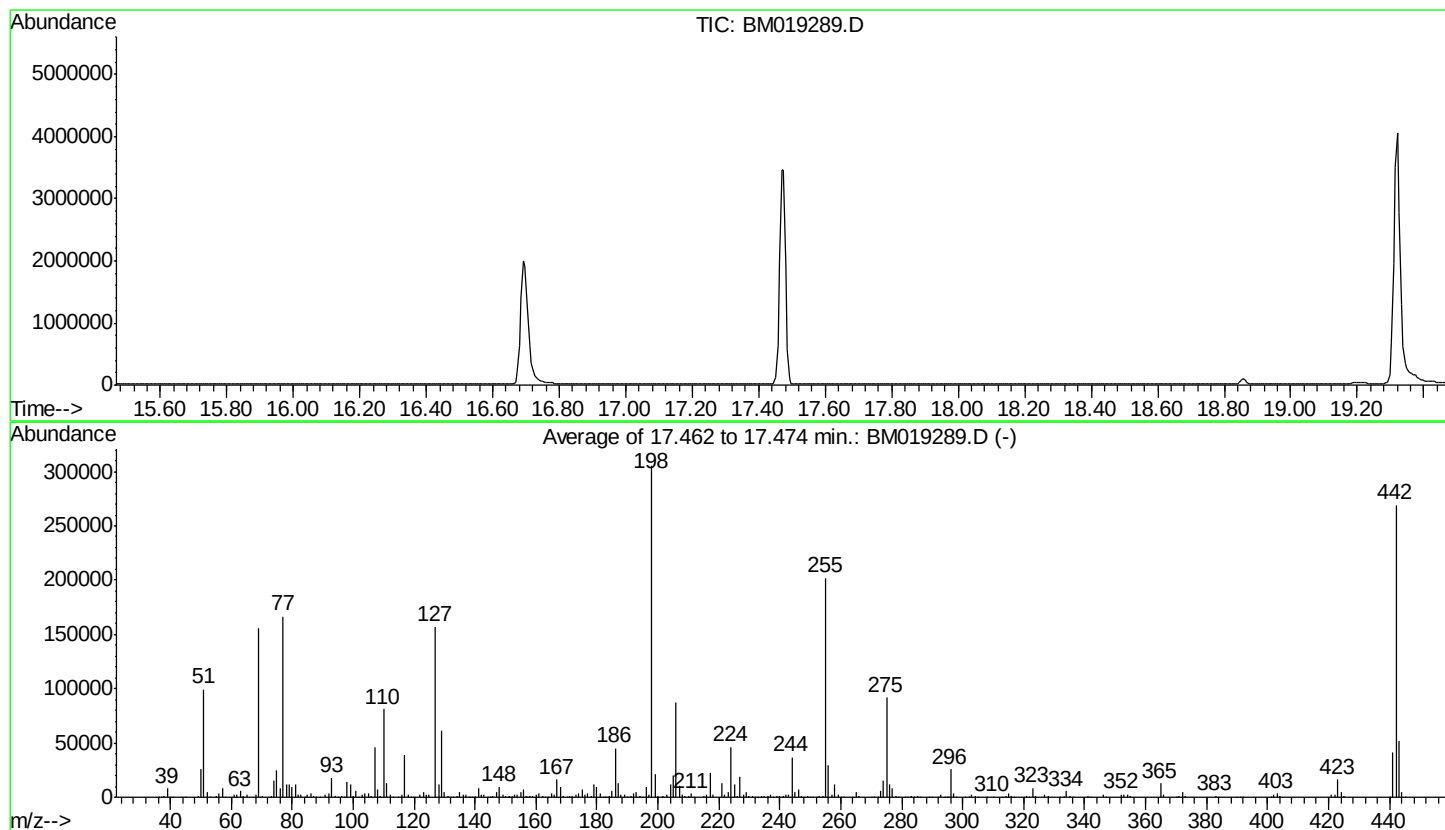

AutoFind: Scans 2461, 2462, 2463; Background Corrected with Scan 2455

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	32.5	99165	PASS
68	69	0.00	2	1.9	2905	PASS
69	198	0.00	100	51.1	156082	PASS
70	69	0.00	2	0.5	719	PASS
127	198	10	80	51.5	157397	PASS
197	198	0.00	2	0.8	2376	PASS
198	198	100	100	100.0	305429	PASS
199	198	5	9	6.8	20674	PASS
275	198	10	60	30.0	91541	PASS
365	198	1	100	4.1	12463	PASS
441	198	0.01	100	13.5	41253	PASS
442	198	50	100	88.0	268909	PASS
443	442	15	24	19.2	51656	PASS