

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044683.D
 Acq On : 20 Mar 2024 14:53
 Operator : MA/JU
 Sample : P1760-01
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0764

Quant Time: Mar 20 15:32:08 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 15 11:12:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.692	152	123114	20.000	ng/u1	0.00
20) Naphthalene-d8	10.469	136	466360	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.339	164	250311	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.092	188	478606	20.000	ng/u1	0.00
79) Chrysene-d12	21.291	240	413940	20.000	ng/u1	0.00
88) Perylene-d12	23.538	264	506544	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.257	96	13576	3.740	ng/uL	0.00
4) Pyridine-d5	3.663	84	80312	7.517	ng/u1	0.00
7) Phenol-d5	6.863	99	215891	17.056	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.039	67	148372	18.977	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.228	132	171658	18.455	ng/u1	0.00
15) 4-Methylphenol-d8	8.398	113	150890	15.179	ng/u1	0.00
21) Nitrobenzene-d5	8.851	128	79350	20.206	ng/u1	0.00
24) 2-Nitrophenol-d4	9.569	143	79625	18.808	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.098	165	137489	19.082	ng/u1	0.00
31) 4-Chloroaniline-d4	10.627	131	147612	12.336	ng/u1	0.00
46) Dimethylphthalate-d6	13.763	166	386569	19.687	ng/u1	0.00
49) Acenaphthylene-d8	14.027	160	448191	19.959	ng/u1	0.00
54) 4-Nitrophenol-d4	14.557	143	47965	11.779	ng/u1	0.00
60) Fluorene-d10	15.339	176	348164	21.100	ng/u1	0.00
65) 4,6-Dinitro-2-methylph...	15.462	200	31234	10.054	ng/u1	-0.01
73) Anthracene-d10	17.192	188	482874	21.107	ng/u1	0.00
81) Pyrene-d10	19.492	212	580084	22.849	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.391	264	599159	22.504	ng/u1	0.00


Target Compounds				Qvalue	
16) Acetophenone	8.522	105	25541	1.657 ng/u1#	93


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044683.D
Acq On : 20 Mar 2024 14:53
Operator : MA/JU
Sample : P1760-01
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0764


Quant Time: Mar 20 15:32:08 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 15 11:12:49 2024
Response via : Initial Calibration

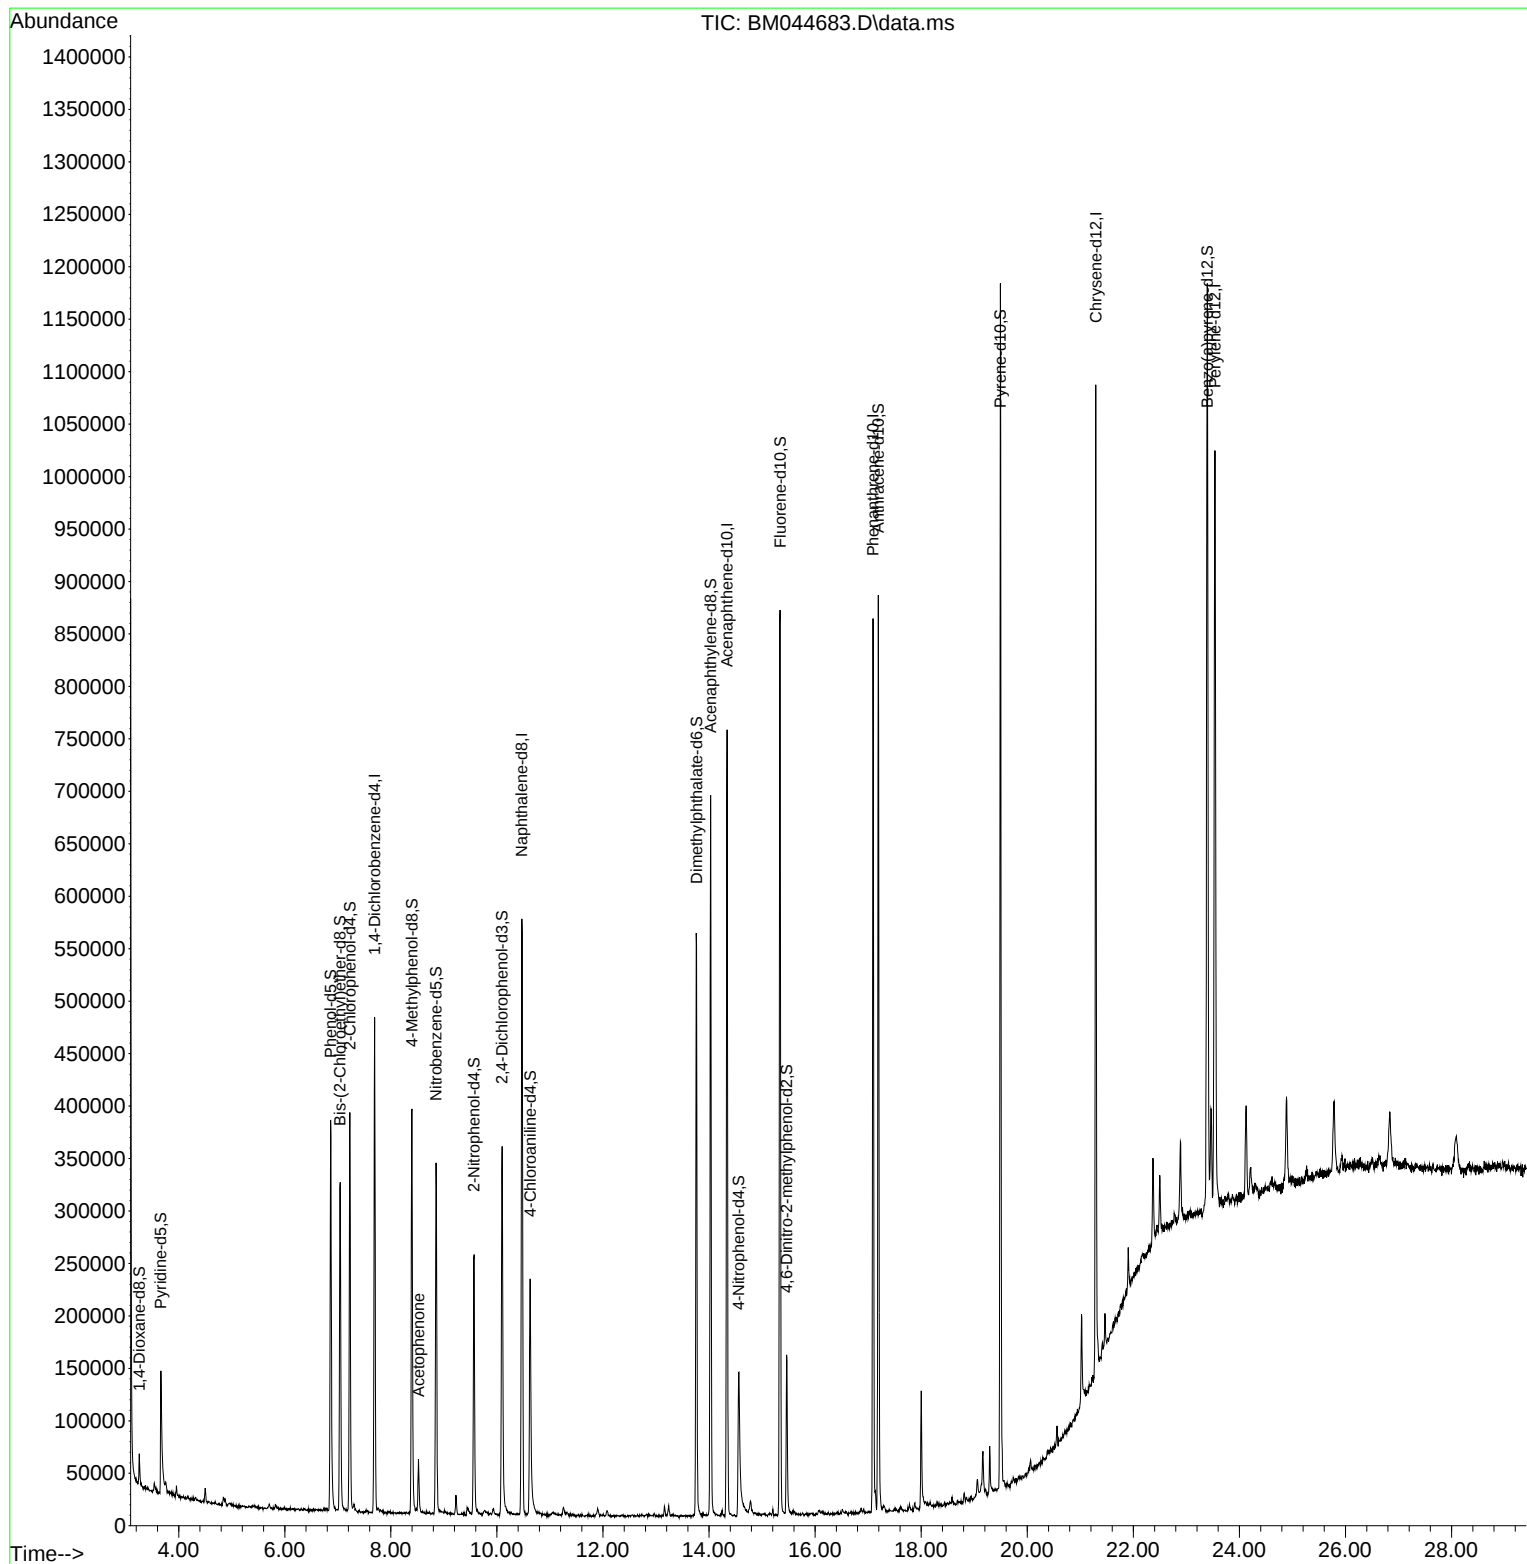

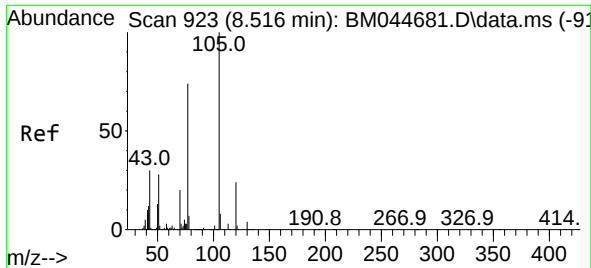

#16
 Acetophenone
 Concen: 1.657 ng/ul
 RT: 8.522 min Scan# 91
 Delta R.T. -0.000 min
 Lab File: BM044683.D
 Acq: 20 Mar 2024 14:53

Instrument :
 BNA_M
 ClientSampleId :
 E0764

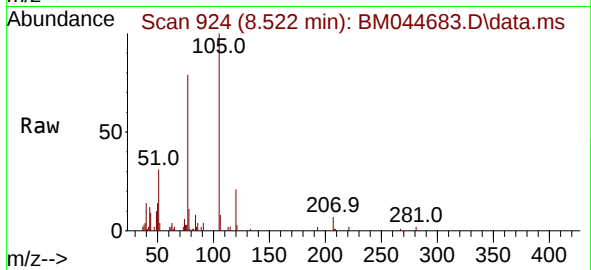

Tgt Ion	Ratio	Lower	Upper
105	100		
77	78.7	59.5	89.3
51	31.4	20.2	30.4

