

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044684.D
 Acq On : 20 Mar 2024 15:30
 Operator : MA/JU
 Sample : P1760-02
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0765

Quant Time: Mar 20 16:04:00 2024
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Quant Title : SVOA CALIBRATION
 QLast Update : Fri Mar 15 11:12:49 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.693	152	143522	20.000	ng/u1	0.00
20) Naphthalene-d8	10.469	136	551475	20.000	ng/u1	-0.01
38) Acenaphthene-d10	14.339	164	300049	20.000	ng/u1	0.00
64) Phenanthrene-d10	17.092	188	565654	20.000	ng/u1	0.00
79) Chrysene-d12	21.292	240	482221	20.000	ng/u1	0.00
88) Perylene-d12	23.539	264	570547	20.000	ng/u1	0.00
System Monitoring Compounds						
3) 1,4-Dioxane-d8	3.258	96	14073	3.326	ng/uL	0.00
4) Pyridine-d5	3.663	84	111090	8.919	ng/u1	0.00
7) Phenol-d5	6.863	99	242652	16.445	ng/u1	0.00
9) Bis-(2-Chloroethyl)eth...	7.040	67	165115	18.116	ng/u1	-0.01
11) 2-Chlorophenol-d4	7.228	132	194471	17.934	ng/u1	0.00
15) 4-Methylphenol-d8	8.393	113	176312	15.215	ng/u1	-0.01
21) Nitrobenzene-d5	8.851	128	90650	19.521	ng/u1	0.00
24) 2-Nitrophenol-d4	9.569	143	92826	18.543	ng/u1	0.00
28) 2,4-Dichlorophenol-d3	10.098	165	154310	18.112	ng/u1	0.00
31) 4-Chloroaniline-d4	10.622	131	173170	12.238	ng/u1	0.00
46) Dimethylphthalate-d6	13.757	166	439747	18.683	ng/u1	-0.01
49) Acenaphthylene-d8	14.027	160	513663	19.082	ng/u1	0.00
54) 4-Nitrophenol-d4	14.557	143	53664	10.994	ng/u1	0.00
60) Fluorene-d10	15.333	176	386534	19.542	ng/u1	-0.01
65) 4,6-Dinitro-2-methylph...	15.463	200	34203	9.315	ng/u1	-0.01
73) Anthracene-d10	17.192	188	542613	20.069	ng/u1	0.00
81) Pyrene-d10	19.492	212	635731	21.495	ng/u1	0.00
92) Benzo(a)pyrene-d12	23.397	264	632353	21.086	ng/u1	0.00


Target Compounds					Qvalue	
16) Acetophenone	8.522	105	22493	1.252	ng/u1#	90


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044684.D
Acq On : 20 Mar 2024 15:30
Operator : MA/JU
Sample : P1760-02
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0765

Quant Time: Mar 20 16:04:00 2024
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION
QLast Update : Fri Mar 15 11:12:49 2024
Response via : Initial Calibration

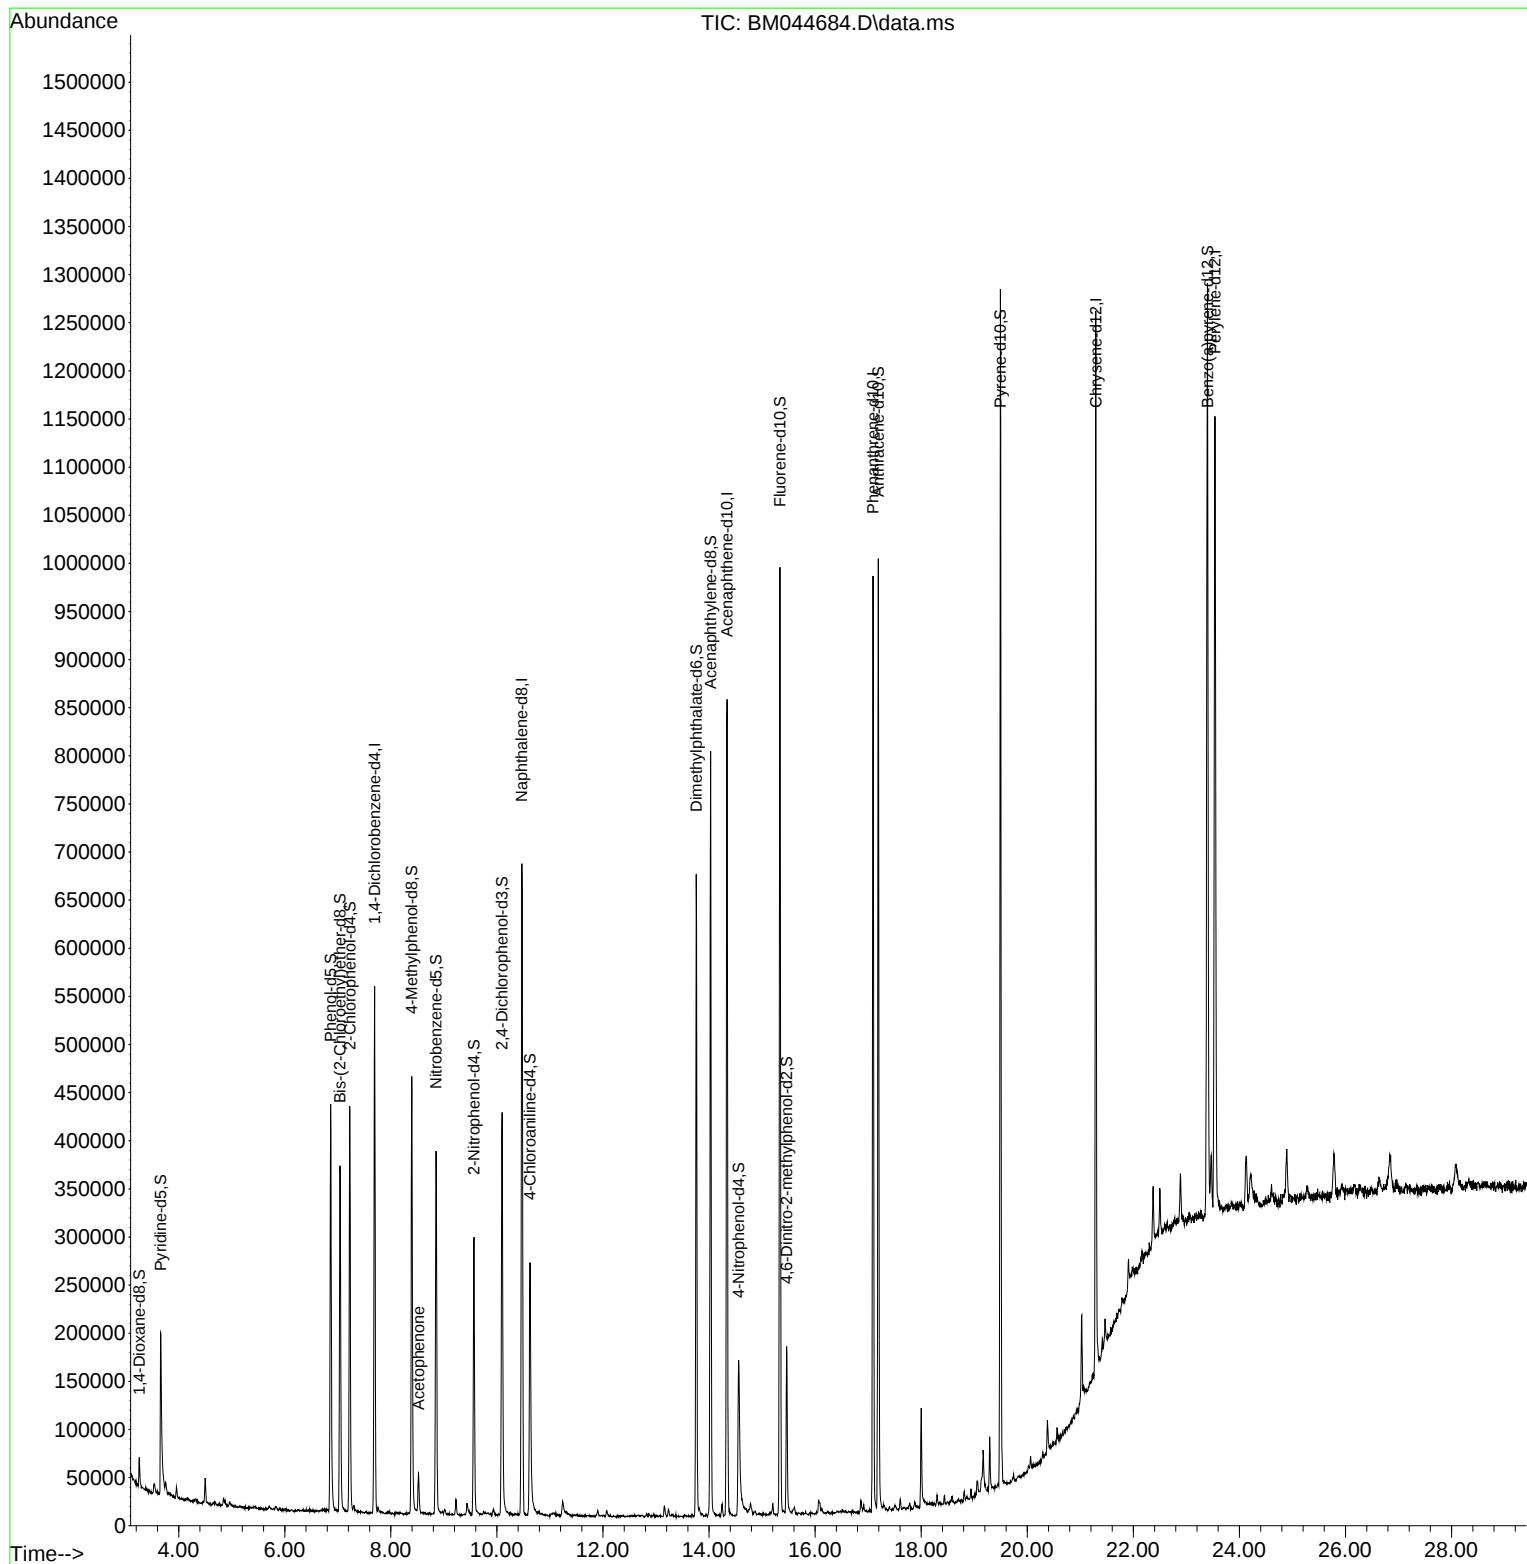

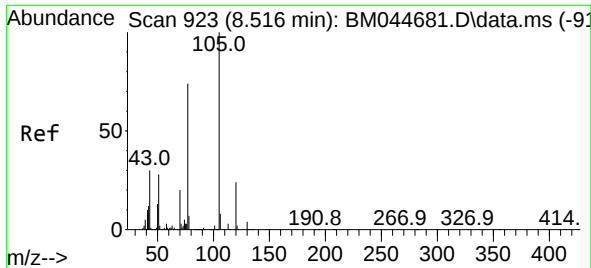

#16
 Acetophenone
 Concen: 1.252 ng/ul
 RT: 8.522 min Scan# 91
 Delta R.T. 0.000 min
 Lab File: BM044684.D
 Acq: 20 Mar 2024 15:30

Instrument :
 BNA_M
 ClientSampleId :
 E0765

Tgt Ion:	105	Resp:	22493
Ion Ratio	Lower	Upper	
105	100		
77	80.9	59.5	89.3
51	34.1	20.2	30.4#

