

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044694.D
 Acq On : 21 Mar 2024 10:49
 Operator : MA/JU
 Sample : PB159693BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK693

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Sampling : 1

Start Thrs: 0.2

Stop Thrs : 0

Filtering: 5

Min Area: 0.1 % of largest Peak

Max Peaks: 100

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044694.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.251	25	28	38	rVB	63076	85625	2.54%	0.208%
2	3.651	92	96	117	rBV	692738	1173140	34.83%	2.851%
3	3.957	144	148	153	rVB	11265	17056	0.51%	0.041%
4	4.275	200	202	205	rBV4	3045	3600	0.11%	0.009%
5	5.604	423	428	429	rBV5	2358	3522	0.10%	0.009%
6	6.269	539	541	544	rBV4	3086	3903	0.12%	0.009%
7	6.863	635	642	655	rBV	832117	1339358	39.76%	3.255%
8	7.039	666	672	684	rBV	716207	1124658	33.39%	2.734%
9	7.222	696	703	713	rBV	839171	1337831	39.72%	3.252%
10	7.292	713	715	719	rVB5	3424	3848	0.11%	0.009%
11	7.692	774	783	793	rBV	633729	1029415	30.56%	2.502%
12	8.392	894	902	913	rBV	990233	1598851	47.47%	3.886%
13	8.851	971	980	991	rBV	772349	1284308	38.13%	3.122%
14	9.563	1093	1101	1112	rBV	644049	1053249	31.27%	2.560%
15	9.633	1112	1113	1118	rVB5	2731	3680	0.11%	0.009%
16	10.092	1183	1191	1214	rBV	881465	1558525	46.27%	3.788%
17	10.469	1248	1255	1263	rBV	849243	1417667	42.09%	3.446%
18	10.616	1273	1280	1303	rBV	851537	1651457	49.03%	4.014%
19	11.886	1495	1496	1503	rVB6	2357	3462	0.10%	0.008%
20	12.080	1524	1529	1541	rBV3	10168	22977	0.68%	0.056%
21	13.233	1720	1725	1732	rBV2	10547	17179	0.51%	0.042%
22	13.757	1807	1814	1825	rBV	1452743	2053844	60.97%	4.992%
23	14.027	1852	1860	1870	rBV	1740711	2565106	76.15%	6.235%
24	14.333	1906	1912	1922	rBV	1176130	1726916	51.27%	4.197%
25	14.551	1941	1949	1973	rBV	434607	913038	27.11%	2.219%
26	14.757	1982	1984	1991	rVB6	4272	7022	0.21%	0.017%
27	15.333	2076	2082	2098	rBV	2092878	3044462	90.38%	7.400%
28	15.462	2098	2104	2119	rVV	617991	882148	26.19%	2.144%
29	15.574	2120	2123	2128	rVB5	10049	14057	0.42%	0.034%
30	16.127	2214	2217	2221	rVB5	6109	7454	0.22%	0.018%
31	16.780	2323	2328	2332	rBV6	2622	4165	0.12%	0.010%
32	17.092	2374	2381	2390	rVV	1320239	1823602	54.14%	4.432%
33	17.192	2390	2398	2415	rVV	2125123	3056643	90.74%	7.429%
34	18.021	2534	2539	2540	rBV5	3038	4352	0.13%	0.011%
35	19.056	2711	2715	2721	rVB2	21108	28703	0.85%	0.070%
36	19.127	2723	2727	2732	rBV2	18302	25664	0.76%	0.062%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044694.D
Acq On : 21 Mar 2024 10:49
Operator : MA/JU
Sample : PB159693BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK693

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	19.492	2783	2789	2799	rBV	2413984	3245777	96.36%	7.889%
38	21.286	3089	3094	3102	rBV	1266896	1733140	51.45%	4.213%
39	23.391	3445	3452	3459	rBV	1833298	3368398	100.00%	8.187%
40	23.532	3469	3476	3485	rBV	1025207	1904900	56.55%	4.630%




Sum of corrected areas: 41142702

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044694.D
Acq On : 21 Mar 2024 10:49
Operator : MA/JU
Sample : PB159693BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK693

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

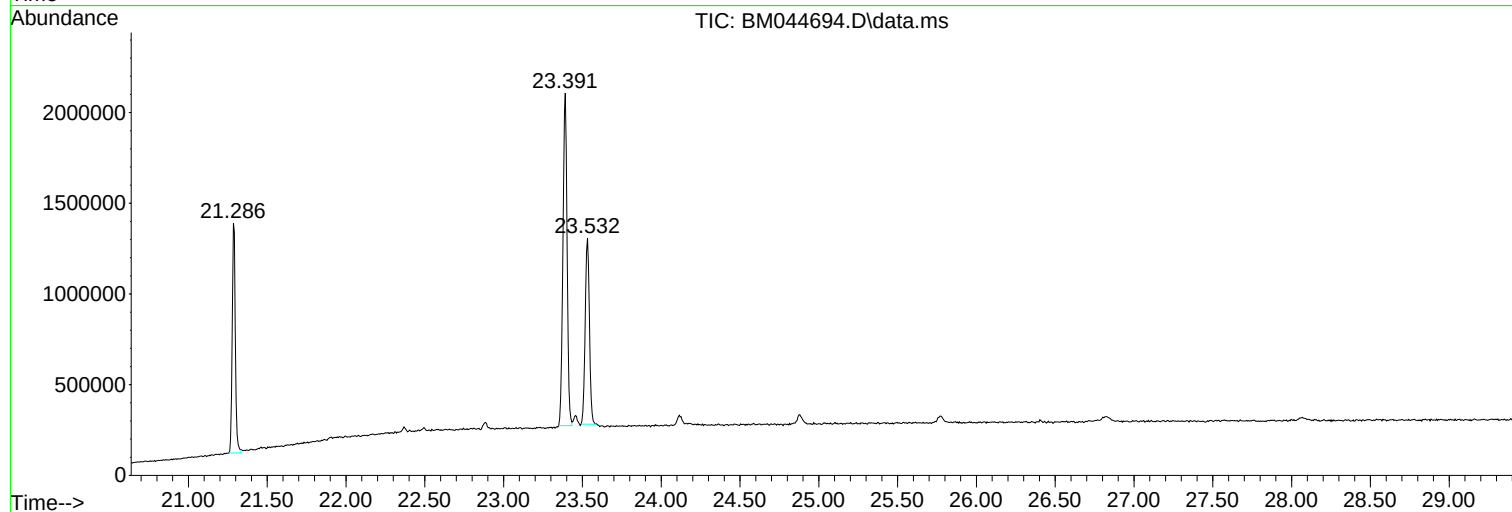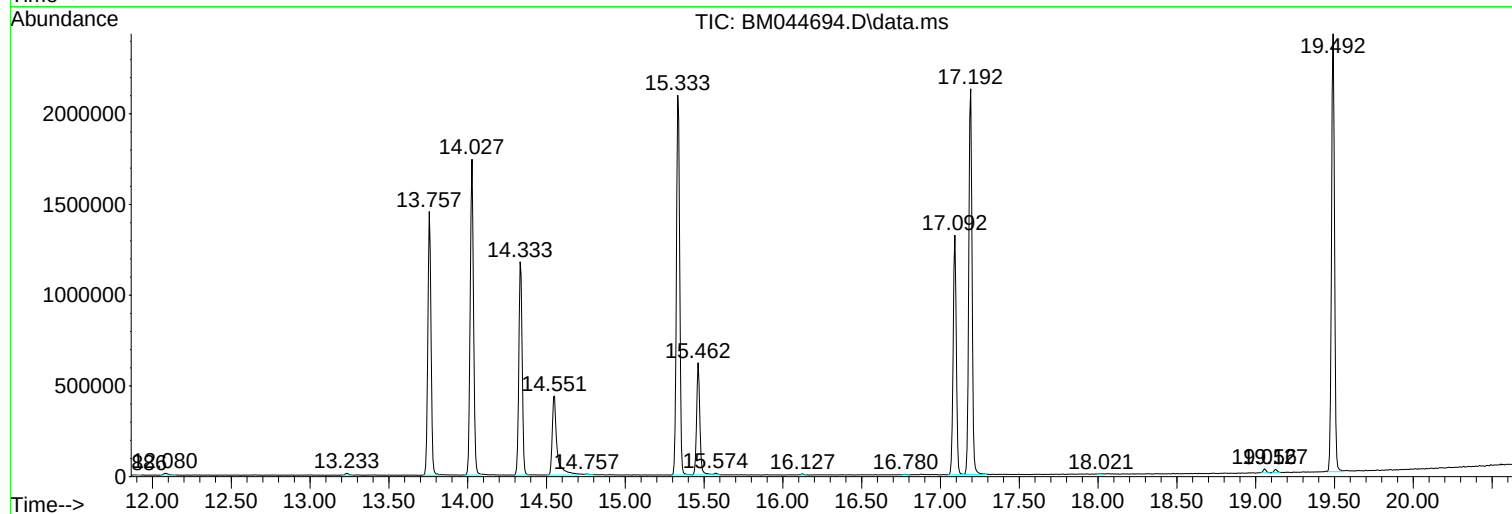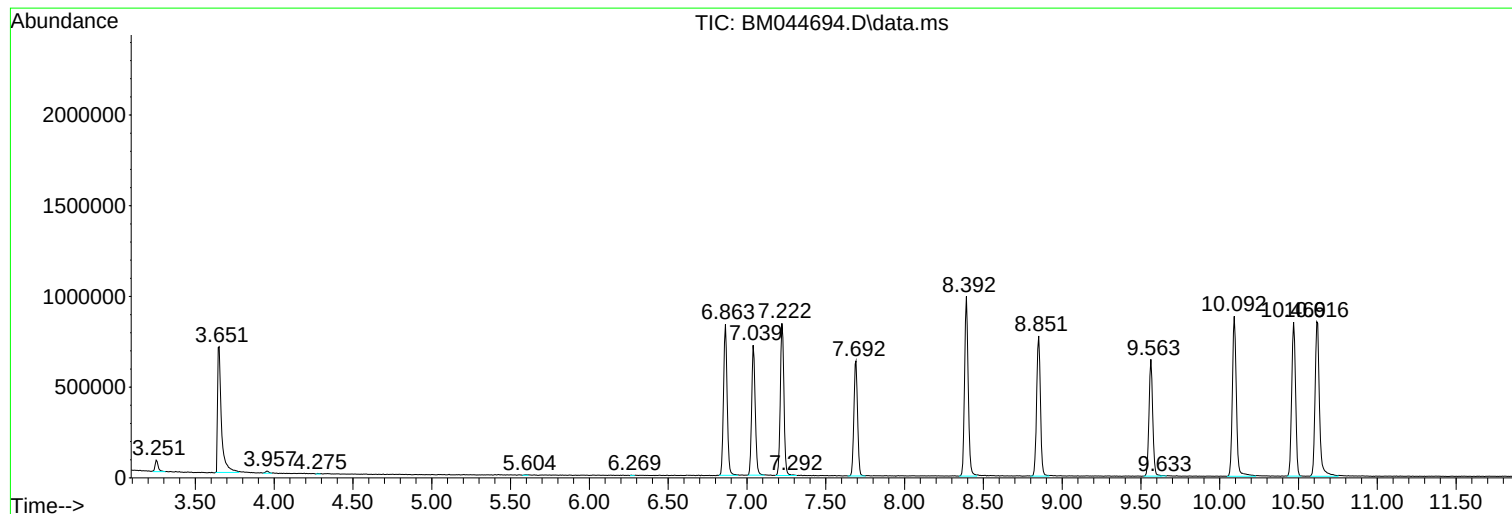

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044694.D
Acq On : 21 Mar 2024 10:49
Operator : MA/JU
Sample : PB159693BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK693

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044694.D
Acq On : 21 Mar 2024 10:49
Operator : MA/JU
Sample : PB159693BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK693

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------