

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044696.D
 Acq On : 21 Mar 2024 12:01
 Operator : MA/JU
 Sample : P1813-01
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LX1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044696.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.257	25	29	38	rVB	47272	67825	2.02%	0.187%
2	3.657	94	97	116	rBV	154275	290529	8.64%	0.802%
3	3.951	145	147	157	rVB4	11920	19980	0.59%	0.055%
4	5.422	393	397	401	rBV7	2845	5459	0.16%	0.015%
5	6.545	584	588	591	rVB5	2314	3367	0.10%	0.009%
6	6.734	618	620	624	rVB5	2388	3373	0.10%	0.009%
7	6.863	636	642	651	rBV	171431	292722	8.70%	0.808%
8	7.040	666	672	685	rBV	646145	1031303	30.66%	2.848%
9	7.222	696	703	712	rBV	605459	965437	28.70%	2.666%
10	7.298	715	716	725	rVB6	6378	8349	0.25%	0.023%
11	7.692	775	783	792	rBV	634400	1028800	30.58%	2.841%
12	8.392	895	902	916	rBV	460352	768163	22.84%	2.122%
13	8.851	971	980	991	rBV	713447	1188961	35.35%	3.284%
14	9.222	1040	1043	1047	rBV3	11111	16707	0.50%	0.046%
15	9.563	1093	1101	1113	rBV	556534	926337	27.54%	2.558%
16	10.092	1184	1191	1210	rBV	737371	1291494	38.39%	3.567%
17	10.469	1246	1255	1264	rBV	852442	1419195	42.19%	3.920%
18	10.616	1272	1280	1301	rBV	612038	1224770	36.41%	3.383%
19	11.722	1459	1468	1472	rBV2	11853	20344	0.60%	0.056%
20	12.080	1523	1529	1540	rVB2	10563	24442	0.73%	0.068%
21	13.227	1720	1724	1731	rBV4	8723	14950	0.44%	0.041%
22	13.757	1807	1814	1829	rBV	1419061	1979161	58.84%	5.466%
23	14.027	1853	1860	1871	rBV	1652056	2384559	70.89%	6.586%
24	14.333	1906	1912	1922	rBV	1160318	1716761	51.04%	4.742%
25	14.427	1925	1928	1933	rVB7	5212	7317	0.22%	0.020%
26	14.563	1944	1951	1963	rBV2	59762	159539	4.74%	0.441%
27	15.333	2075	2082	2096	rBV	2036367	2973402	88.39%	8.212%
28	15.462	2098	2104	2117	rBV	659534	907812	26.99%	2.507%
29	15.580	2120	2124	2130	rVB5	9344	14625	0.43%	0.040%
30	16.121	2213	2216	2220	rVB3	5836	6665	0.20%	0.018%
31	16.515	2276	2283	2286	rBV7	4543	8770	0.26%	0.024%
32	16.921	2350	2352	2357	rVB5	2481	4001	0.12%	0.011%
33	17.092	2374	2381	2391	rBV	1316253	1815156	53.96%	5.013%
34	17.192	2391	2398	2408	rVV	2121775	3081686	91.61%	8.511%
35	17.392	2429	2432	2435	rBV4	2949	3783	0.11%	0.010%
36	17.998	2530	2535	2543	rBV2	57122	90994	2.71%	0.251%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044696.D
Acq On : 21 Mar 2024 12:01
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	19.056	2711	2715	2720	rBV3	23405	34405	1.02%	0.095%
38	19.127	2723	2727	2731	rBV2	20290	27771	0.83%	0.077%
39	19.286	2751	2754	2759	rBV3	25202	37197	1.11%	0.103%
40	19.492	2783	2789	2799	rBV	2502512	3296715	98.01%	9.105%
41	21.286	3089	3094	3103	rBV	1267582	1717606	51.06%	4.744%
42	23.386	3445	3451	3460	rBV2	1836688	3363797	100.00%	9.290%
43	23.533	3469	3476	3492	rVB	996608	1962650	58.35%	5.421%




Sum of corrected areas: 36206879

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044696.D
Acq On : 21 Mar 2024 12:01
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

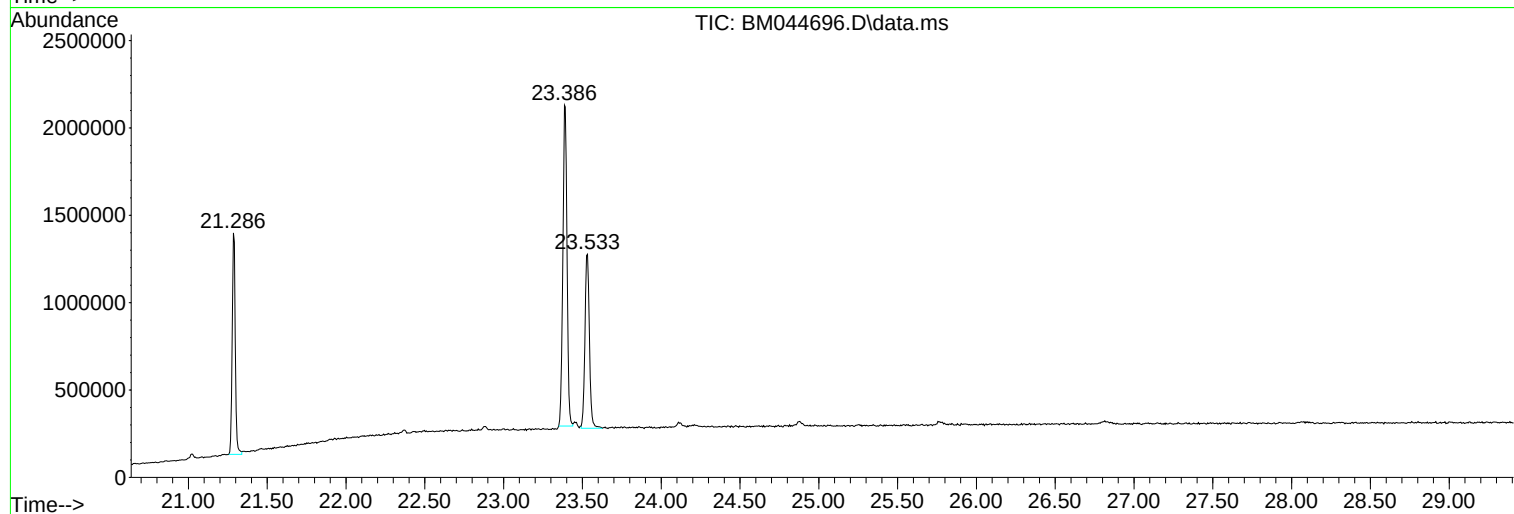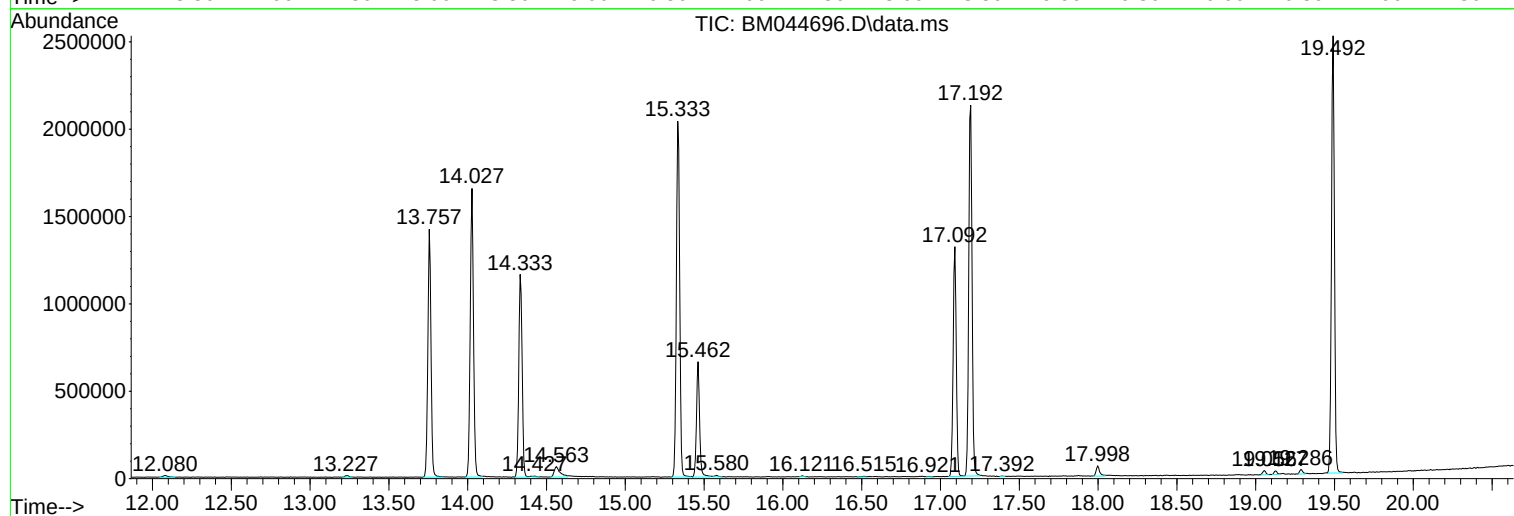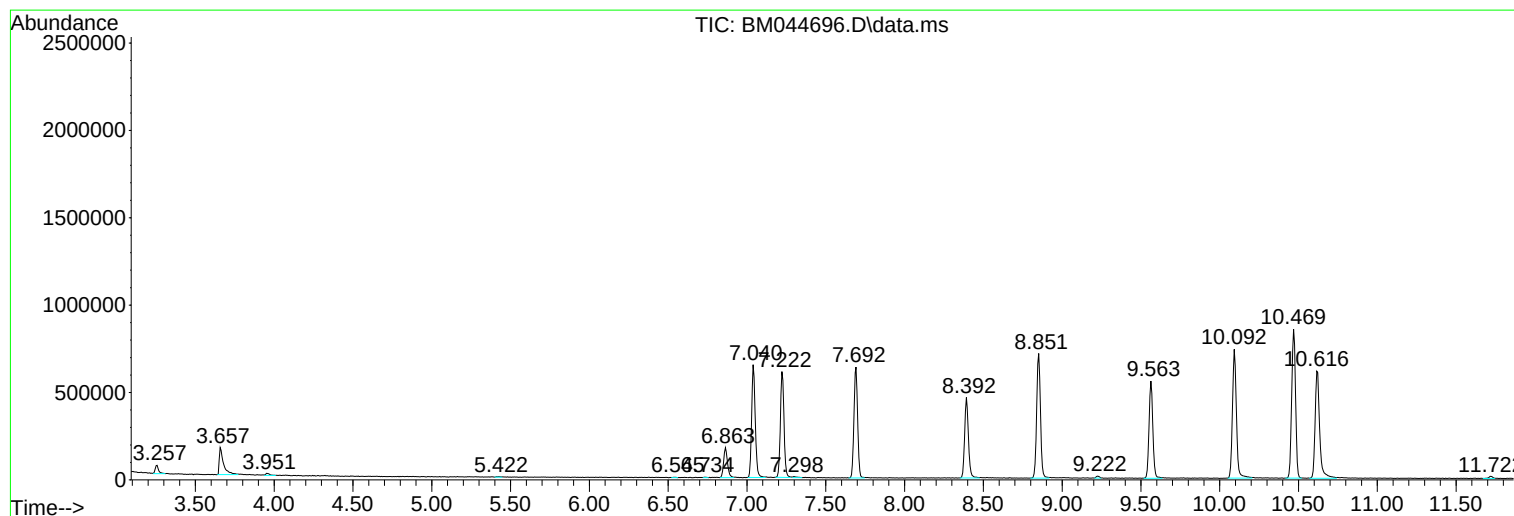

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044696.D
Acq On : 21 Mar 2024 12:01
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044696.D
Acq On : 21 Mar 2024 12:01
Operator : MA/JU
Sample : P1813-01
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX1

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc