

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044697.D
 Acq On : 21 Mar 2024 12:37
 Operator : MA/JU
 Sample : P1813-02
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LX2

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044697.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.258	25	29	36	rVB	43869	62098	1.48%	0.165%
2	3.658	94	97	116	rBV	156697	301214	7.16%	0.799%
3	3.952	144	147	154	rVB3	10273	15682	0.37%	0.042%
4	6.863	636	642	656	rBV	158551	267857	6.37%	0.710%
5	7.040	665	672	689	rBV	673704	1043042	24.81%	2.765%
6	7.222	696	703	713	rBV	597819	943678	22.44%	2.502%
7	7.693	776	783	790	rBV	572222	930783	22.14%	2.468%
8	7.757	790	794	799	rVB4	10512	17342	0.41%	0.046%
9	8.093	847	851	855	rBV4	2926	5880	0.14%	0.016%
10	8.393	895	902	915	rBV2	437303	734561	17.47%	1.947%
11	8.851	972	980	991	rBV	703325	1186650	28.22%	3.146%
12	9.228	1037	1044	1049	rBV	35941	53374	1.27%	0.142%
13	9.563	1093	1101	1115	rBV	543499	915112	21.76%	2.426%
14	10.092	1183	1191	1206	rBV	746848	1298936	30.89%	3.444%
15	10.469	1247	1255	1263	rVB	762394	1271510	30.24%	3.371%
16	10.616	1271	1280	1297	rBV	607419	1214980	28.90%	3.221%
17	11.716	1460	1467	1472	rBV	21397	34253	0.81%	0.091%
18	12.075	1523	1528	1534	rBV4	11572	21124	0.50%	0.056%
19	13.233	1719	1725	1731	rVV2	14063	21758	0.52%	0.058%
20	13.757	1807	1814	1826	rBV	1521724	2062107	49.04%	5.467%
21	14.028	1853	1860	1871	rBV	1665253	2445951	58.17%	6.485%
22	14.333	1905	1912	1920	rBV	1024932	1498863	35.65%	3.974%
23	14.422	1926	1927	1932	rVB5	4035	4364	0.10%	0.012%
24	14.563	1945	1951	1963	rBV	59976	158924	3.78%	0.421%
25	14.775	1986	1987	1994	rVB7	4214	5851	0.14%	0.016%
26	15.333	2075	2082	2097	rBV	2143006	3102838	73.79%	8.226%
27	15.463	2097	2104	2120	rVV	698540	979562	23.30%	2.597%
28	15.574	2120	2123	2130	rVB5	10224	17112	0.41%	0.045%
29	16.121	2212	2216	2225	rVB7	6530	13220	0.31%	0.035%
30	16.516	2278	2283	2287	rBV8	3873	6538	0.16%	0.017%
31	17.092	2372	2381	2390	rVV	1147516	1637193	38.94%	4.341%
32	17.192	2391	2398	2408	rVV	2298992	3304813	78.60%	8.762%
33	17.298	2410	2416	2420	rVB8	7504	16970	0.40%	0.045%
34	17.874	2509	2514	2518	rBV9	6751	10382	0.25%	0.028%
35	17.998	2529	2535	2545	rBV	88457	140735	3.35%	0.373%
36	18.433	2607	2609	2613	rBV5	4950	6286	0.15%	0.017%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044697.D
Acq On : 21 Mar 2024 12:37
Operator : MA/JU
Sample : P1813-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX2

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	19.051	2710	2714	2719	rVB2	25514	38270	0.91%	0.101%
38	19.127	2723	2727	2731	rBV	20703	31297	0.74%	0.083%
39	19.168	2731	2734	2736	rVV4	6807	8141	0.19%	0.022%
40	19.286	2750	2754	2762	rBV3	36909	61731	1.47%	0.164%
41	19.439	2778	2780	2783	rBV4	5482	6774	0.16%	0.018%
42	19.492	2783	2789	2798	rVV	2902293	3741159	88.97%	9.919%
43	21.021	3046	3049	3056	rBV3	58987	87143	2.07%	0.231%
44	21.286	3089	3094	3104	rBV	1330552	1771289	42.13%	4.696%
45	23.392	3445	3452	3459	rBV	2329473	4204763	100.00%	11.148%
46	23.533	3469	3476	3487	rVB	1042016	2016485	47.96%	5.346%




Sum of corrected areas: 37718595

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044697.D
Acq On : 21 Mar 2024 12:37
Operator : MA/JU
Sample : P1813-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

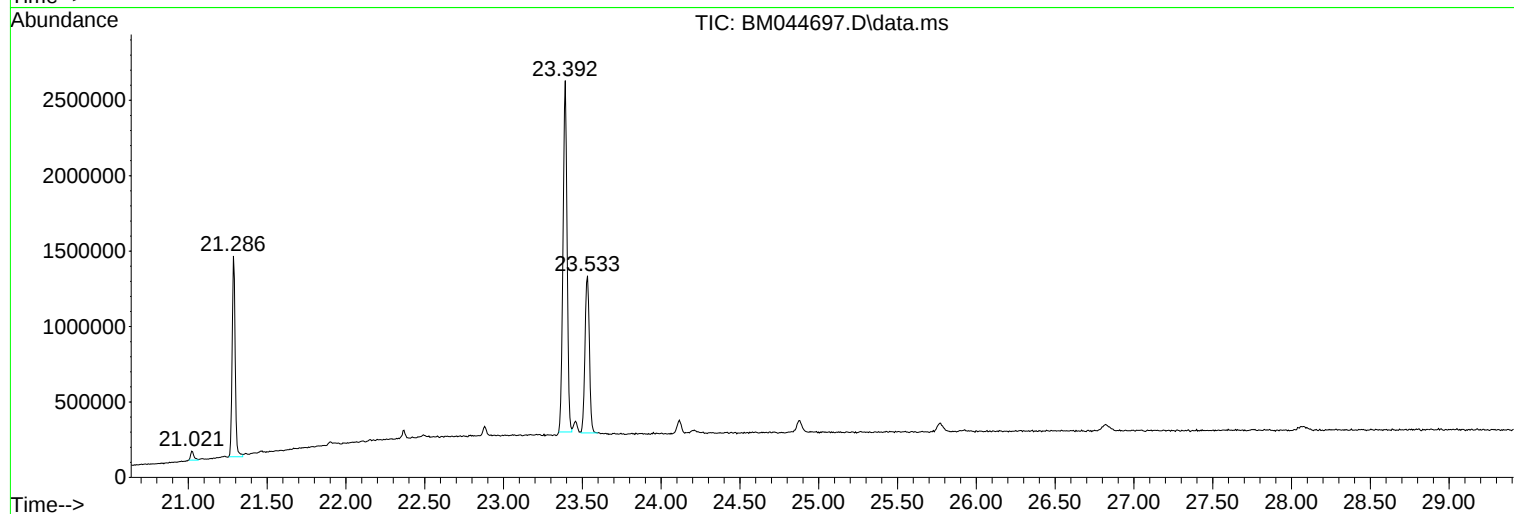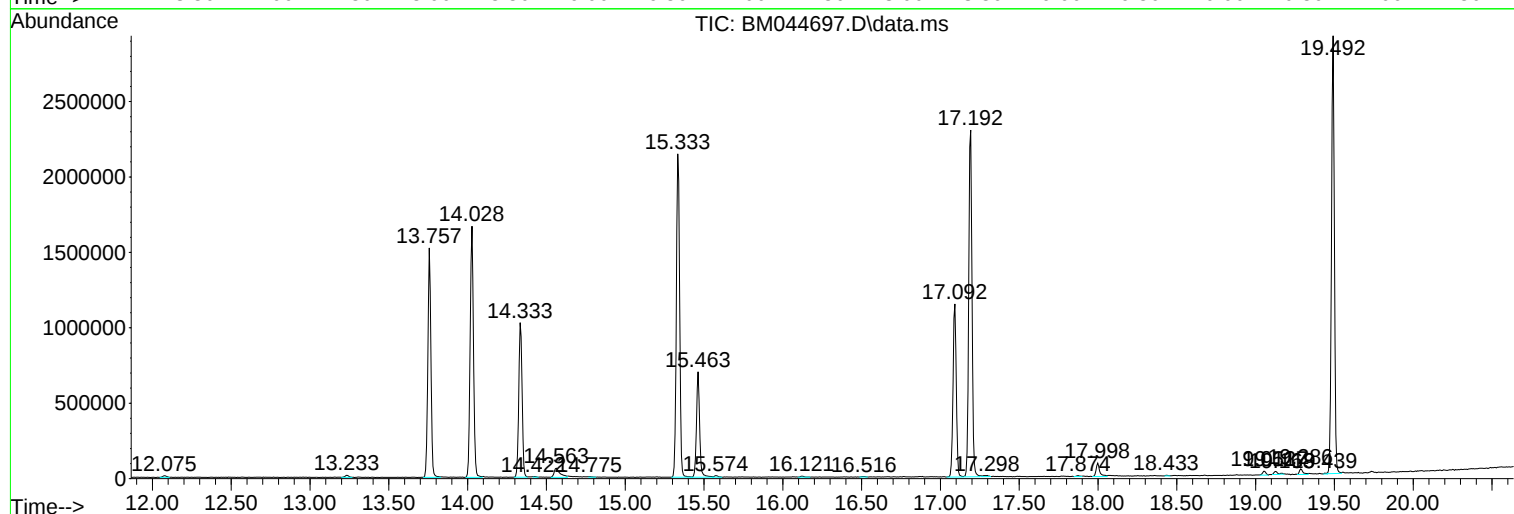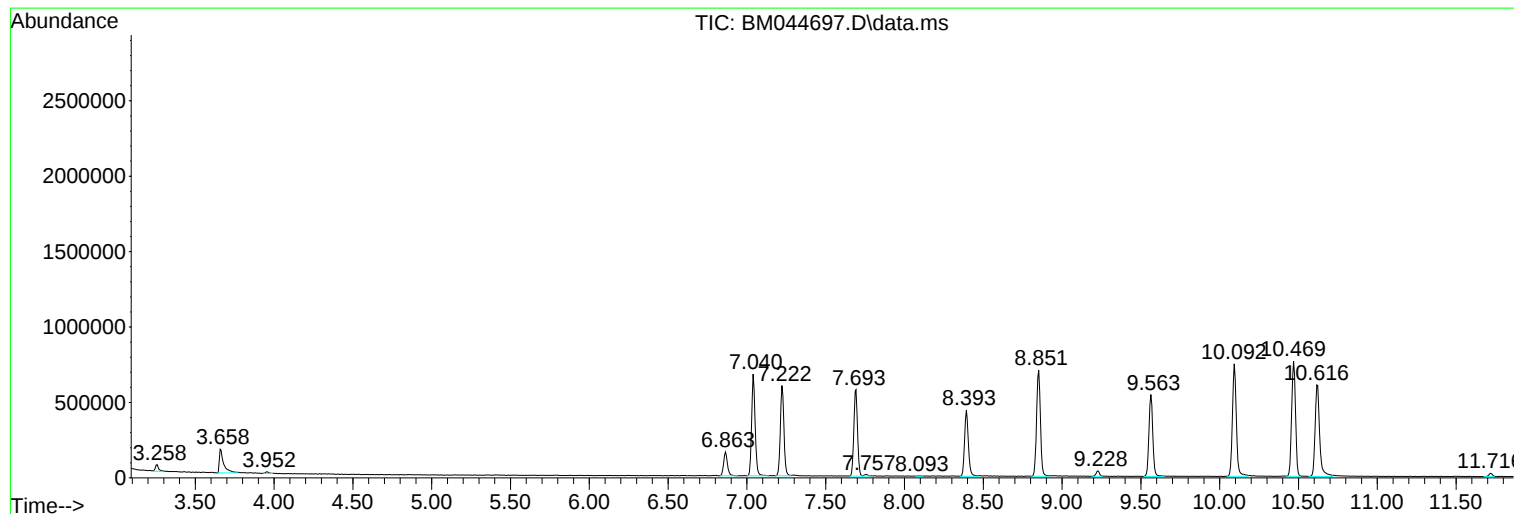

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044697.D
Acq On : 21 Mar 2024 12:37
Operator : MA/JU
Sample : P1813-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044697.D
Acq On : 21 Mar 2024 12:37
Operator : MA/JU
Sample : P1813-02
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc