

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044699.D
 Acq On : 21 Mar 2024 13:50
 Operator : MA/JU
 Sample : P1813-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044699.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	25	28	33	rBV	47254	57475	1.46%	0.142%
2	3.658	93	97	118	rBV	237204	439347	11.16%	1.087%
3	3.958	145	148	151	rVB	12024	14762	0.37%	0.037%
4	6.863	635	642	655	rBV	198647	340667	8.65%	0.842%
5	7.040	665	672	684	rBV	711538	1132707	28.76%	2.801%
6	7.222	696	703	714	rBV	668735	1069242	27.15%	2.644%
7	7.299	714	716	723	rVB6	6857	10549	0.27%	0.026%
8	7.693	776	783	791	rVV	598050	959959	24.38%	2.374%
9	8.051	839	844	848	rBV6	3876	6290	0.16%	0.016%
10	8.393	895	902	915	rBV	541671	904752	22.98%	2.238%
11	8.851	972	980	992	rBV	804695	1310730	33.29%	3.242%
12	8.951	994	997	1003	rVV5	11986	22121	0.56%	0.055%
13	9.022	1007	1009	1014	rVB5	3462	4273	0.11%	0.011%
14	9.228	1042	1044	1048	rVB5	3802	4735	0.12%	0.012%
15	9.563	1093	1101	1115	rBV	604290	1014068	25.75%	2.508%
16	10.092	1184	1191	1205	rBV	885291	1507536	38.28%	3.728%
17	10.469	1245	1255	1266	rBV	794633	1342677	34.10%	3.321%
18	10.622	1273	1281	1302	rBV	689492	1351718	34.33%	3.343%
19	11.281	1386	1393	1394	rBV6	6581	9487	0.24%	0.023%
20	11.651	1453	1456	1461	rVB6	2411	4255	0.11%	0.011%
21	11.822	1479	1485	1494	rBV8	4931	12001	0.30%	0.030%
22	12.075	1522	1528	1535	rBV4	13042	25852	0.66%	0.064%
23	12.228	1550	1554	1559	rBV4	8894	13822	0.35%	0.034%
24	13.233	1719	1725	1731	rVB3	18613	30514	0.77%	0.075%
25	13.310	1733	1738	1742	rBV6	2620	4176	0.11%	0.010%
26	13.757	1807	1814	1824	rBV	1677013	2355084	59.81%	5.824%
27	14.027	1851	1860	1873	rBV	1978201	2823067	71.69%	6.982%
28	14.110	1873	1874	1882	rVB8	2778	5019	0.13%	0.012%
29	14.333	1906	1912	1920	rBV	1075916	1593725	40.47%	3.941%
30	14.422	1925	1927	1932	rVB5	6185	7446	0.19%	0.018%
31	14.557	1944	1950	1965	rBV2	86415	217051	5.51%	0.537%
32	14.892	2004	2007	2012	rVB5	3612	5097	0.13%	0.013%
33	15.198	2056	2059	2063	rVB6	3411	4418	0.11%	0.011%
34	15.333	2075	2082	2091	rBV	2423488	3490855	88.65%	8.633%
35	15.463	2098	2104	2119	rBV	785115	1073073	27.25%	2.654%
36	15.580	2120	2124	2132	rVB6	22931	45384	1.15%	0.112%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044699.D
 Acq On : 21 Mar 2024 13:50
 Operator : MA/JU
 Sample : P1813-04
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0LX4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

37	15.863	2166	2172	2184	rBV	108478	171363	4.35%	0.424%
38	15.963	2186	2189	2194	rBV7	5187	8706	0.22%	0.022%
39	16.057	2200	2205	2207	rBV6	4439	5466	0.14%	0.014%
40	16.121	2213	2216	2221	rBV7	9135	14186	0.36%	0.035%
41	16.204	2226	2230	2232	rVV4	6808	8328	0.21%	0.021%
42	16.304	2245	2247	2251	rVV5	5004	7140	0.18%	0.018%
43	16.380	2254	2260	2268	rBV2	72007	126329	3.21%	0.312%
44	16.510	2277	2282	2288	rVB8	7584	12692	0.32%	0.031%
45	16.774	2322	2327	2332	rVB9	4760	7389	0.19%	0.018%
46	17.092	2374	2381	2390	rBV	1194393	1666374	42.32%	4.121%
47	17.192	2391	2398	2409	rBV	2548927	3576185	90.82%	8.844%
48	17.468	2441	2445	2446	rBV4	2716	4085	0.10%	0.010%
49	17.874	2510	2514	2517	rBV6	7203	10208	0.26%	0.025%
50	17.998	2530	2535	2542	rBV	94929	143622	3.65%	0.355%
51	19.057	2711	2715	2720	rBV2	30354	42760	1.09%	0.106%
52	19.127	2723	2727	2731	rVV	25904	33338	0.85%	0.082%
53	19.286	2751	2754	2763	rVB2	35799	48082	1.22%	0.119%
54	19.492	2783	2789	2797	rBV	2801690	3905921	99.19%	9.660%
55	21.021	3046	3049	3055	rBV3	73859	101905	2.59%	0.252%
56	21.286	3089	3094	3103	rBV	1239594	1599756	40.63%	3.956%
57	23.392	3445	3452	3460	rBV	2206493	3937840	100.00%	9.739%
58	23.527	3469	3475	3487	rVB	912265	1789995	45.46%	4.427%




Sum of corrected areas: 40435604

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044699.D
Acq On : 21 Mar 2024 13:50
Operator : MA/JU
Sample : P1813-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

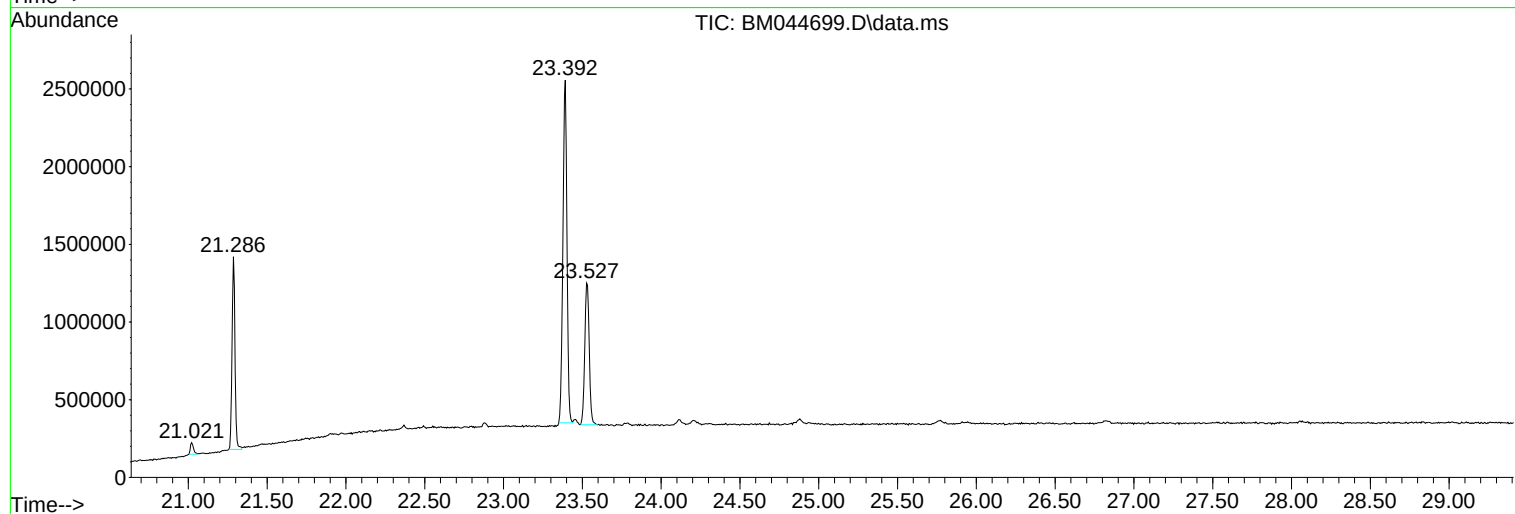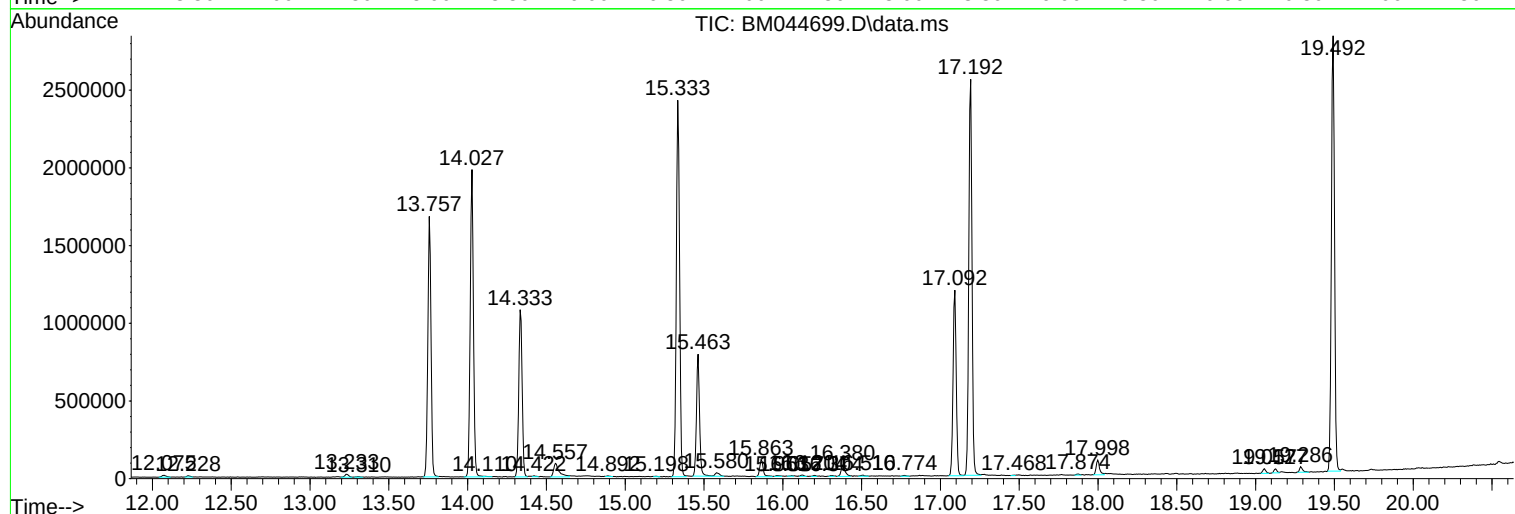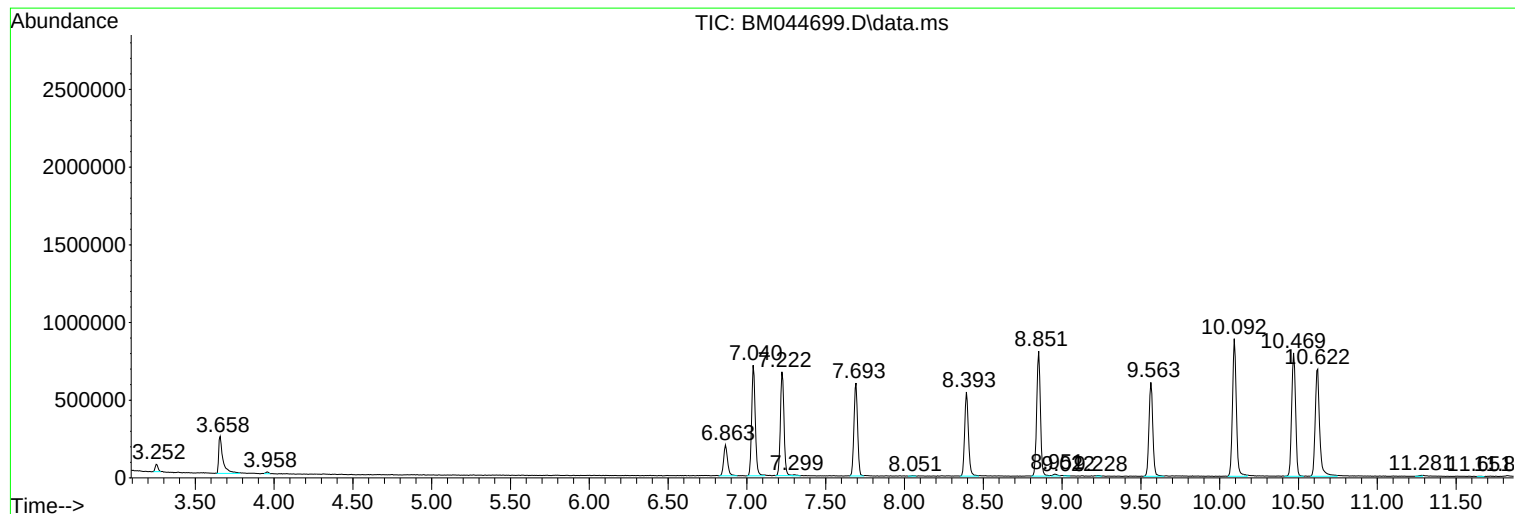

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044699.D
Acq On : 21 Mar 2024 13:50
Operator : MA/JU
Sample : P1813-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EOLX4










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Benzenesulfonamide, N-ethyl... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
15.863	2.06 ng/ul	171363	Phenanthrene-d10	17.092

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Benzenesulfonamide, N-ethyl-2-me...	199	C9H13NO2S	001077-56-1	95
2			4-Toluenesulfonylmethyl isocyanide	195	C9H9NO2S	036635-61-7	50
3			Tolbutamide	270	C12H18N2O3S	000064-77-7	50
4			p-Toluenesulfonylacetonitrile	195	C9H9NO2S	005697-44-9	47
5			(O-p-Tosylisonitroso)malononitrile	249	C10H7N3O3S	020893-01-0	47

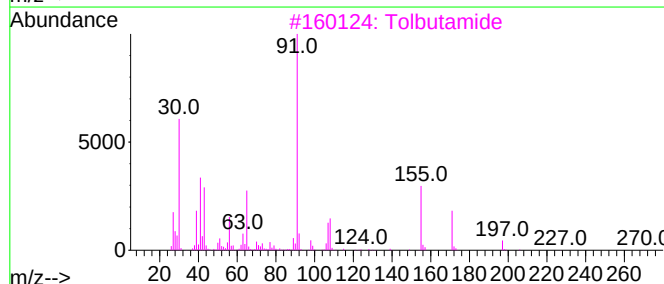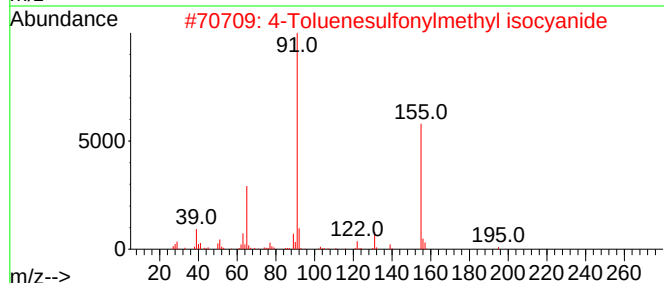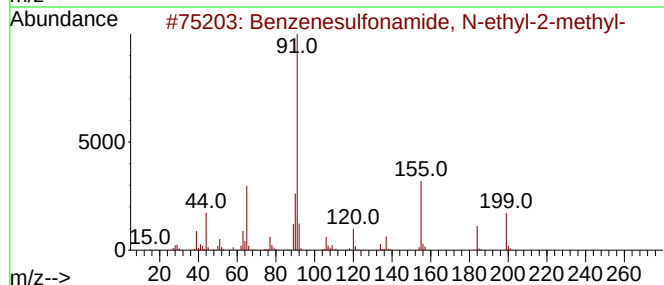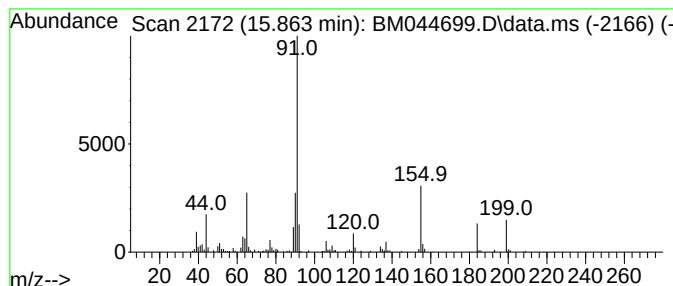

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044699.D
Acq On : 21 Mar 2024 13:50
Operator : MA/JU
Sample : P1813-04
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0LX4

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Benzenesulfonam...	15.863	2.1	ng/ul	171363	4	17.092	1666370	20.0