

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044702.D
 Acq On : 21 Mar 2024 16:10
 Operator : MA/JU
 Sample : PB159719BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK719

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044702.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.251	24	28	36	rVB	62661	86916	2.62%	0.205%
2	3.651	92	96	121	rBV	712587	1204495	36.35%	2.835%
3	3.957	144	148	151	rBV2	11541	13978	0.42%	0.033%
4	4.610	256	259	262	rBV5	2584	3494	0.11%	0.008%
5	5.010	324	327	331	rBV6	2757	4974	0.15%	0.012%
6	6.345	552	554	557	rVB3	3076	3655	0.11%	0.009%
7	6.863	635	642	653	rBV	857230	1381470	41.69%	3.251%
8	7.039	664	672	682	rBV	697023	1138776	34.36%	2.680%
9	7.222	696	703	712	rBV	846392	1354597	40.87%	3.188%
10	7.692	776	783	793	rVB	714534	1146507	34.60%	2.698%
11	7.828	803	806	809	rVB4	2664	3386	0.10%	0.008%
12	8.392	895	902	912	rBV	974323	1610042	48.58%	3.789%
13	8.851	972	980	993	rBV	797406	1312515	39.61%	3.089%
14	9.563	1093	1101	1115	rBV	645410	1081359	32.63%	2.545%
15	10.092	1183	1191	1211	rBV	907619	1576766	47.58%	3.711%
16	10.469	1246	1255	1264	rBV	969087	1616603	48.78%	3.805%
17	10.622	1273	1281	1301	rBV	870513	1647675	49.72%	3.878%
18	12.080	1522	1529	1535	rBV3	11037	23486	0.71%	0.055%
19	13.239	1721	1726	1730	rBV4	9450	14491	0.44%	0.034%
20	13.763	1808	1815	1827	rBV	1420671	2078875	62.73%	4.893%
21	14.027	1853	1860	1871	rBV2	1748869	2572416	77.62%	6.054%
22	14.339	1906	1913	1921	rBV	1358530	1946457	58.73%	4.581%
23	14.551	1942	1949	1973	rBV	440284	910513	27.47%	2.143%
24	14.704	1973	1975	1978	rVB4	4036	4380	0.13%	0.010%
25	14.786	1988	1989	1994	rVB5	3985	5143	0.16%	0.012%
26	15.339	2074	2083	2095	rBV	2078619	3081611	92.99%	7.252%
27	15.462	2098	2104	2118	rVV	636649	902374	27.23%	2.124%
28	15.580	2120	2124	2129	rVB5	8844	13549	0.41%	0.032%
29	16.127	2213	2217	2222	rBV5	6889	10679	0.32%	0.025%
30	16.880	2339	2345	2349	rBV6	4530	7471	0.23%	0.018%
31	17.092	2375	2381	2391	rBV	1481184	2045742	61.73%	4.815%
32	17.192	2391	2398	2415	rVV	2190171	3085130	93.09%	7.261%
33	17.862	2507	2512	2514	rBV5	2369	3737	0.11%	0.009%
34	18.009	2535	2537	2541	rVB5	3236	3353	0.10%	0.008%
35	19.056	2711	2715	2720	rBV3	22208	32532	0.98%	0.077%
36	19.127	2723	2727	2733	rBV	20666	28013	0.85%	0.066%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044702.D
Acq On : 21 Mar 2024 16:10
Operator : MA/JU
Sample : PB159719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK719

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	19.256	2748	2749	2752	rBV3	3470	3749	0.11%	0.009%
38	19.492	2783	2789	2799	rBV	2422166	3226980	97.37%	7.595%
39	21.291	3090	3095	3108	rBV	1457084	1875515	56.59%	4.414%
40	23.391	3445	3452	3461	rBV	1832280	3314007	100.00%	7.799%
41	23.538	3470	3477	3487	rVB	1072335	2113123	63.76%	4.973%




Sum of corrected areas: 42490534

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044702.D
Acq On : 21 Mar 2024 16:10
Operator : MA/JU
Sample : PB159719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

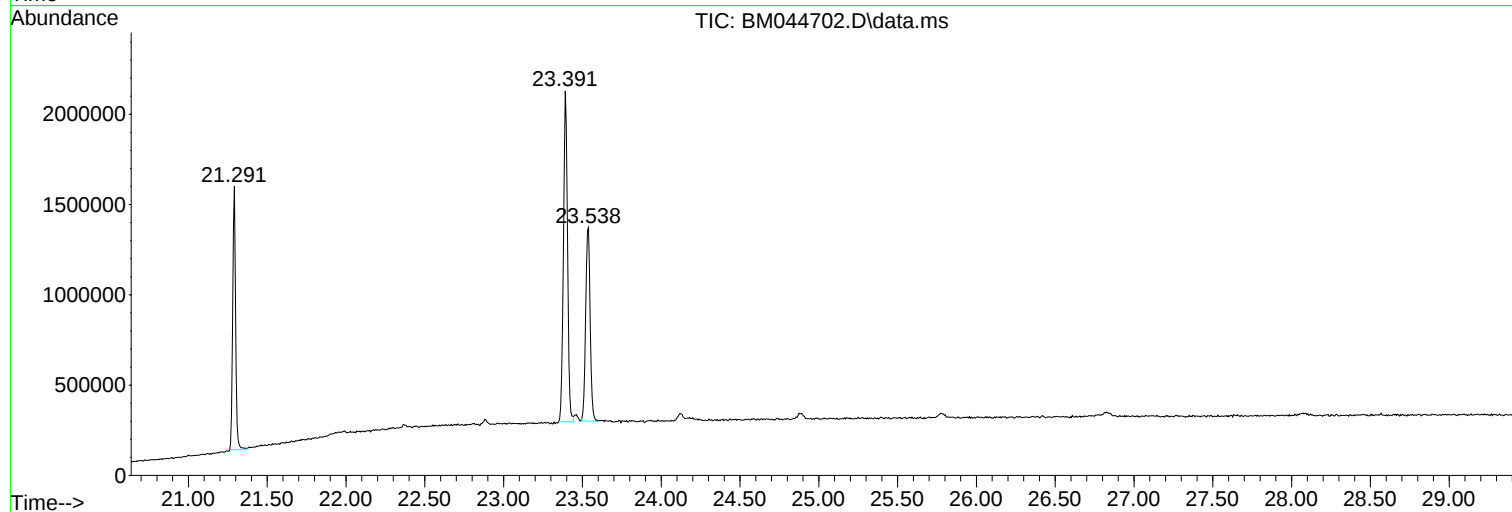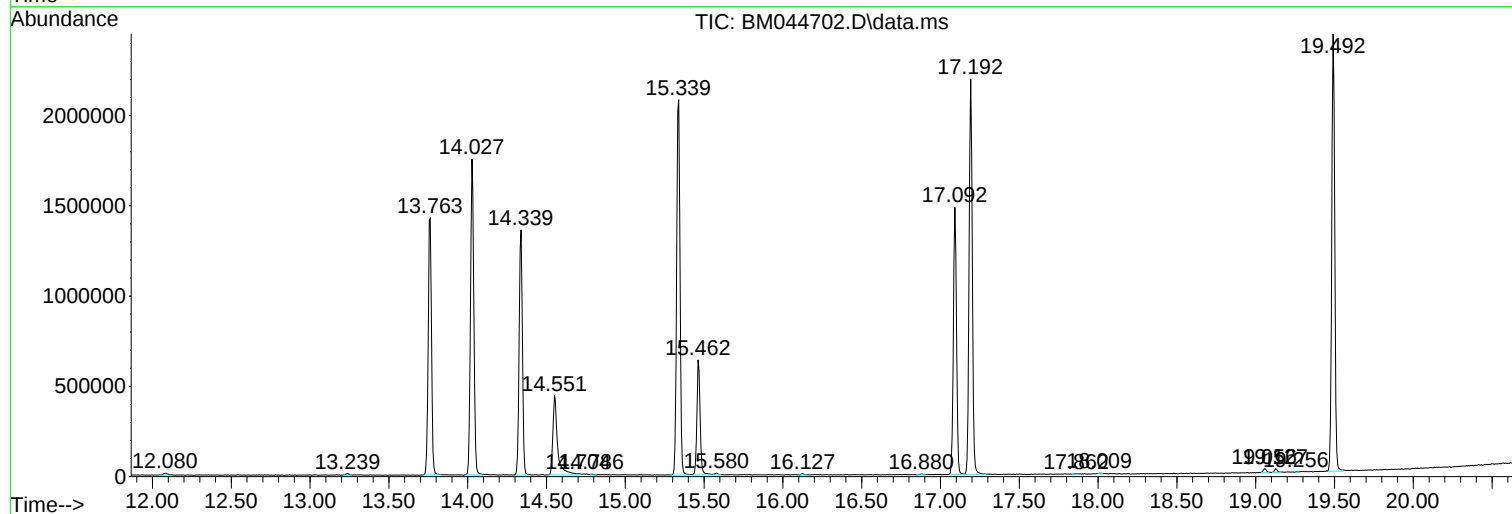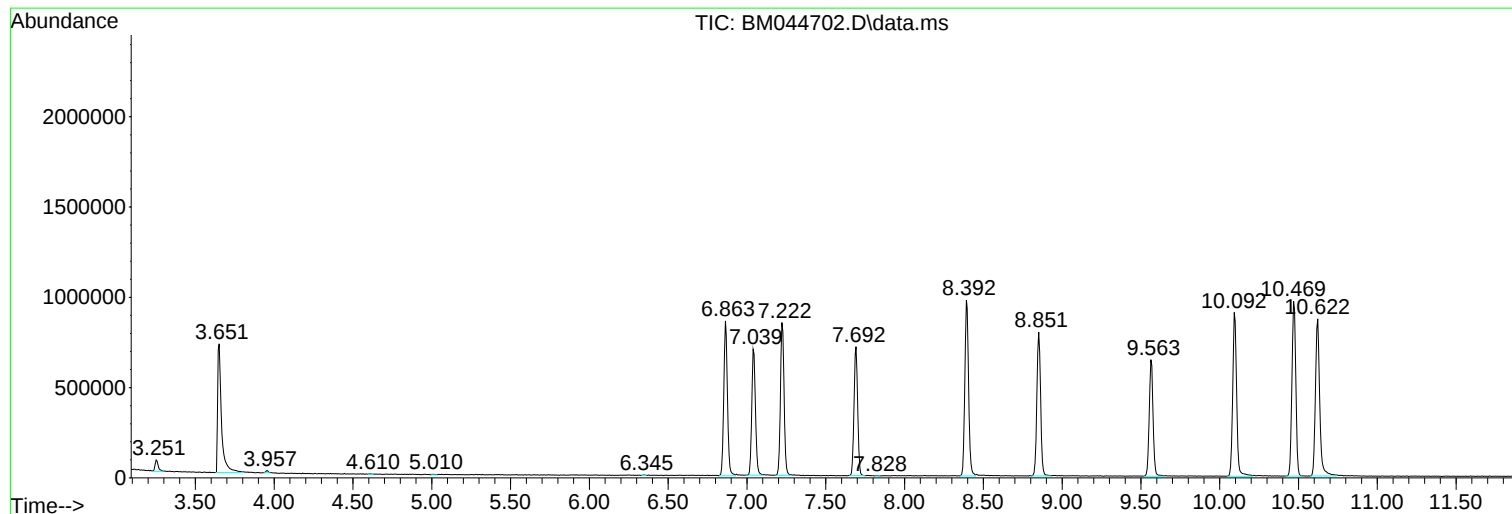

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044702.D
Acq On : 21 Mar 2024 16:10
Operator : MA/JU
Sample : PB159719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044702.D
Acq On : 21 Mar 2024 16:10
Operator : MA/JU
Sample : PB159719BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK719

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc