

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044707.D
 Acq On : 21 Mar 2024 19:18
 Operator : MA/JU
 Sample : P1823-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0779

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044707.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.251	25	28	39	rVB	44511	62472	1.29%	0.134%
2	3.657	94	97	114	rBV	186797	351242	7.25%	0.754%
3	3.951	144	147	152	rVB2	17058	23230	0.48%	0.050%
4	4.316	207	209	214	rVB5	5073	5320	0.11%	0.011%
5	4.875	301	304	307	rVB4	4935	5785	0.12%	0.012%
6	5.710	443	446	450	rVB6	4078	6300	0.13%	0.014%
7	5.775	453	457	463	rBV8	3926	8961	0.19%	0.019%
8	6.863	634	642	652	rBV	196030	366943	7.58%	0.788%
9	7.039	665	672	685	rBV	828755	1310661	27.06%	2.814%
10	7.222	697	703	712	rBV	706881	1170242	24.16%	2.512%
11	7.692	776	783	790	rBV	657174	1084003	22.38%	2.327%
12	8.398	896	903	913	rBV	511844	871263	17.99%	1.870%
13	8.580	930	934	940	rVB5	4944	8357	0.17%	0.018%
14	8.851	972	980	991	rBV	940780	1564863	32.31%	3.360%
15	9.010	1003	1007	1012	rVB6	13642	23757	0.49%	0.051%
16	9.227	1040	1044	1049	rBV4	6479	10207	0.21%	0.022%
17	9.563	1093	1101	1110	rBV	739301	1233166	25.46%	2.647%
18	10.092	1183	1191	1205	rBV	953032	1659091	34.26%	3.562%
19	10.469	1247	1255	1267	rVB	930316	1550859	32.02%	3.329%
20	10.621	1273	1281	1304	rBV	932598	1746314	36.06%	3.749%
21	12.074	1522	1528	1535	rBV	16538	29699	0.61%	0.064%
22	13.233	1720	1725	1730	rBV2	14455	23501	0.49%	0.050%
23	13.757	1808	1814	1824	rBV	1918121	2649224	54.70%	5.688%
24	14.027	1853	1860	1873	rBV	2208688	3239811	66.89%	6.955%
25	14.333	1904	1912	1924	rBV	1241625	1904867	39.33%	4.090%
26	14.568	1945	1952	1963	rBV	67564	180523	3.73%	0.388%
27	15.039	2025	2032	2036	rBV5	6198	10869	0.22%	0.023%
28	15.333	2075	2082	2092	rBV	2671423	3972709	82.02%	8.529%
29	15.462	2098	2104	2119	rBV	890192	1271695	26.26%	2.730%
30	15.574	2119	2123	2129	rVB5	11940	18271	0.38%	0.039%
31	16.121	2211	2216	2220	rBV4	8589	13125	0.27%	0.028%
32	16.874	2341	2344	2348	rBV5	4273	5450	0.11%	0.012%
33	17.092	2374	2381	2391	rBV	1419288	2032068	41.96%	4.363%
34	17.192	2391	2398	2408	rBV	2964144	4293031	88.64%	9.217%
35	17.392	2427	2432	2433	rBV5	3394	4990	0.10%	0.011%
36	17.492	2445	2449	2453	rBV6	5311	9189	0.19%	0.020%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044707.D
 Acq On : 21 Mar 2024 19:18
 Operator : MA/JU
 Sample : P1823-01
 Misc :
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 E0779

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

37	17.780	2493	2498	2502	rVB	15966	22792	0.47%	0.049%
38	17.939	2522	2525	2530	rVB7	6139	8028	0.17%	0.017%
39	18.003	2530	2536	2541	rBV4	21463	37631	0.78%	0.081%
40	18.256	2574	2579	2583	rBV8	2846	6073	0.13%	0.013%
41	18.862	2680	2682	2686	rVB5	4973	5270	0.11%	0.011%
42	19.056	2710	2715	2719	rBV2	35196	54807	1.13%	0.118%
43	19.097	2719	2722	2724	rVV4	12048	14906	0.31%	0.032%
44	19.127	2724	2727	2732	rVB2	28330	35092	0.72%	0.075%
45	19.292	2751	2755	2761	rBV8	15137	26546	0.55%	0.057%
46	19.492	2783	2789	2799	rBV	3417761	4626010	95.51%	9.931%
47	21.291	3089	3095	3102	rBV	1443387	1989958	41.09%	4.272%
48	23.391	3445	3452	3460	rBV2	2577575	4843301	100.00%	10.398%
49	23.532	3470	3476	3487	rVB	1141258	2186902	45.15%	4.695%




Sum of corrected areas: 46579374

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044707.D
Acq On : 21 Mar 2024 19:18
Operator : MA/JU
Sample : P1823-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0779

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

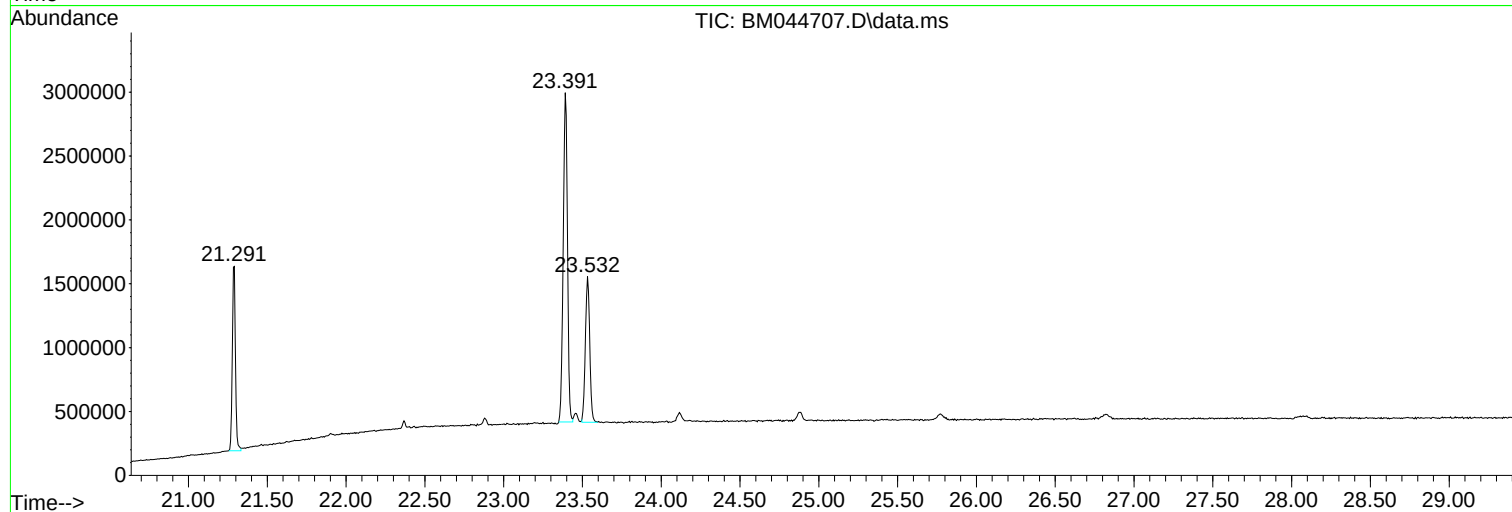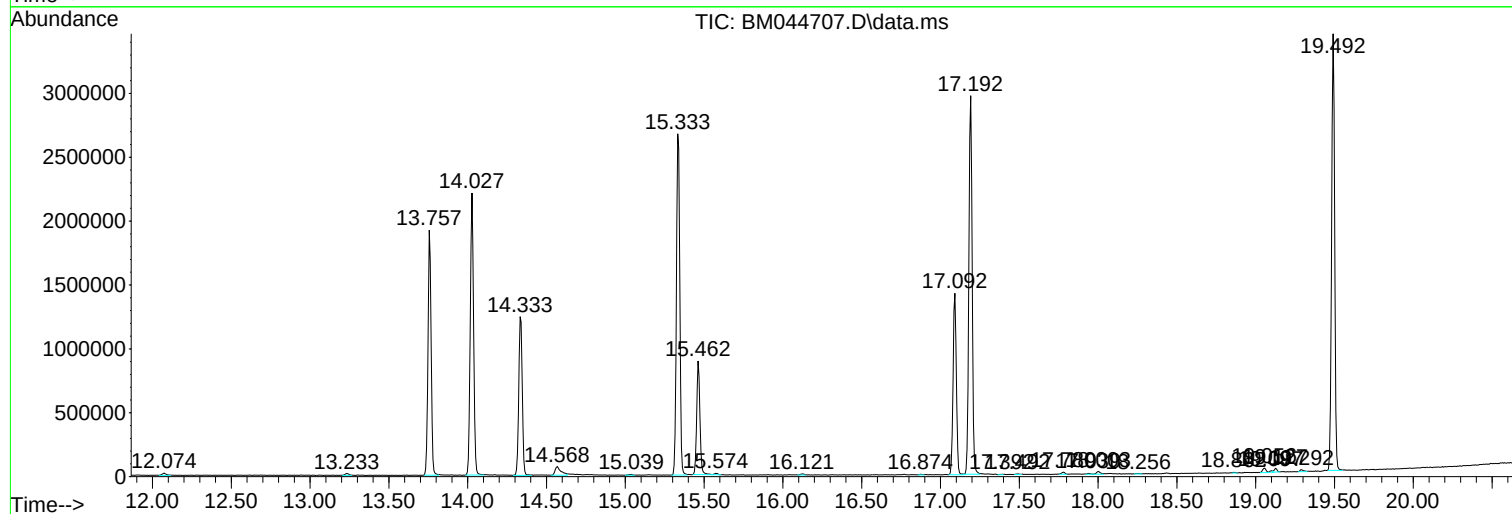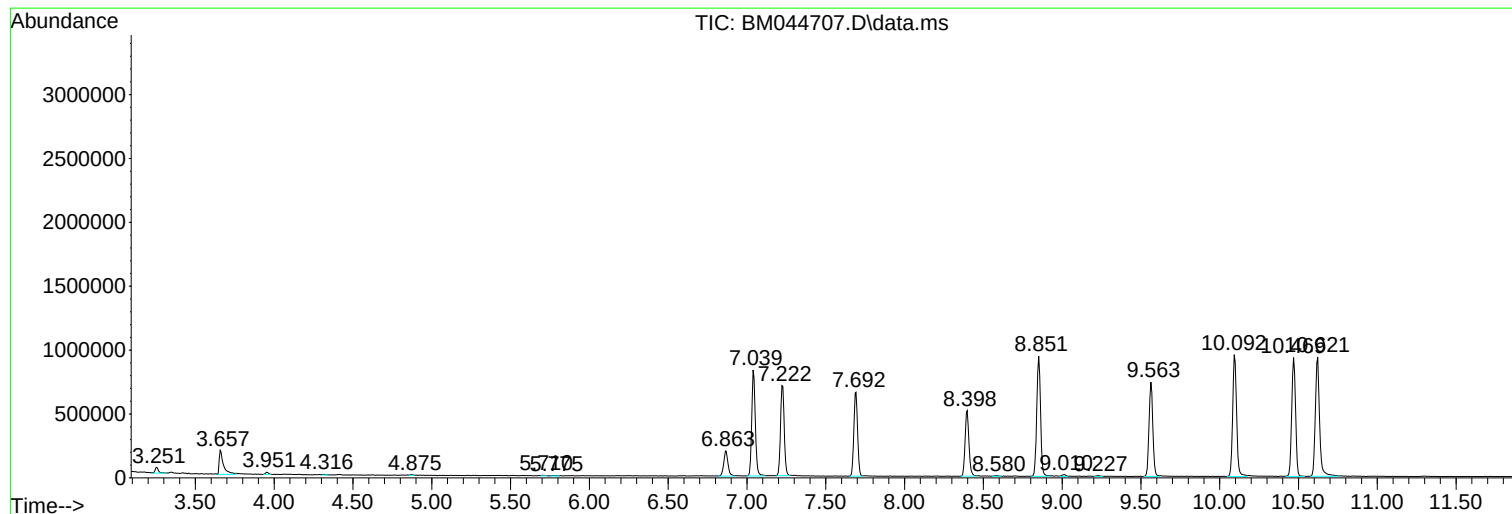

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044707.D
Acq On : 21 Mar 2024 19:18
Operator : MA/JU
Sample : P1823-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0779

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044707.D
Acq On : 21 Mar 2024 19:18
Operator : MA/JU
Sample : P1823-01
Misc :
ALS Vial : 8 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
E0779

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------