

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
 Data File : BM044710.D
 Acq On : 21 Mar 2024 21:07
 Operator : MA/JU
 Sample : PB159721BL
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SBLK721

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0.1 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
 Title : SVOA CALIBRATION

Signal : TIC: BM044710.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	3.252	25	28	37	rVB	58331	82856	2.48%	0.203%
2	3.652	93	96	119	rBV	671749	1096725	32.81%	2.683%
3	3.952	144	147	152	rVB2	10753	15571	0.47%	0.038%
4	4.534	243	246	248	rBV3	3578	4586	0.14%	0.011%
5	6.863	636	642	660	rVB	785837	1281696	38.35%	3.136%
6	7.040	666	672	686	rBV	675257	1063587	31.82%	2.602%
7	7.222	696	703	713	rBV	802245	1280352	38.31%	3.132%
8	7.687	775	782	792	rBV	641242	1051194	31.45%	2.572%
9	8.393	895	902	916	rBV	923615	1548769	46.34%	3.789%
10	8.851	970	980	993	rBV	739507	1253849	37.51%	3.067%
11	9.563	1092	1101	1109	rBV	621960	1028518	30.77%	2.516%
12	10.093	1183	1191	1206	rBV	852015	1502642	44.96%	3.676%
13	10.469	1247	1255	1263	rBV	887174	1488143	44.52%	3.641%
14	10.616	1272	1280	1298	rBV	817922	1592773	47.65%	3.897%
15	12.081	1521	1529	1537	rBV3	9879	24260	0.73%	0.059%
16	13.233	1716	1725	1729	rBV5	7635	13865	0.41%	0.034%
17	13.757	1807	1814	1826	rBV	1451712	2028728	60.70%	4.963%
18	14.028	1853	1860	1872	rBV2	1656173	2535606	75.86%	6.203%
19	14.333	1905	1912	1924	rBV	1226650	1826873	54.66%	4.469%
20	14.557	1943	1950	1976	rBV	372773	875669	26.20%	2.142%
21	14.751	1981	1983	1987	rVV5	4878	7566	0.23%	0.019%
22	15.333	2075	2082	2092	rBV	2073817	3027018	90.56%	7.405%
23	15.463	2098	2104	2116	rBV	590903	836506	25.03%	2.046%
24	15.580	2120	2124	2127	rVB3	8220	11084	0.33%	0.027%
25	16.122	2212	2216	2221	rVB6	8032	11816	0.35%	0.029%
26	16.769	2322	2326	2331	rVB7	3064	4604	0.14%	0.011%
27	16.880	2340	2345	2347	rBV5	3441	5035	0.15%	0.012%
28	16.951	2353	2357	2360	rVB6	2470	3724	0.11%	0.009%
29	17.092	2374	2381	2389	rBV	1313359	1911471	57.19%	4.676%
30	17.186	2391	2397	2418	rVB2	2045410	3042895	91.04%	7.444%
31	17.433	2436	2439	2442	rBV5	2460	3728	0.11%	0.009%
32	18.021	2535	2539	2542	rBV6	2648	4116	0.12%	0.010%
33	19.057	2710	2715	2720	rVB2	24310	35572	1.06%	0.087%
34	19.127	2723	2727	2731	rBV2	18668	26623	0.80%	0.065%
35	19.492	2783	2789	2797	rBV	2330619	3172697	94.92%	7.762%
36	21.286	3089	3094	3104	rBV	1317293	1809075	54.12%	4.426%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044710.D
Acq On : 21 Mar 2024 21:07
Operator : MA/JU
Sample : PB159721BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0.1 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Title : SVOA CALIBRATION

37	23.392	3445	3452	3460	rBV2	1773053	3342447	100.00%	8.177%
38	23.533	3469	3476	3484	rBV	1071422	2024094	60.56%	4.952%




Sum of corrected areas: 40876333

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044710.D
Acq On : 21 Mar 2024 21:07
Operator : MA/JU
Sample : PB159721BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

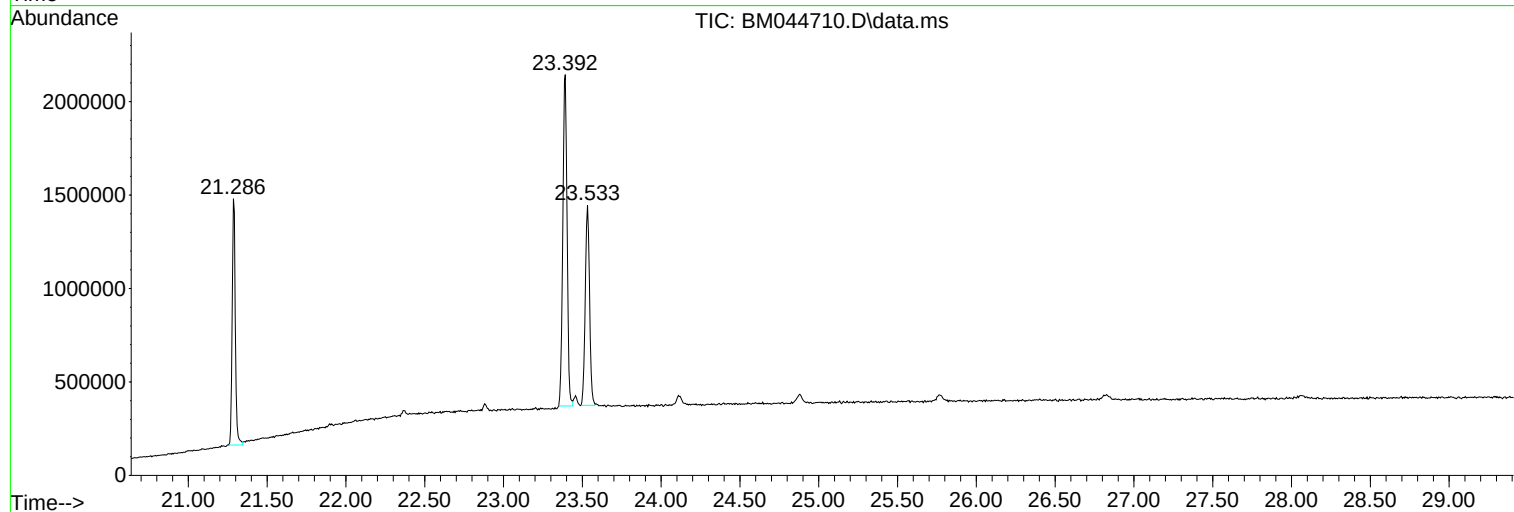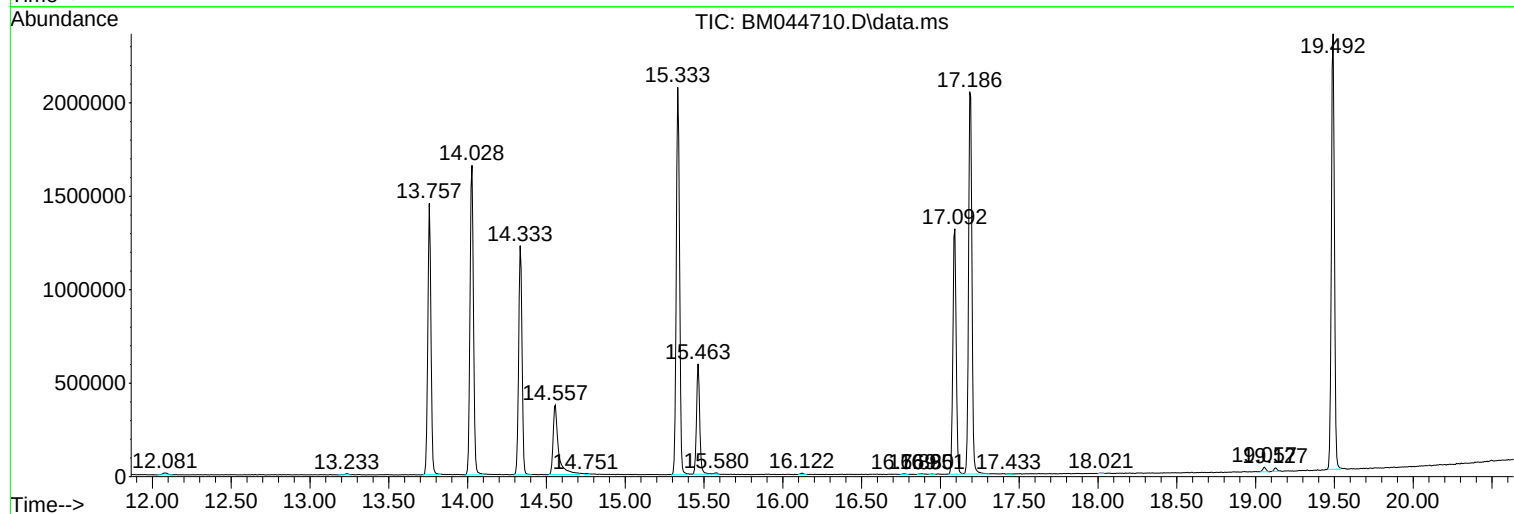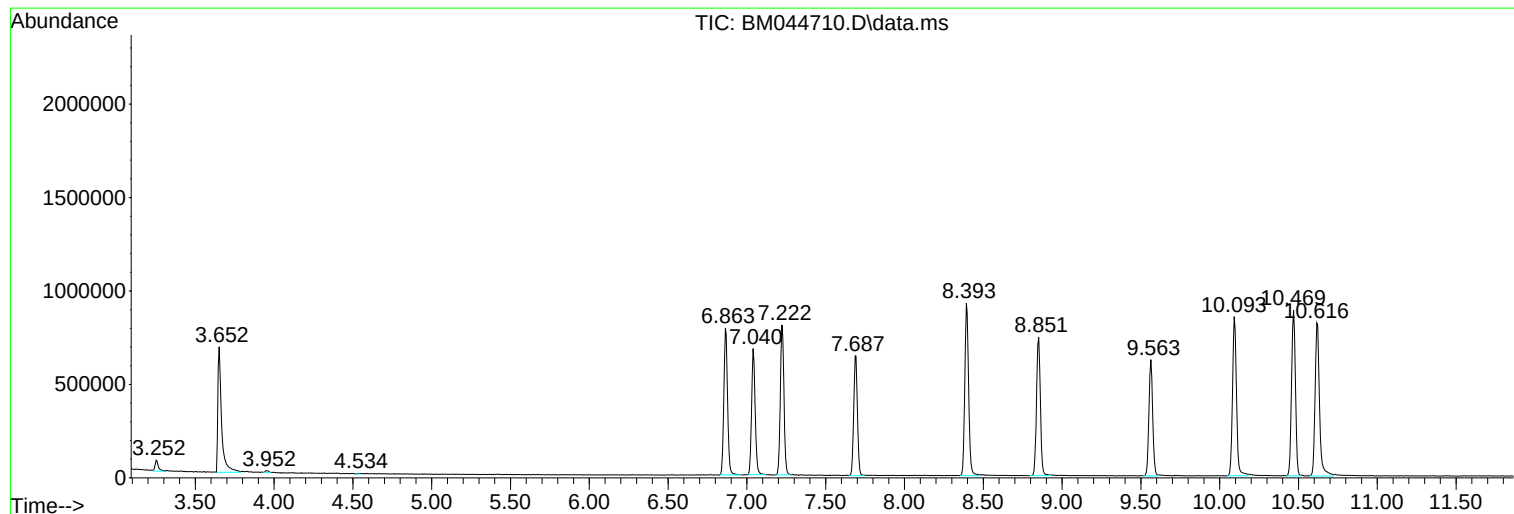

Library Search Compound Report

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044710.D
Acq On : 21 Mar 2024 21:07
Operator : MA/JU
Sample : PB159721BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032124\
Data File : BM044710.D
Acq On : 21 Mar 2024 21:07
Operator : MA/JU
Sample : PB159721BL
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SBLK721

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\SFAM-EPA-BM030524.MA.M
Quant Title : SVOA CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------