

Quantitation Report (Qedit)




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032216\
 Data File : BM004727.D
 Acq On : 22 Mar 2016 13:41
 Operator : UM/SJ
 Sample : SSTD3.262
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD3.262

Manual Integrations
 APPROVED

Sohil
 3/23/2016 12:13:07 PM

Quant Time: Mar 22 14:18:14 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 22 13:28:23 2016
 Response via : Initial Calibration

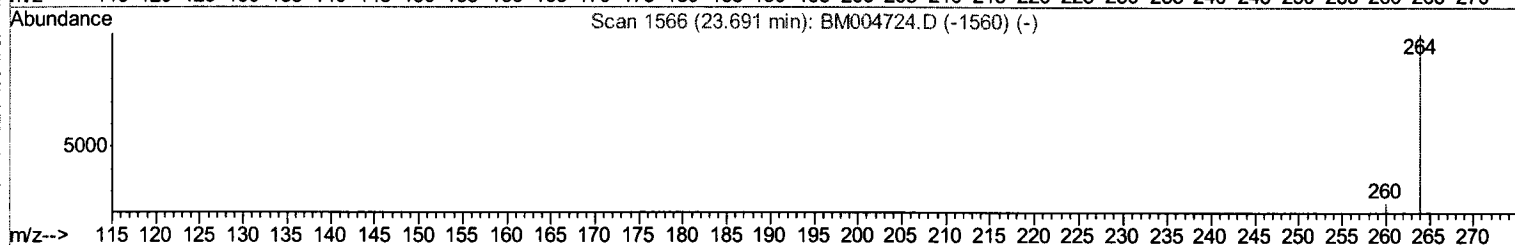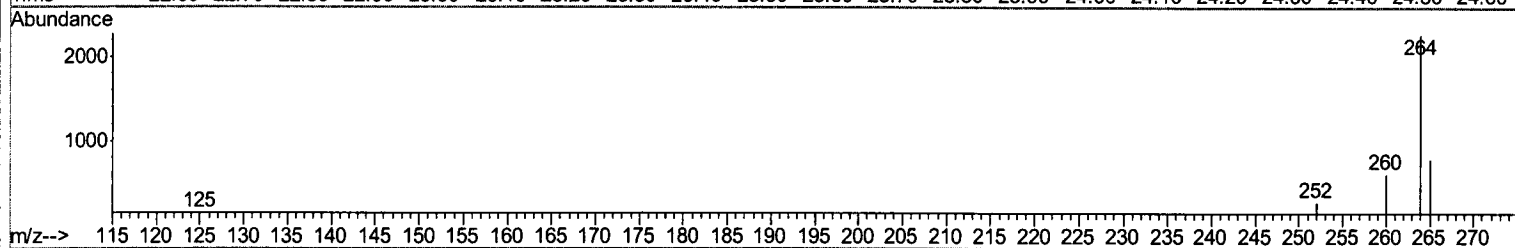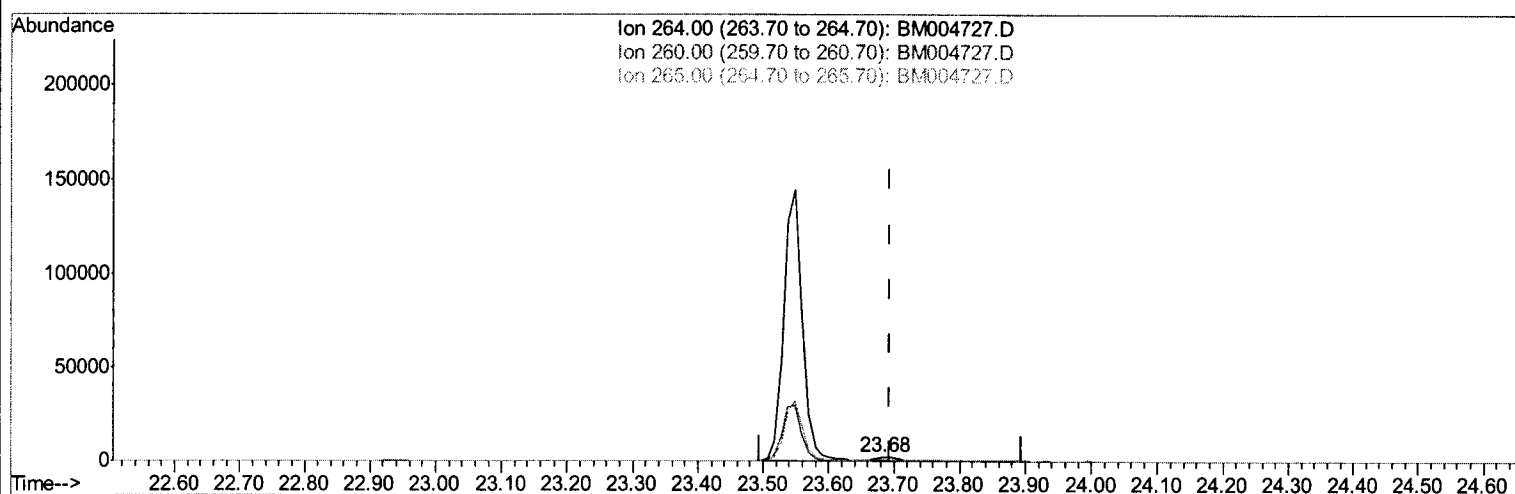

TIC: BM004727.D

(22) Perylene-d12 (I)

23.684min (-0.010) 0.40ng/ul m

response 5972

U.M
 04/05/16

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	27.46
265.00	38.20	34.95
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032216\
Data File : BM004727.D
Acq On : 22 Mar 2016 13:41
Operator : UM/SJ
Sample : SSTD3.262
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD3.262

Manual Integrations
APPROVED

Sohil
3/23/2016 12:13:07 PM

Quant Time: Mar 22 14:18:14 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 13:28:23 2016
Response via : Initial Calibration

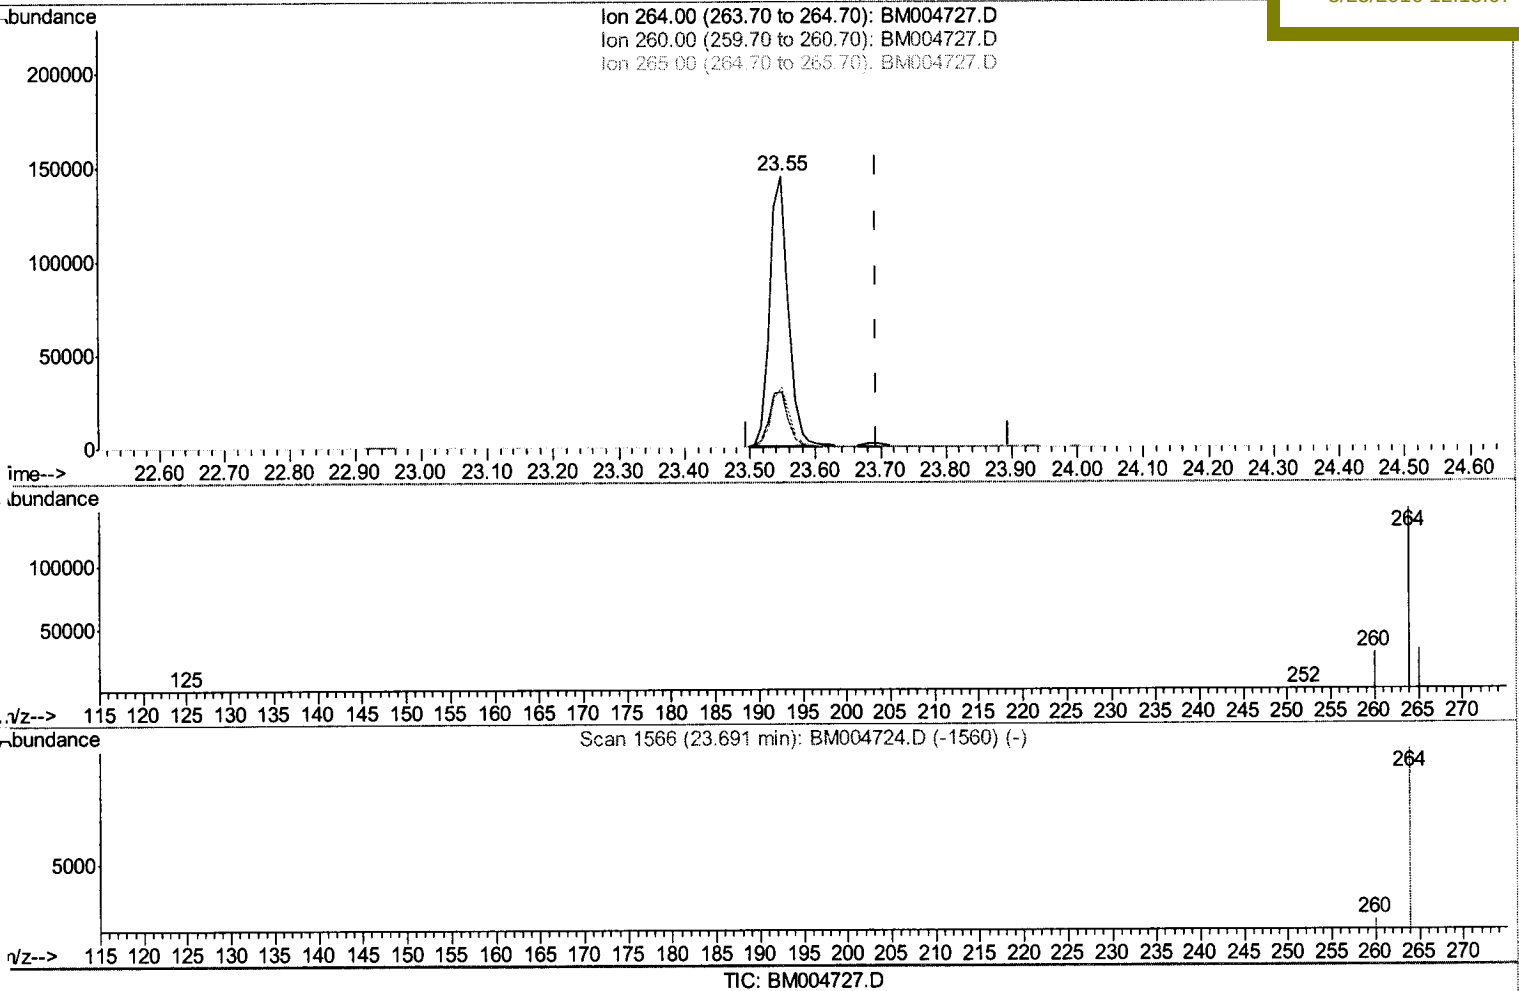

(22) Perylene-d12 (I)

23.548min (-0.146) 0.40ng/ul

response 283459

Ion	Exp%	Act%
264.00	100	100
260.00	25.60	20.53
265.00	38.20	22.14#
0.00	0.00	0.00

Quantitation Report (Qedit)


Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032216\
 Data File : BM004727.D
 Acq On : 22 Mar 2016 13:41
 Operator : UM/SJ
 Sample : SSTD3.262
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD3.262

Manual Integrations
 APPROVED

Sohil
 3/23/2016 12:13:07 PM

Quant Time: Mar 22 14:18:14 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 22 13:28:23 2016
 Response via : Initial Calibration

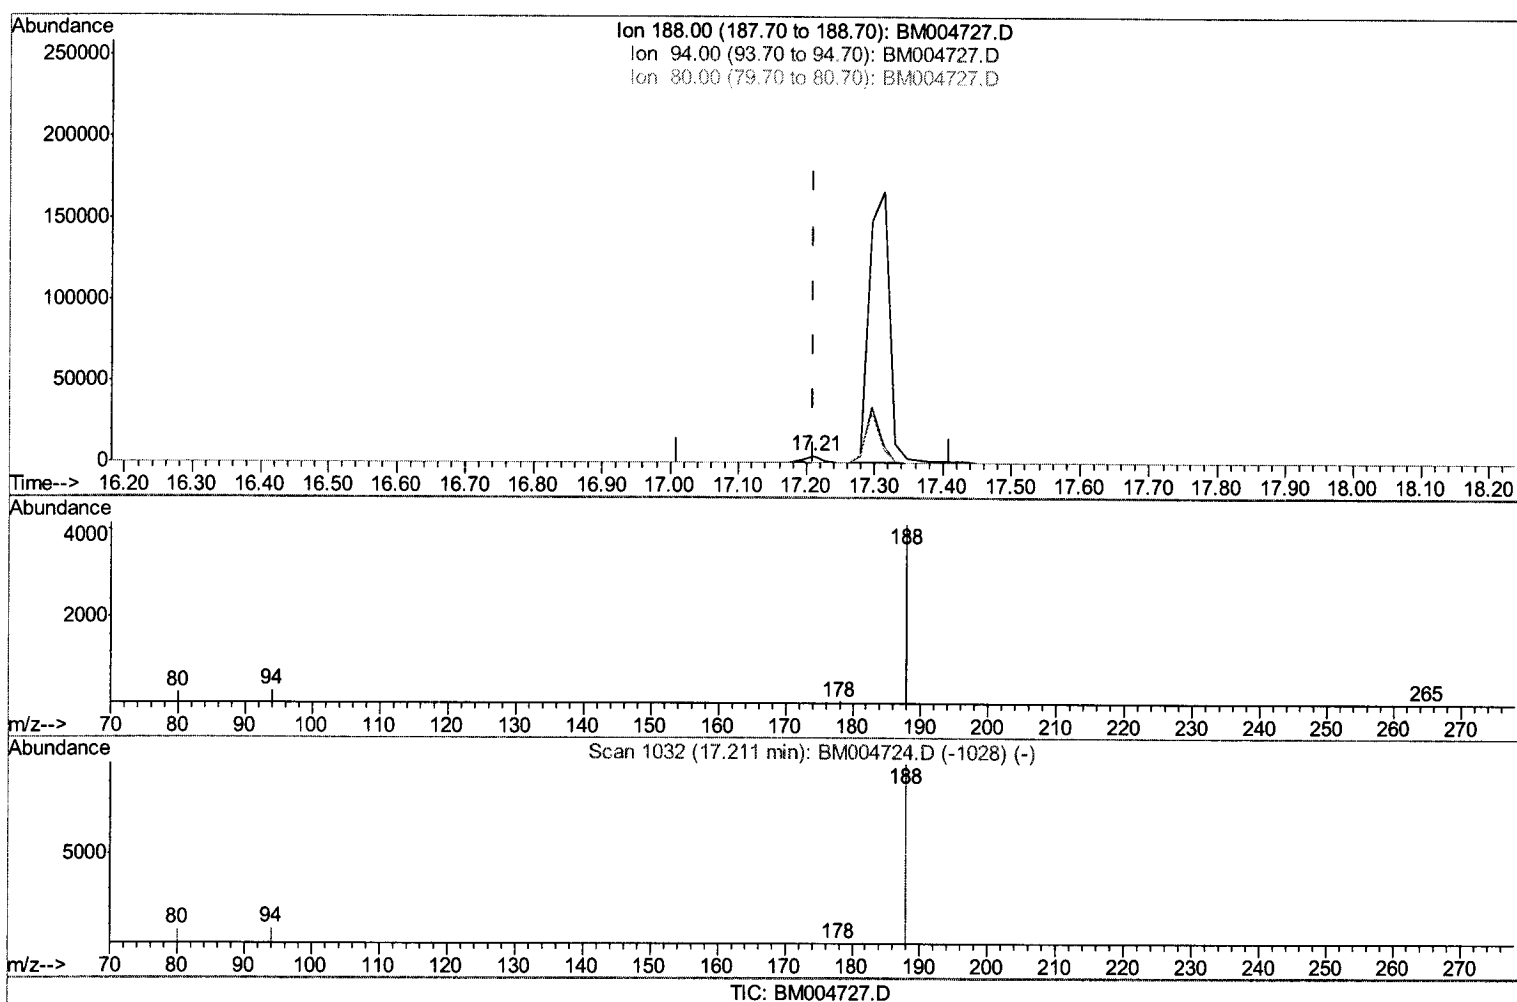

(12) Phenanthrene-d10 (I)

17.210min (-0.000) 0.40ng/ul m

response 6464

> U.M
 04/05/16

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	7.96#
80.00	11.90	7.14#
0.00	0.00	0.00




Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032216\
Data File : BM004727.D
Acq On : 22 Mar 2016 13:41
Operator : UM/SJ
Sample : SSTD3.262
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
SSTD3.262

Quant Time: Mar 22 14:18:14 2016
Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Mar 22 13:28:23 2016
Response via : Initial Calibration

Manual Integrations
APPROVED

Sohil
3/23/2016 12:13:07 PM

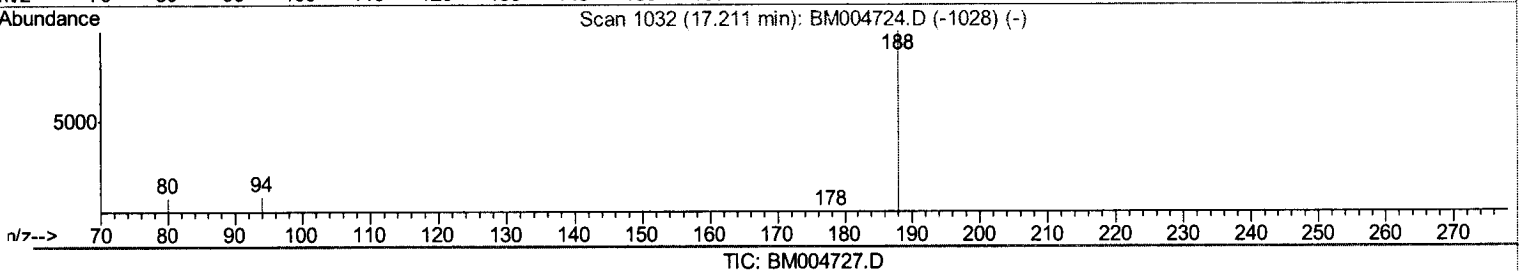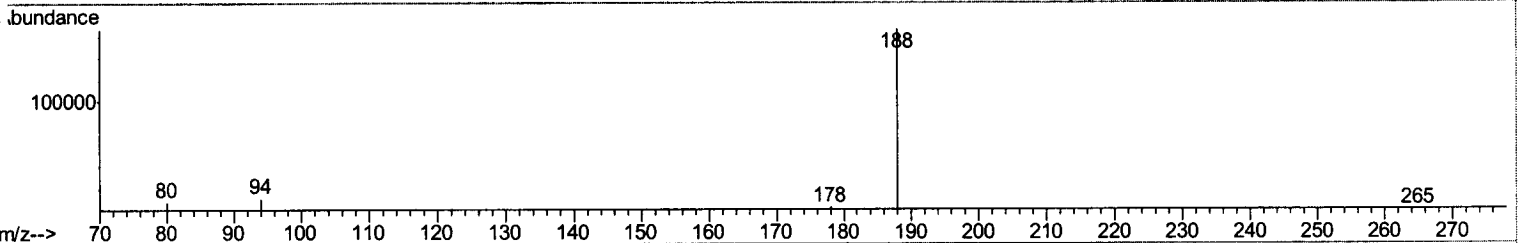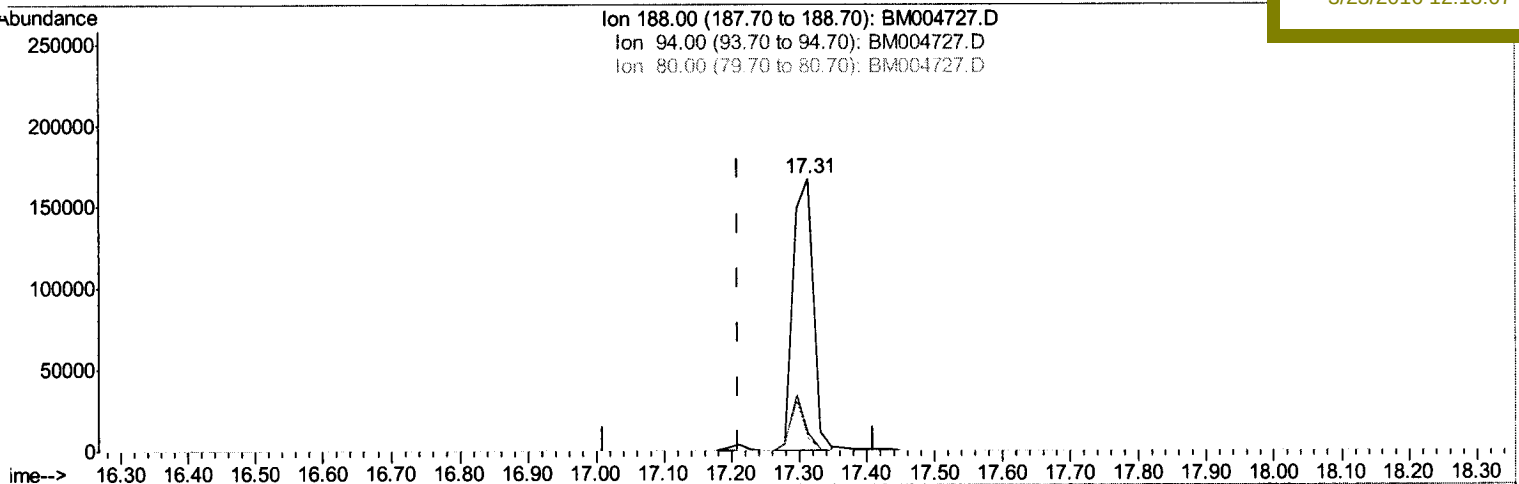

(12) Phenanthrene-d10 (I)

17.313min (+0.103) 0.40ng/ul

response 342104

Ion	Exp%	Act%
188.00	100	100
94.00	11.70	6.40#
80.00	11.90	4.36#
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032216\
 Data File : BM004727.D
 Acq On : 22 Mar 2016 13:41
 Operator : UM/SJ
 Sample : SSTD3.262
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD3.262

Quant Time: Mar 22 14:22:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 22 13:28:23 2016
 Response via : Initial Calibration

Manual Integrations
 APPROVED

Sohil
 3/23/2016 12:13:07 PM

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1714	0.40	ng/ul	0.00
4) Naphthalene-d8	10.62	136	7119	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.47	164	3558	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.21	188	6464m	0.40	ng/ul	0.00
18) Chrysene-d12	21.39	240	5926	0.40	ng/ul	-0.01
22) Perylene-d12	23.68	264	5972m	0.40	ng/ul	-0.01

System Monitoring Compounds

2) 1,4-Dioxane-d8	0.00	96	0d	0.00	ng/uL
6) 2-Methylnaphthalene-d10	0.00	152	0d	0.00	ng/ul
16) Fluoranthene-d10	0.00	212	0d	0.00	ng/ul

Target Compounds

					Qvalue
13) Pentachlorophenol	16.85	266	3629	6.80	ng/ul 96

(#) = qualifier out of range (m) = manual integration (+) = signals summed

U.M
 04/05/16

Quantitation Report (QT Reviewed)

Data Path : Z:\HPCHEM1\BNA_M\DATA\BM032216\
 Data File : BM004727.D
 Acq On : 22 Mar 2016 13:41
 Operator : UM/SJ
 Sample : SSTD3.262
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 SSTD3.262

Manual Integrations
 APPROVED

Sohil
 3/23/2016 12:13:07 PM

Quant Time: Mar 22 14:22:41 2016
 Quant Method : Z:\HPCHEM1\BNA_M\METHODS\SOM-EPA-SIM-BM032216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Mar 22 13:28:23 2016
 Response via : Initial Calibration

