

Data Path : Z:\HPCHEM1\BNA M\DATA\BM032216\
 Data File : BM004742.D
 Acq On : 23 Mar 2016 00:44
 Operator : UM/SJ
 Sample : H1835-18
 Misc :
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T29

Manual Integrations
 APPROVED

Sohil
 4/5/2016 5:21:12 PM

Quant Time: Apr 05 16:34:11 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 15:47:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1409	0.40	ng/ul	0.00
4) Naphthalene-d8	10.62	136	5769	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.47	164	2947	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.21	188	5608m	0.40	ng/ul	0.00
18) Chrysene-d12	21.39	240	4347	0.40	ng/ul	-0.02
22) Perylene-d12	23.68	264	3240m	0.40	ng/ul	-0.02
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.32	96	1868	0.55	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.22	152	2308	0.35	ng/ul	0.00
16) Fluoranthene-d10	19.23	212	5082	0.45	ng/ul	0.00
Target Compounds						Ovalue
13) Pentachlorophenol	16.87	266	54	0.07	ng/ul#	78

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM032216\
Data File : BM004742.D
Acq On : 23 Mar 2016 00:44
Operator : UM/SJ
Sample : H1835-18
Misc :
ALS Vial : 20 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4T29

Manual Integrations
APPROVED

Sohil
4/5/2016 5:21:12 PM

Quant Time: Apr 05 16:34:11 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 15:47:13 2016
Response via : Initial Calibration

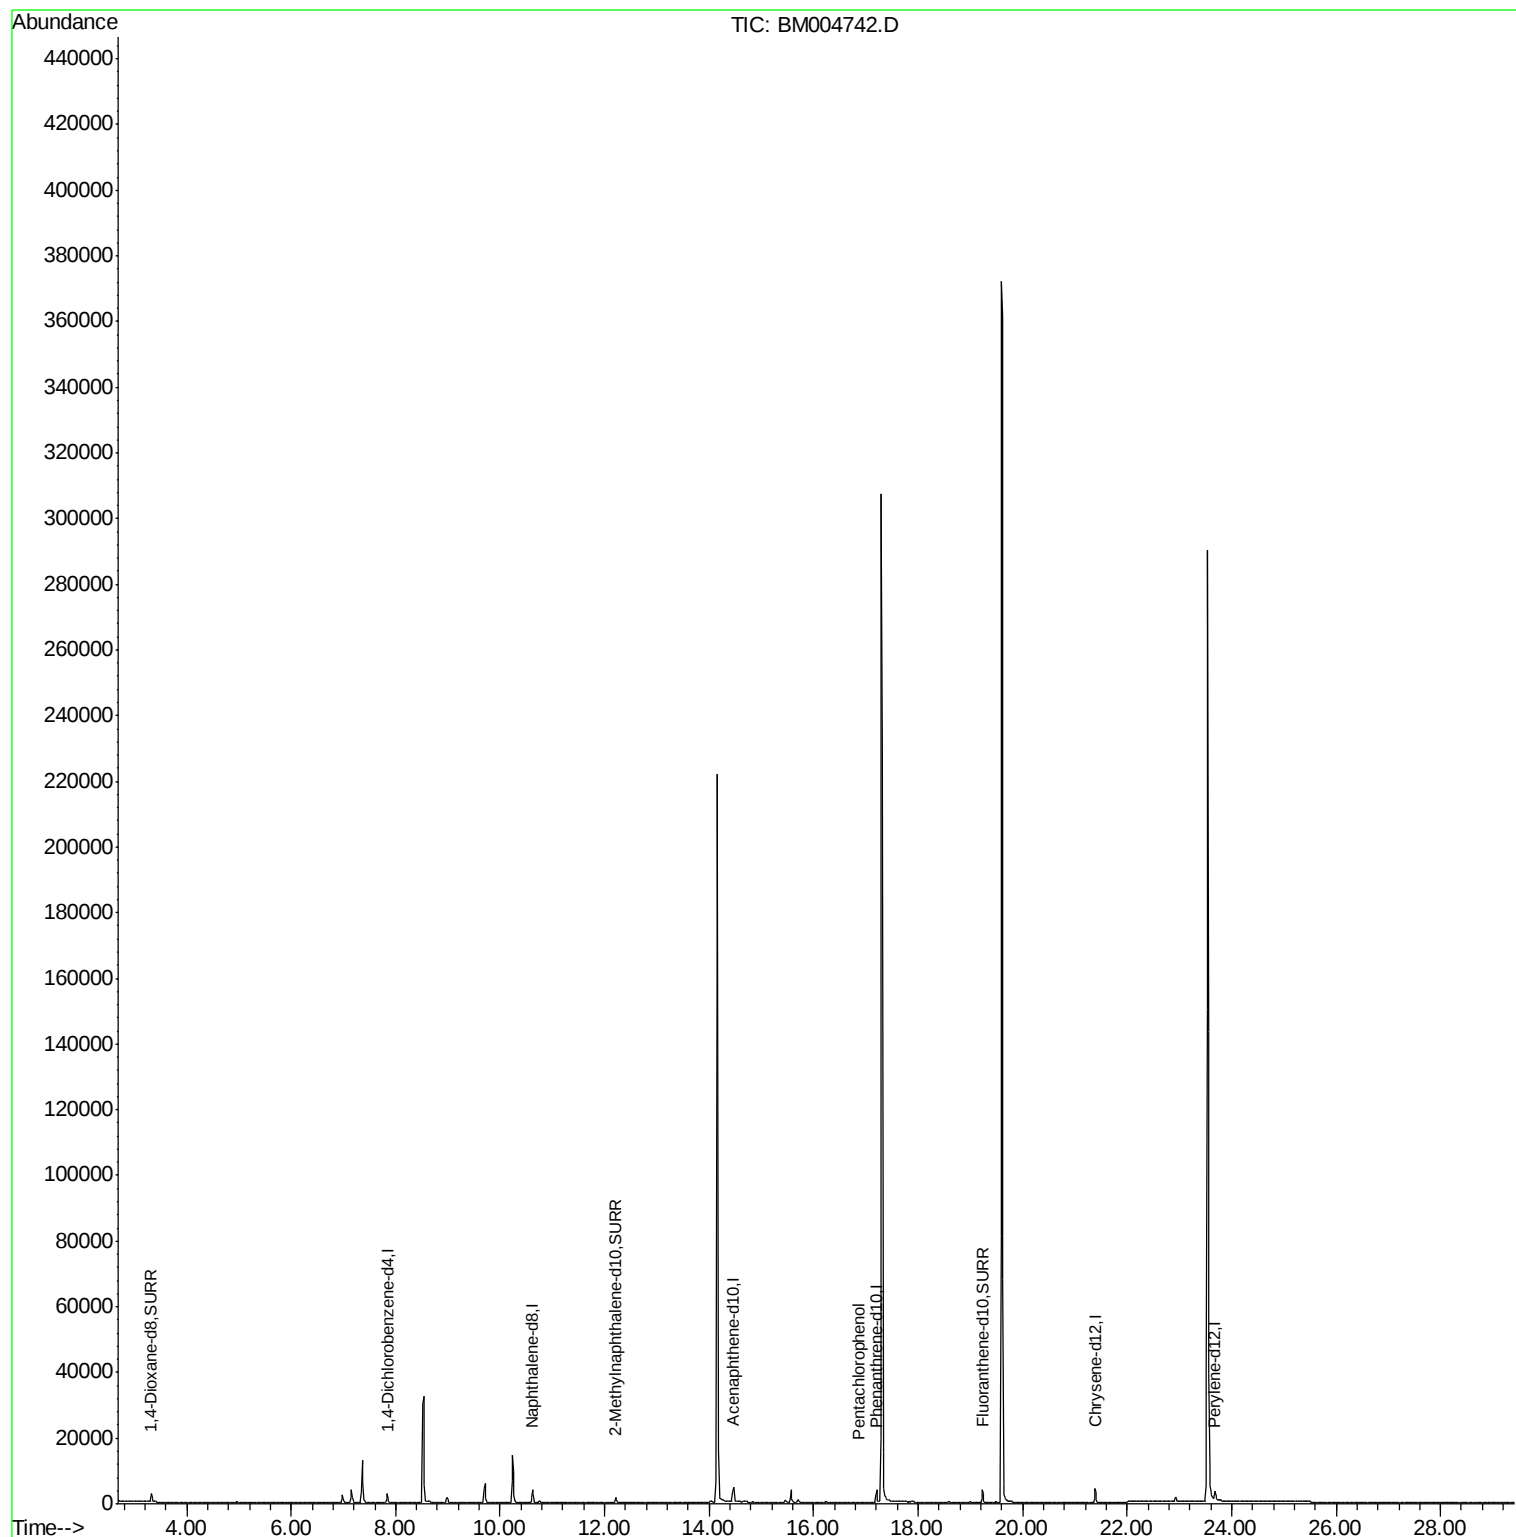

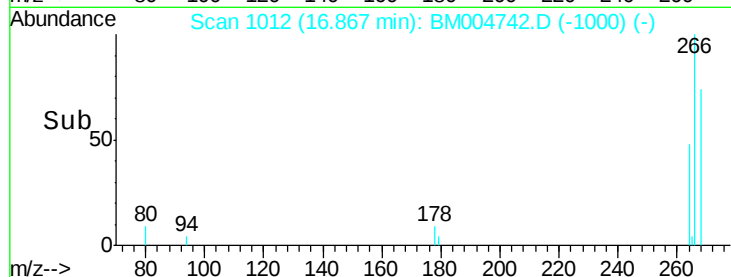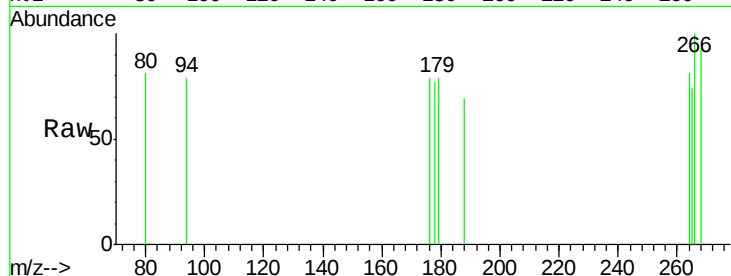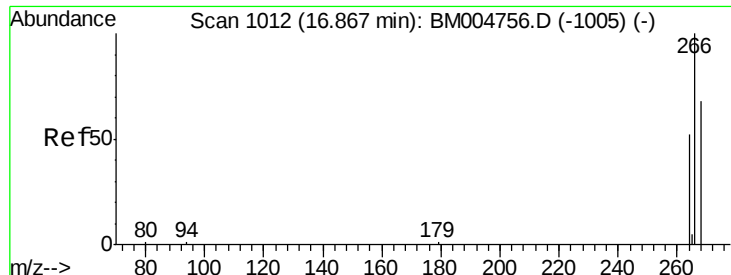

#13
 Pentachlorophenol
 Concen: 0.07 ng/ul
 RT: 16.87 min Scan# 1012
 Delta R.T. 0.00 min
 Lab File: BM004742.D
 Acq: 23 Mar 2016 00:44

Instrument :
 BNA_M
 ClientSampleId :
 A4T29

Tot Ion	Ratio	Lower	Upper
266	100		
264	79.6	51.8	77.8#
268	77.8	46.8	70.2#

Manual Integrations
 APPROVED

Sohil
 4/5/2016 5:21:12 PM

