

Data Path : Z:\HPCHEM1\BNA M\DATA\BM032216\
 Data File : BM004746.D
 Acq On : 23 Mar 2016 03:08
 Operator : UM/SJ
 Sample : H1835-23
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 A4T34

Manual Integrations
 APPROVED

Sohil
 4/5/2016 5:21:17 PM

Quant Time: Apr 05 16:28:39 2016
 Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032216.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Tue Apr 05 15:47:13 2016
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) 1,4-Dichlorobenzene-d4	7.84	152	1255	0.40	ng/ul	0.00
4) Naphthalene-d8	10.62	136	5112	0.40	ng/ul	0.00
8) Acenaphthene-d10	14.47	164	2716	0.40	ng/ul	0.00
12) Phenanthrene-d10	17.21	188	5341m	0.40	ng/ul	0.00
18) Chrysene-d12	21.40	240	4607	0.40	ng/ul	-0.01
22) Perylene-d12	23.69	264	3115m	0.40	ng/ul	-0.01
System Monitoring Compounds						
2) 1,4-Dioxane-d8	3.32	96	1917	0.63	ng/uL	0.00
6) 2-Methylnaphthalene-d10	12.22	152	2219	0.38	ng/ul	0.00
16) Fluoranthene-d10	19.24	212	4931	0.46	ng/ul	0.00
Target Compounds						Ovalue
13) Pentachlorophenol	16.87	266	52	0.07	ng/ul#	81

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\HPCHEM1\BNA M\DATA\BM032216\
Data File : BM004746.D
Acq On : 23 Mar 2016 03:08
Operator : UM/SJ
Sample : H1835-23
Misc :
ALS Vial : 24 Sample Multiplier: 1




Instrument :
BNA_M
ClientSampleId :
A4T34

Manual Integrations
APPROVED

Sohil
4/5/2016 5:21:17 PM

Quant Time: Apr 05 16:28:39 2016
Quant Method : Z:\HPCHEM1\BNA M\METHODS\SOM-EPA-SIM-BM032216.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Tue Apr 05 15:47:13 2016
Response via : Initial Calibration

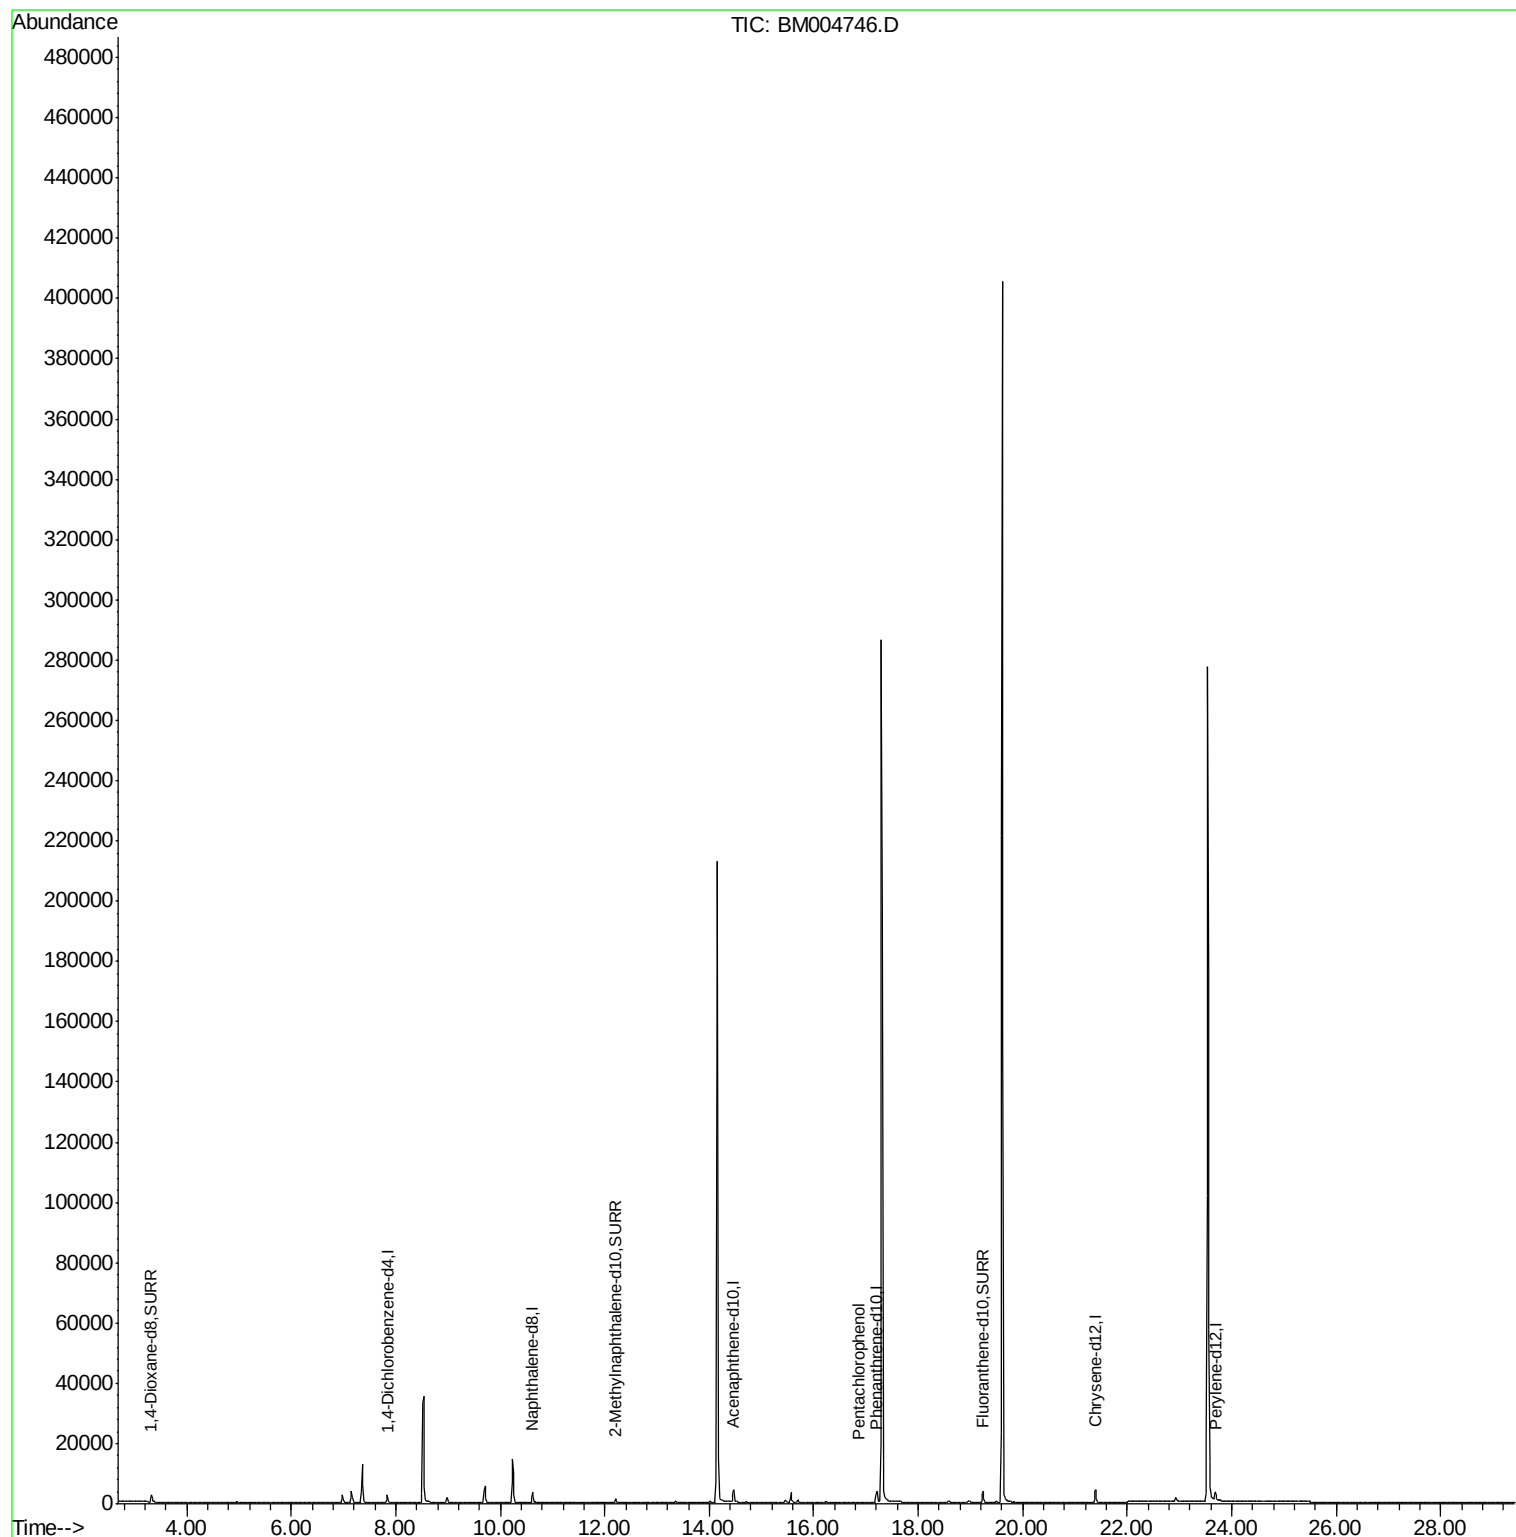

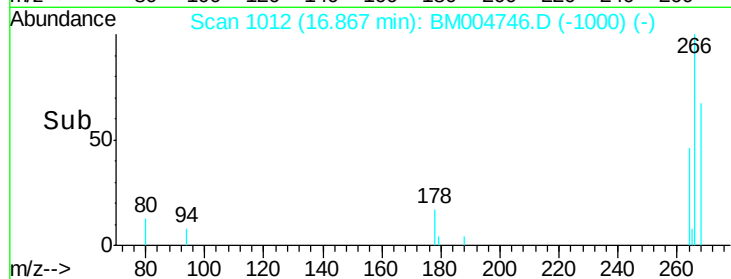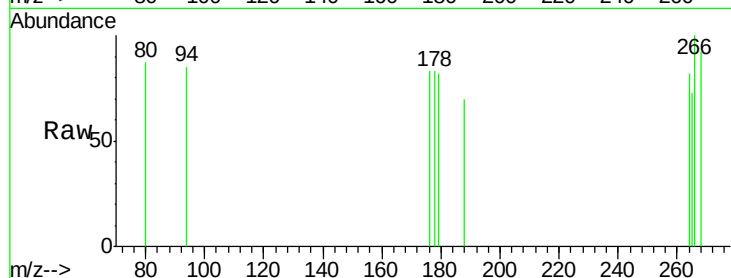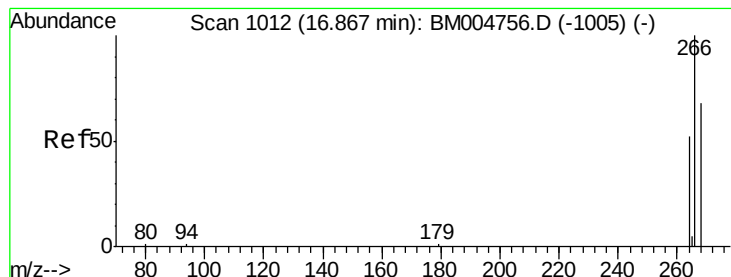

#13

Pentachlorophenol

Concen: 0.07 ng/ul

RT: 16.87 min Scan# 1012

Delta R.T. -0.00 min

Lab File: BM004746.D

Acq: 23 Mar 2016 03:08

Tot Ion:	266	Resp:	52
Ion Ratio	Lower	Upper	
266	100		
264	90.4	51.8	77.8#
268	61.5	46.8	70.2

Instrument :

BNA_M

ClientSampleId :

A4T34

Manual Integrations
APPROVED

Sohil
4/5/2016 5:21:17 PM

