
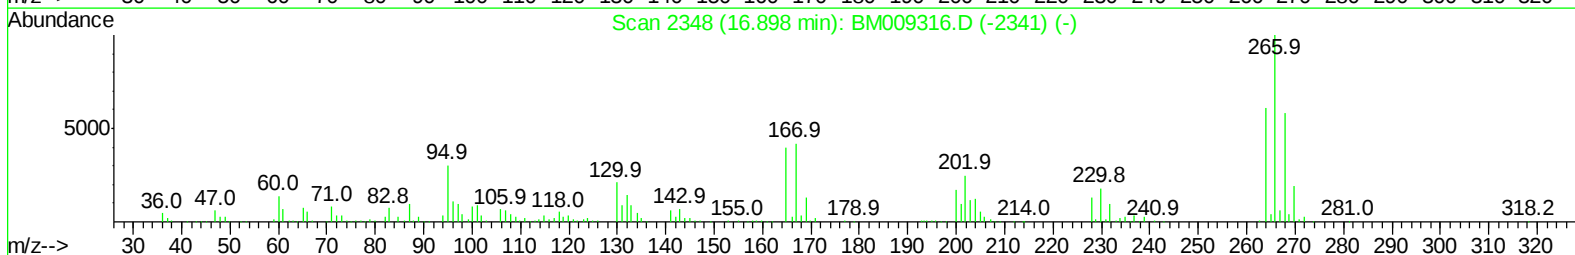
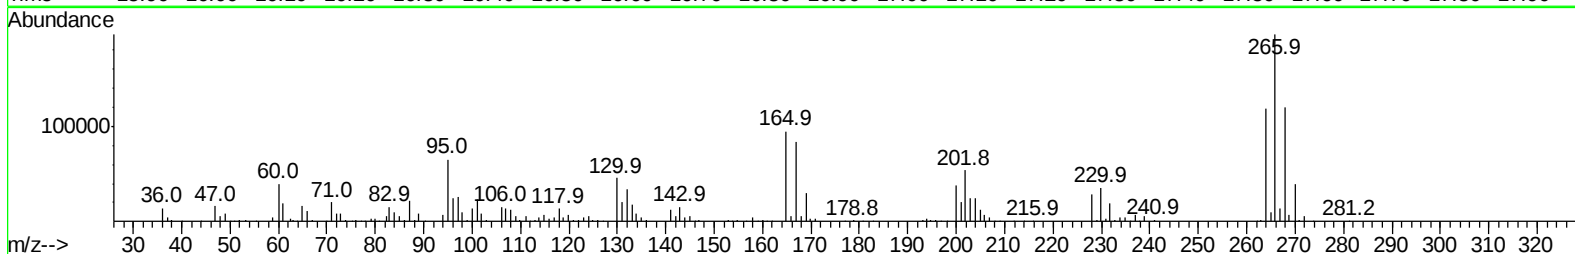


Data Path : Z:\HPCHEM1\BNA M\Data\BM032217\
Data File : BM009321.D
Acq On : 22 Mar 2017 17:00
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:40:48 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 16:43:02 2017
Response via : Initial Calibration

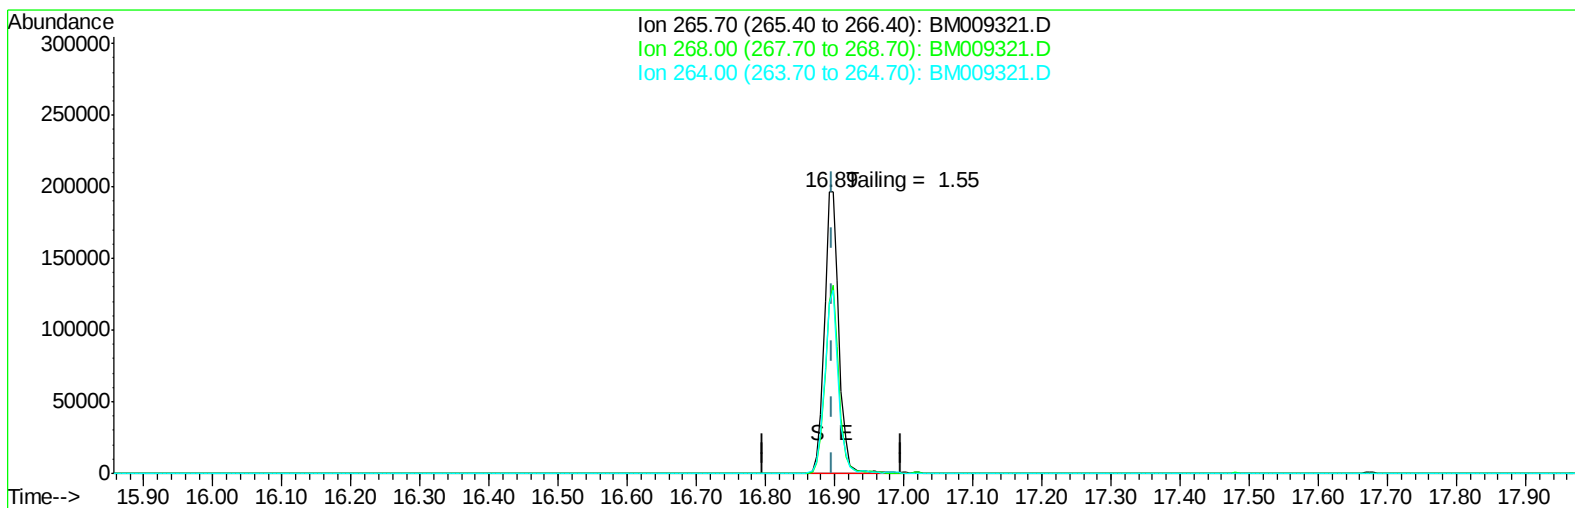

TIC: BM009321.D

(69) Pentachlorophenol (C)




16.892min (-0.006) 0.00ng

response 283128

Ion	Exp%	Act%
265.70	100	100
268.00	65.00	61.03
264.00	61.20	60.68
0.00	0.00	0.00

Data Path : Z:\HPCHEM1\BNA M\Data\BM032217\
Data File : BM009321.D
Acq On : 22 Mar 2017 17:00
Operator : SJ/MA
Sample : DFTPP
Misc :
ALS Vial : 1 Sample Multiplier: 1

Quant Time: Mar 23 07:40:48 2017
Quant Method : Z:\HPCHEM1\BNA M\METHODS\8270-BM032217.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 22 16:43:02 2017
Response via : Initial Calibration

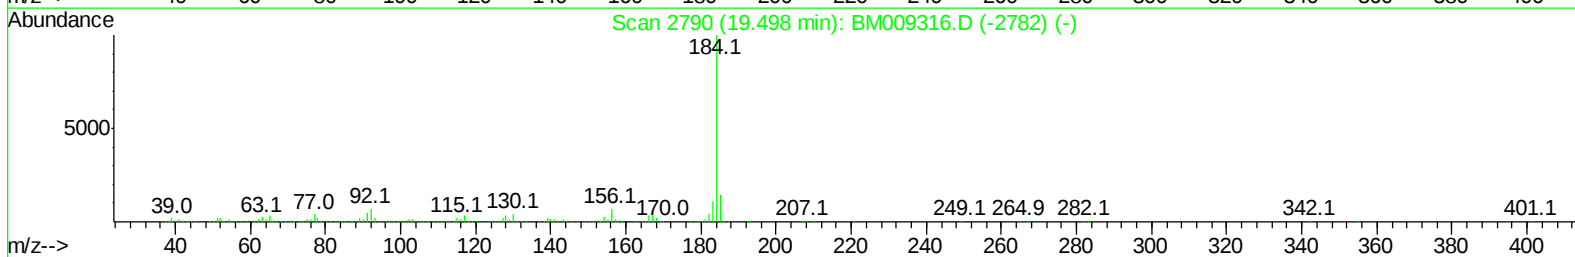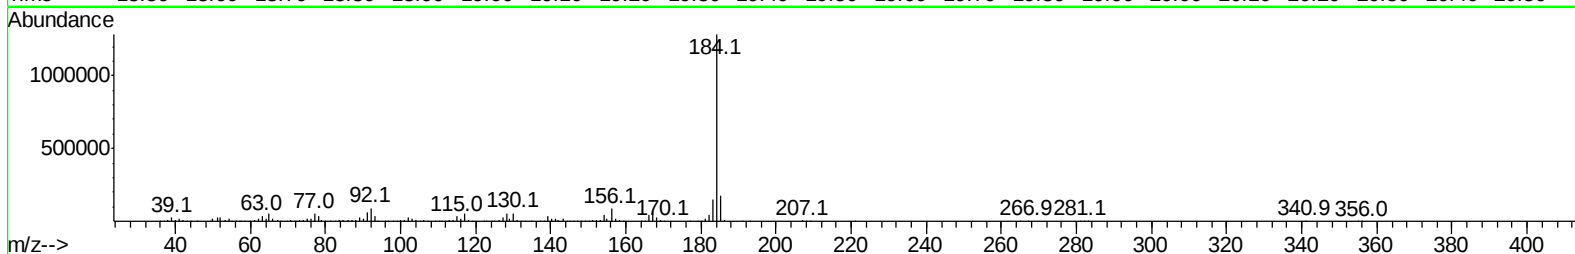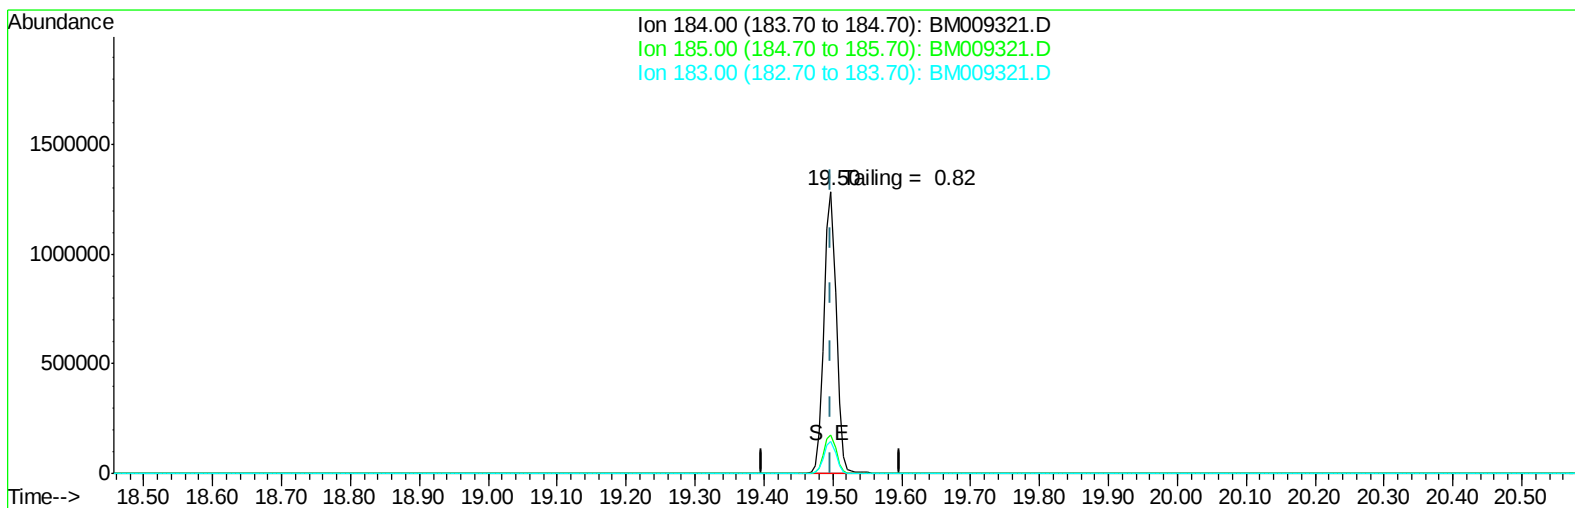

TIC: BM009321.D

(76) Benzidine

19.498min (+0.000) 174883.80ng

response 1574059

Ion	Exp%	Act%
184.00	100	100
185.00	14.10	13.88
183.00	11.10	11.59
0.00	0.00	0.00