


Data Path : Z:\HPCHEM1\BNA_M\Data\BM032217\
 Data File : BM009312.D
 Acq On : 22 Mar 2017 10:16
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 22 16:43:02 2017

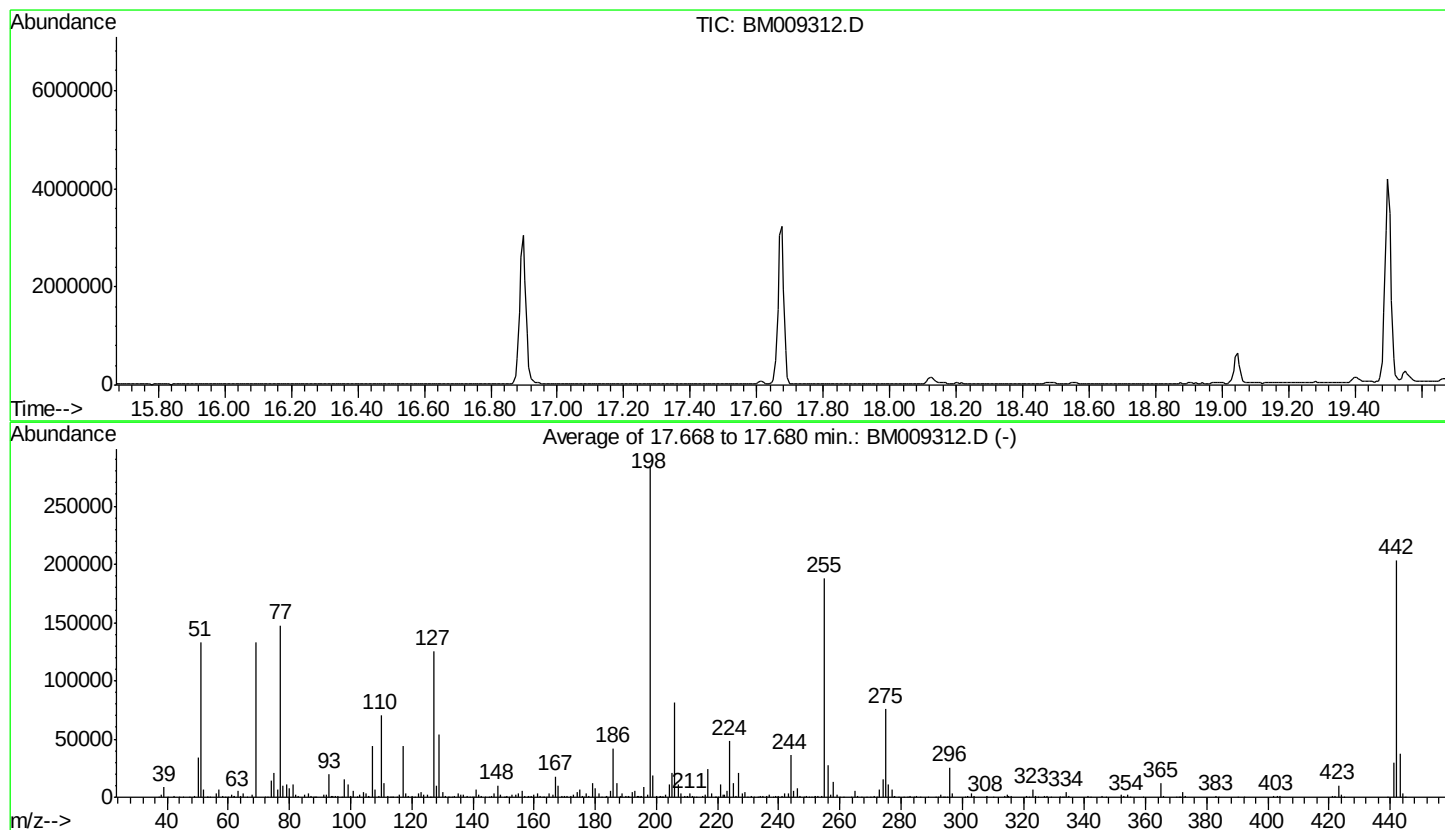

AutoFind: Scans 2479, 2480, 2481; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	46.8	133216	PASS
68	69	0.00	2	2.0	2597	PASS
69	198	0.00	100	46.7	132997	PASS
70	69	0.00	2	0.0	0	PASS
127	198	10	80	44.2	125874	PASS
197	198	0.00	2	0.7	1951	PASS
198	198	100	100	100.0	284714	PASS
199	198	5	9	6.7	19054	PASS
275	198	10	60	26.8	76336	PASS
365	198	1	100	4.4	12579	PASS
441	442	0.01	24	14.9	30224	PASS
442	198	50	100	71.5	203456	PASS
443	442	15	24	18.5	37640	PASS