


Data Path : Z:\HPCHEM1\BNA M\DATA\BM032217\
 Data File : BM009321.D
 Acq On : 22 Mar 2017 17:00
 Operator : SJ/MA
 Sample : DFTPP
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 DFTPP

Integration File: rteint.p

Method : Z:\HPCHEM1\BNA_M\METHODS\8270-BM032217.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 Last Update : Wed Mar 22 16:43:02 2017

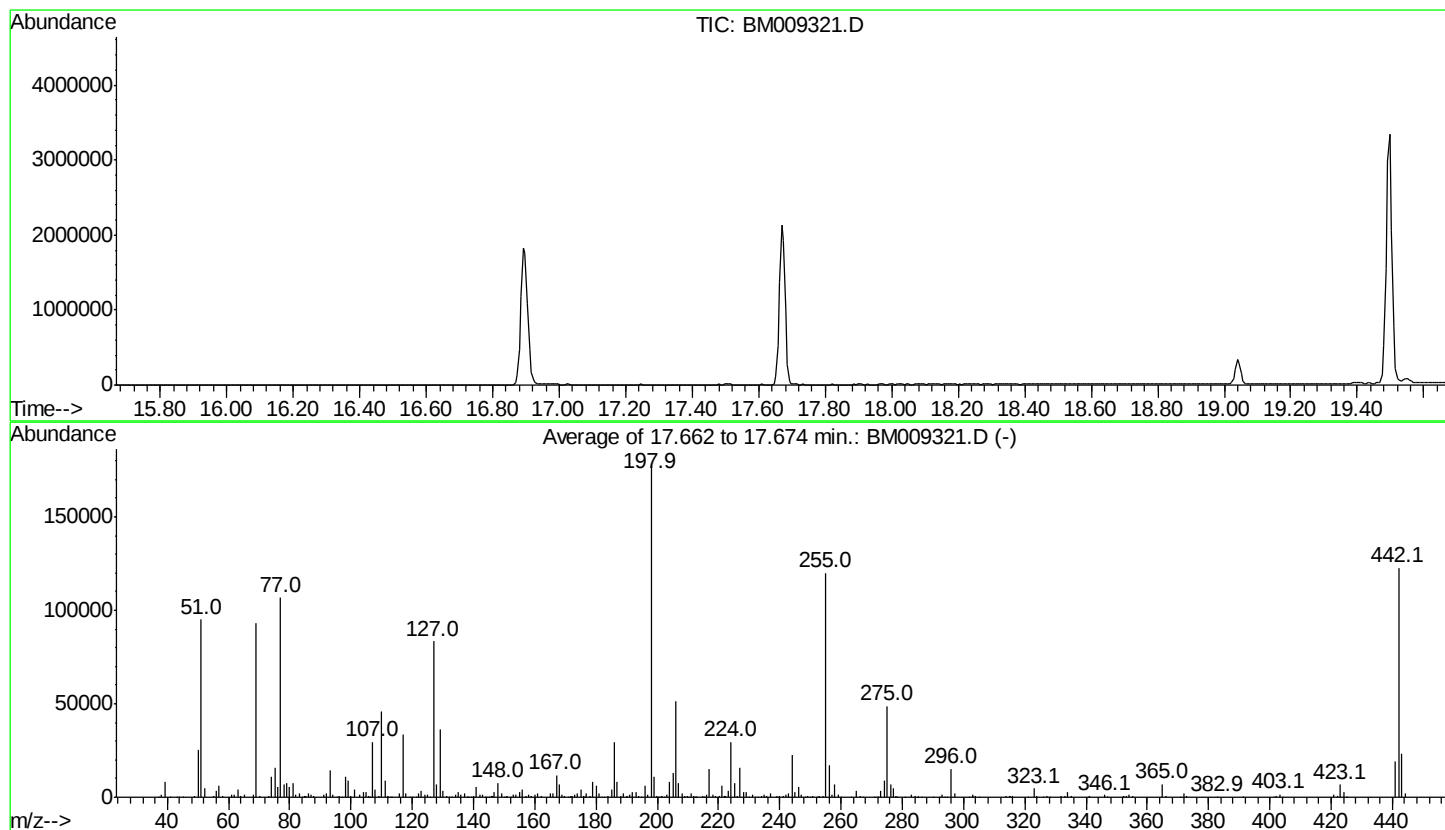

AutoFind: Scans 2478, 2479, 2480; Background Corrected with Scan 2472

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
51	198	10	80	53.5	94984	PASS
68	69	0.00	2	1.9	1734	PASS
69	198	0.00	100	52.5	93221	PASS
70	69	0.00	2	0.9	831	PASS
127	198	10	80	47.0	83434	PASS
197	198	0.00	2	0.9	1667	PASS
198	198	100	100	100.0	177450	PASS
199	198	5	9	6.3	11263	PASS
275	198	10	60	27.5	48816	PASS
365	198	1	100	4.0	7135	PASS
441	442	0.01	24	15.5	19080	PASS
442	198	50	100	69.2	122738	PASS
443	442	15	24	19.3	23649	PASS