

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034323.D
 Acq On : 22 Mar 2022 23:04
 Operator : CG/JU
 Sample : N1949-09
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CP-BH2-031422-0-2

Quant Time: Mar 23 05:08:06 2022
 Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
 QLast Update : Wed Mar 16 02:38:26 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) 1,4-Dichlorobenzene-d4	7.937	152	164989	20.000	ng	-0.01
21) Naphthalene-d8	10.748	136	659487	20.000	ng	-0.02
39) Acenaphthene-d10	14.577	164	389443	20.000	ng	-0.01
64) Phenanthrene-d10	17.318	188	748986	20.000	ng	-0.01
76) Chrysene-d12	21.489	240	717682	20.000	ng	-0.01
86) Perylene-d12	23.900	264	788368	20.000	ng	-0.01
System Monitoring Compounds						
5) 2-Fluorophenol	5.496	112	790850	85.991	ng	0.00
7) Phenol-d6	7.096	99	1094846	83.145	ng	-0.01
23) Nitrobenzene-d5	9.101	82	736465	54.370	ng	-0.01
42) 2,4,6-Tribromophenol	16.060	330	366902	69.897	ng	-0.01
45) 2-Fluorobiphenyl	13.207	172	1478955	51.894	ng	-0.01
79) Terphenyl-d14	19.936	244	2012497	48.725	ng	-0.01


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034323.D
Acq On : 22 Mar 2022 23:04
Operator : CG/JU
Sample : N1949-09
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CP-BH2-031422-0-2

Quant Time: Mar 23 05:08:06 2022
Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION
QLast Update : Wed Mar 16 02:38:26 2022
Response via : Initial Calibration




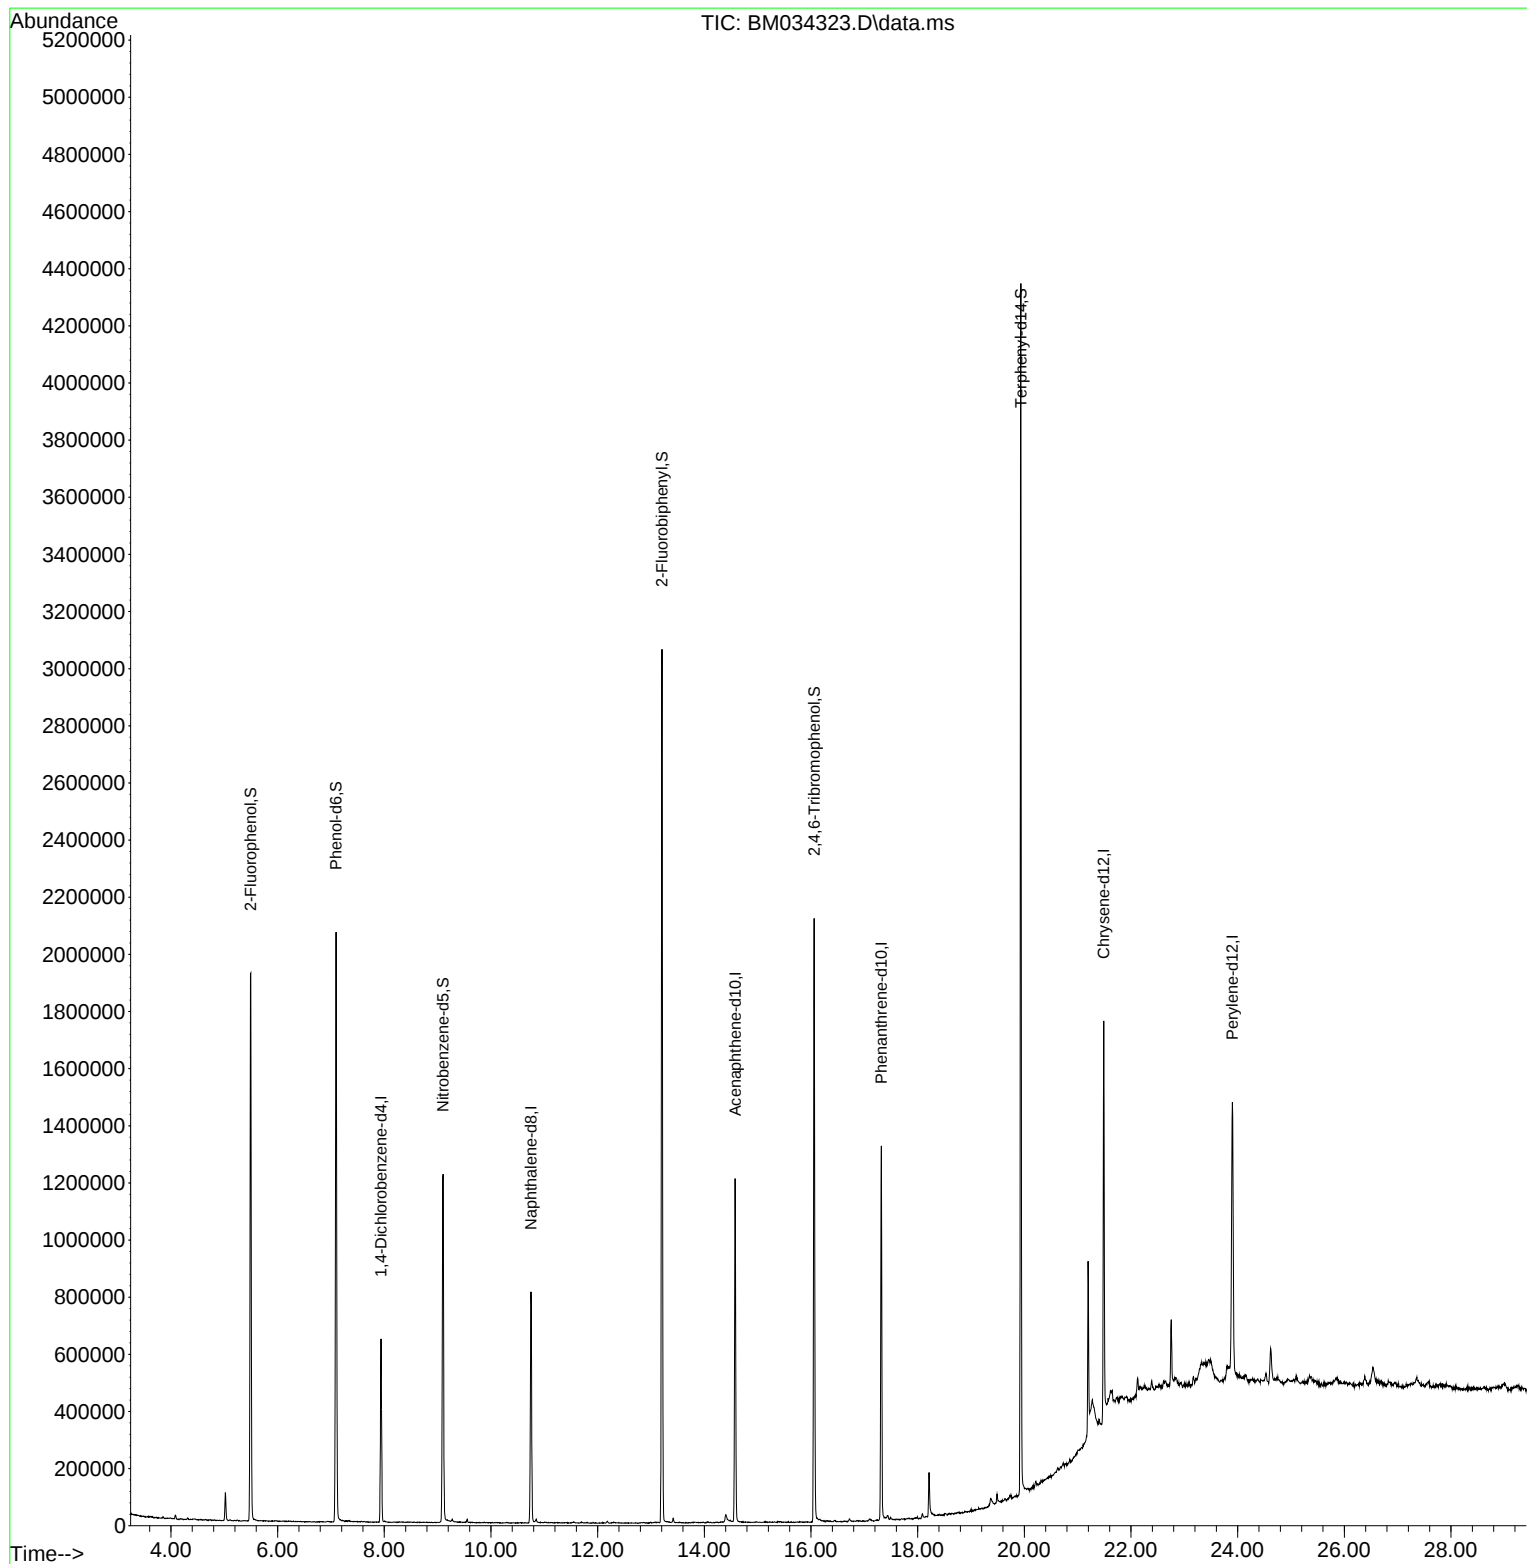


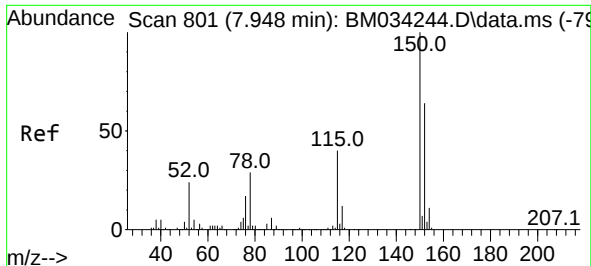

#1
1,4-Dichlorobenzene-d4
Concen: 20.000 ng
RT: 7.937 min Scan# 79
Delta R.T. -0.011 min
Lab File: BM034323.D
Acq: 22 Mar 2022 23:04




Instrument :
BNA_M
ClientSampleId :
CP-BH2-031422-0-2

Tgt Ion:152 Resp: 164989
Ion Ratio Lower Upper
152 100
150 155.3 125.4 188.2
115 59.5 50.1 75.1

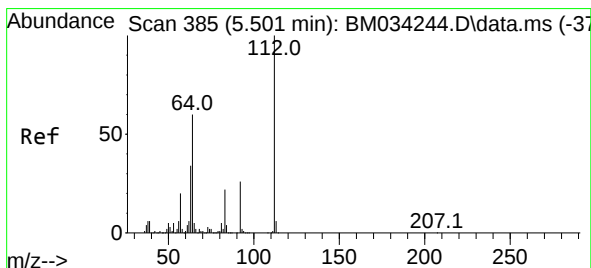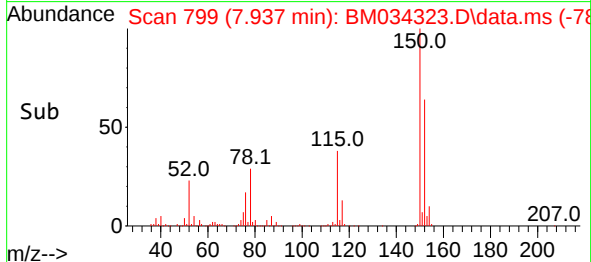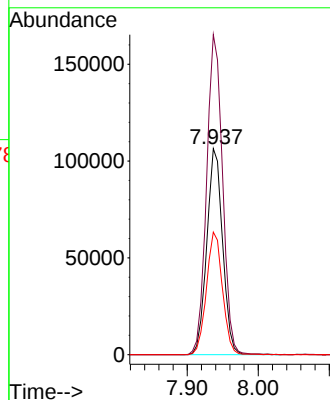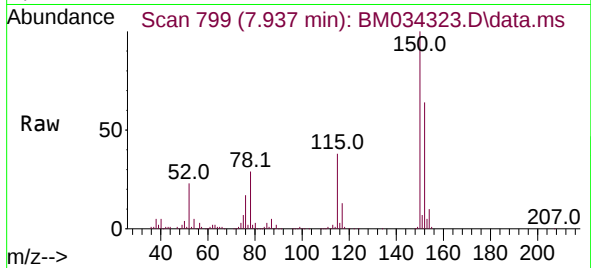

#5
2-Fluorophenol
Concen: 85.991 ng
RT: 5.496 min Scan# 384
Delta R.T. -0.006 min
Lab File: BM034323.D
Acq: 22 Mar 2022 23:04

Tgt Ion:112 Resp: 790850
Ion Ratio Lower Upper
112 100
64 62.2 47.9 71.9
63 33.0 27.1 40.7


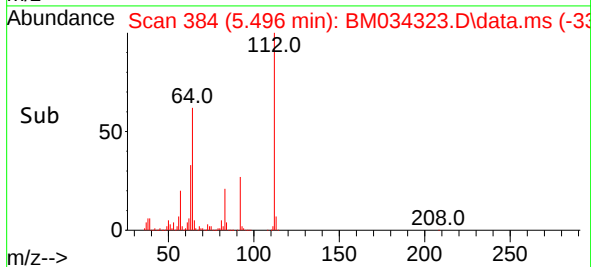
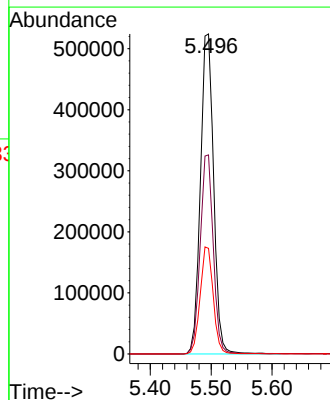
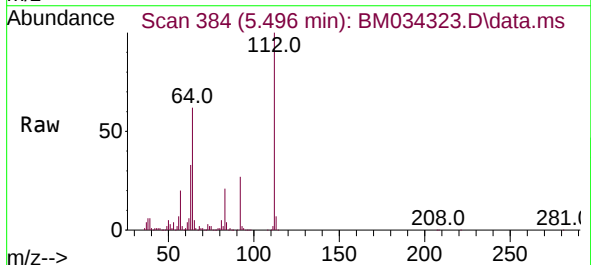




#7
Phenol-d6
Concen: 83.145 ng
RT: 7.096 min Scan# 61
Delta R.T. -0.012 min
Lab File: BM034323.D
Acq: 22 Mar 2022 23:04




Instrument :
BNA_M
ClientSampleId :
CP-BH2-031422-0-2


Tgt Ion: 99 Resp: 1094846
Ion Ratio Lower Upper
99 100
42 18.7 15.6 23.4
71 36.7 30.6 46.0

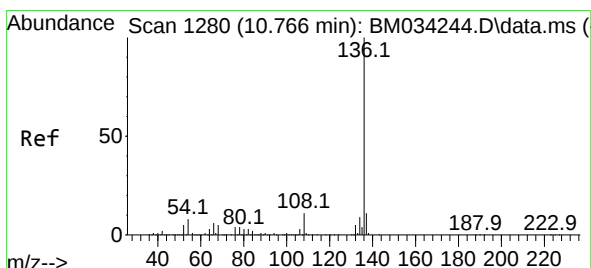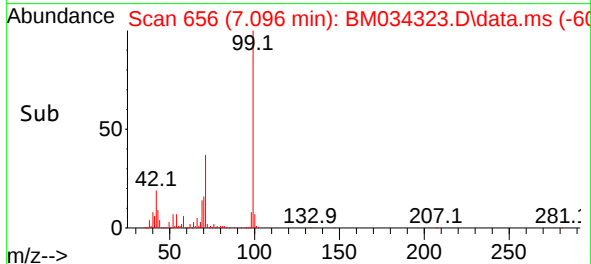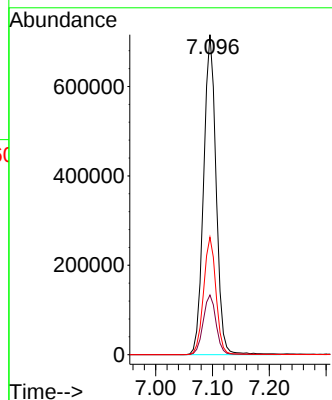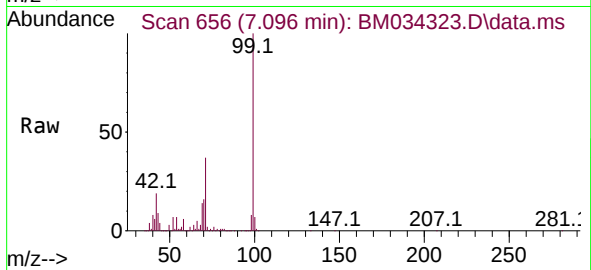

#21
Naphthalene-d8
Concen: 20.000 ng
RT: 10.748 min Scan# 1277
Delta R.T. -0.017 min
Lab File: BM034323.D
Acq: 22 Mar 2022 23:04

Tgt Ion: 136 Resp: 659487
Ion Ratio Lower Upper
136 100
137 11.0 8.6 13.0
54 8.4 6.2 9.4
68 6.1 4.3 6.5


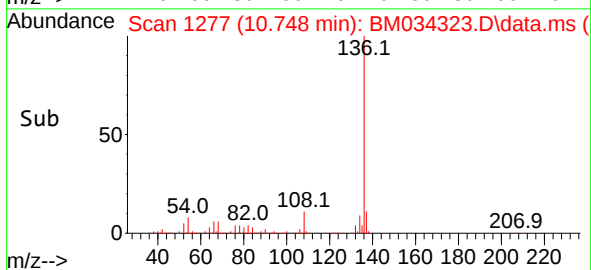
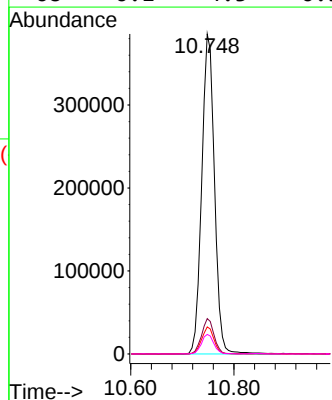
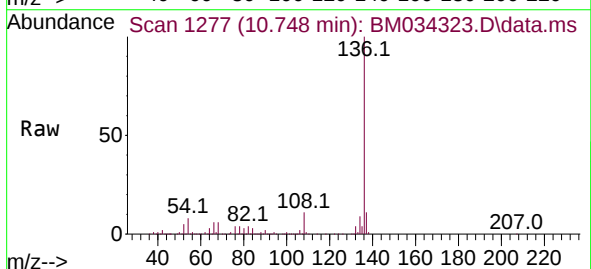


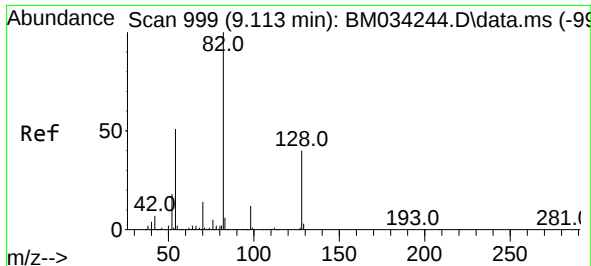

#23
Nitrobenzene-d5
Concen: 54.370 ng
RT: 9.101 min Scan# 91
Delta R.T. -0.012 min
Lab File: BM034323.D
Acq: 22 Mar 2022 23:04




Instrument :
BNA_M
ClientSampleId :
CP-BH2-031422-0-2


Tgt Ion: 82 Resp: 736465
Ion Ratio Lower Upper
82 100
128 40.7 31.9 47.9
54 50.1 40.6 61.0

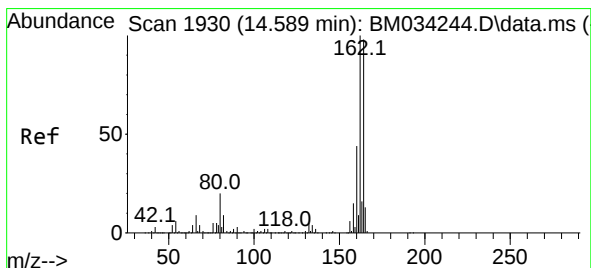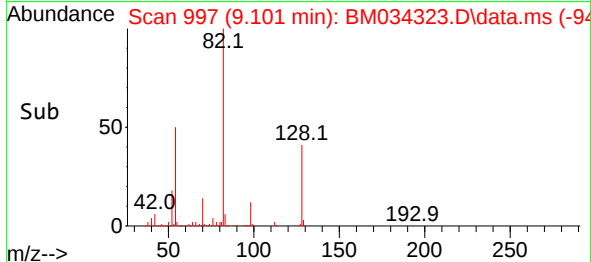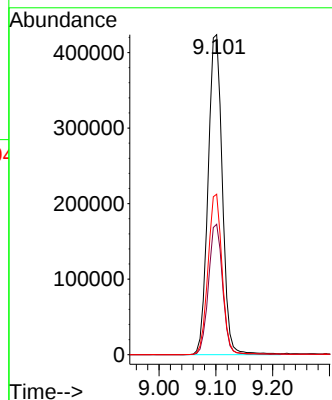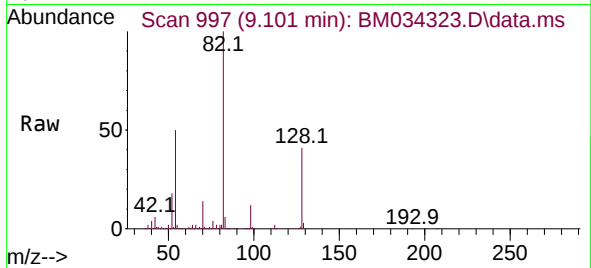

#39
Acenaphthene-d10
Concen: 20.000 ng
RT: 14.577 min Scan# 1928
Delta R.T. -0.012 min
Lab File: BM034323.D
Acq: 22 Mar 2022 23:04

Tgt Ion:164 Resp: 389443
Ion Ratio Lower Upper
164 100
162 101.3 81.6 122.4
160 44.4 35.6 53.4

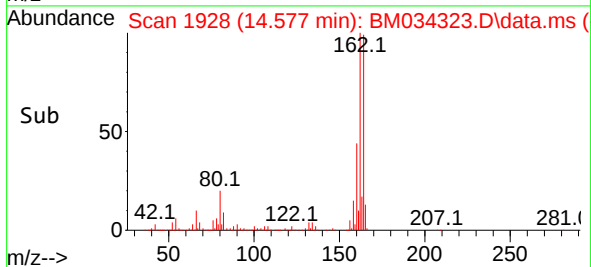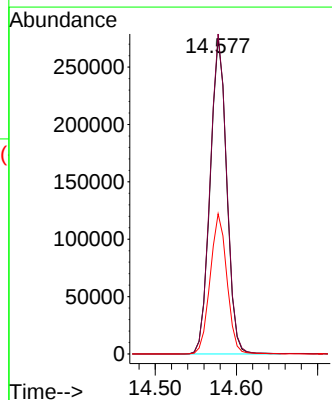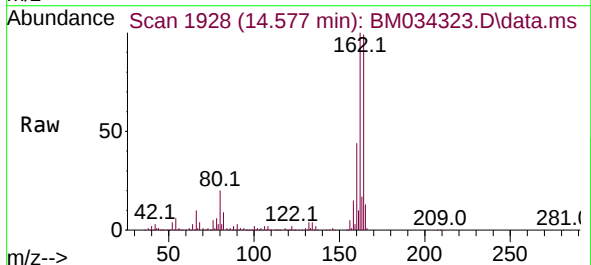

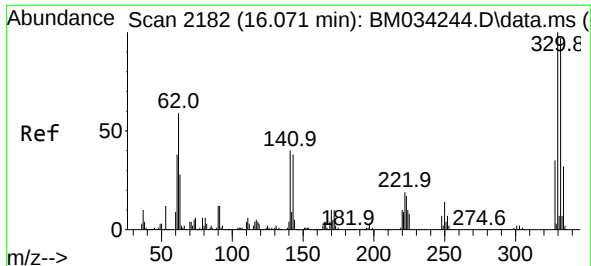

#42

2,4,6-Tribromophenol

Concen: 69.897 ng

RT: 16.060 min Scan# 21

Delta R.T. -0.012 min

Lab File: BM034323.D

Acq: 22 Mar 2022 23:04

Instrument :

BNA_M

ClientSampleId :

CP-BH2-031422-0-2





Tgt Ion:330 Resp: 366902

Ion Ratio Lower Upper

330 100

332 95.9 78.2 117.4

141 36.7 30.6 45.8

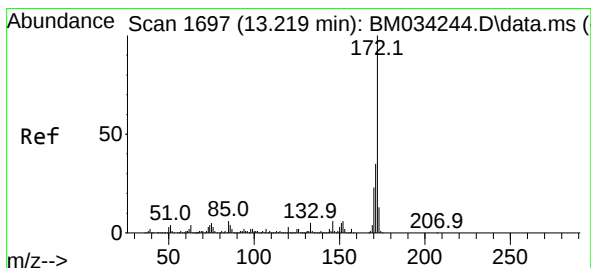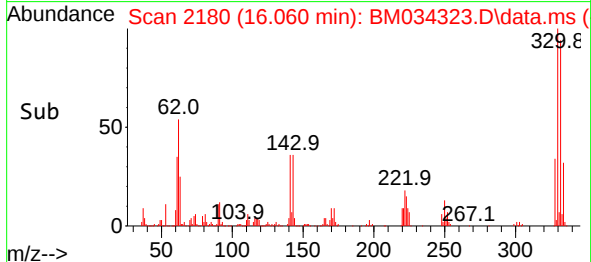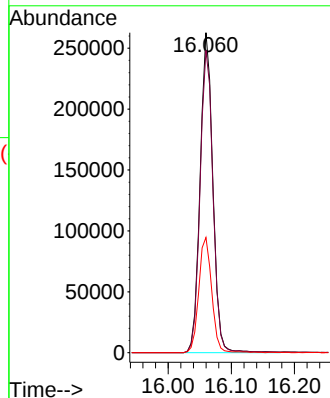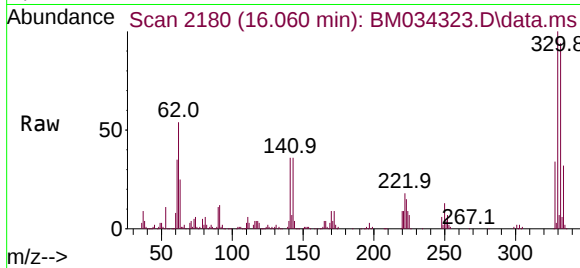

#45

2-Fluorobiphenyl

Concen: 51.894 ng

RT: 13.207 min Scan# 1695

Delta R.T. -0.012 min

Lab File: BM034323.D

Acq: 22 Mar 2022 23:04




Tgt Ion:172 Resp: 1478955


Ion Ratio Lower Upper

172 100

171 35.5 28.0 42.0

170 22.9 18.6 28.0


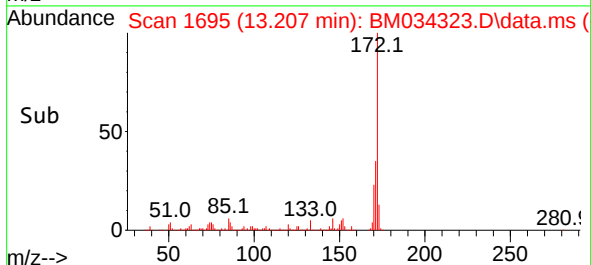
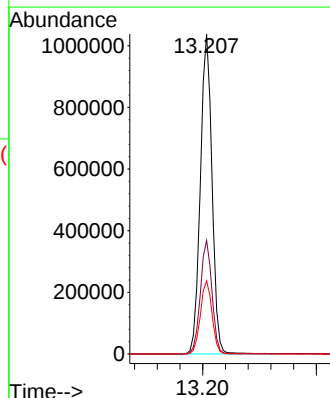
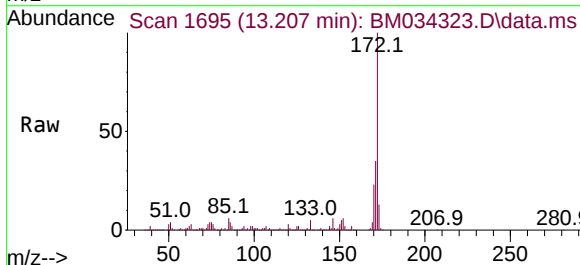


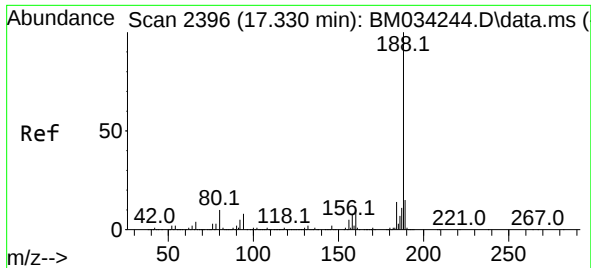

#64
Phenanthrene-d10
Concen: 20.000 ng
RT: 17.318 min Scan# 21
Delta R.T. -0.012 min
Lab File: BM034323.D
Acq: 22 Mar 2022 23:04




Instrument :
BNA_M
ClientSampleId :
CP-BH2-031422-0-2


Tgt Ion:188 Resp: 748986
Ion Ratio Lower Upper
188 100
94 8.9 6.6 9.8
80 9.7 7.8 11.8

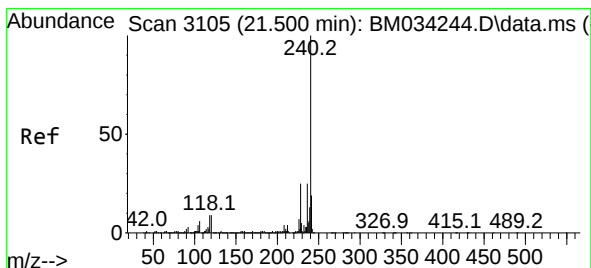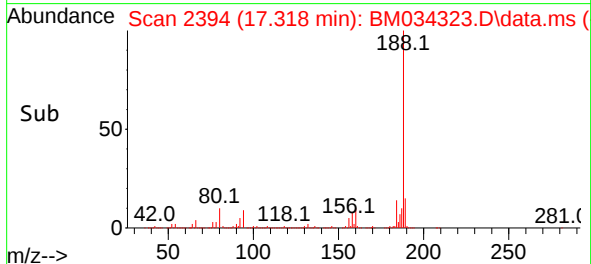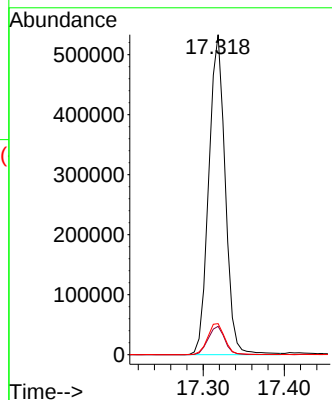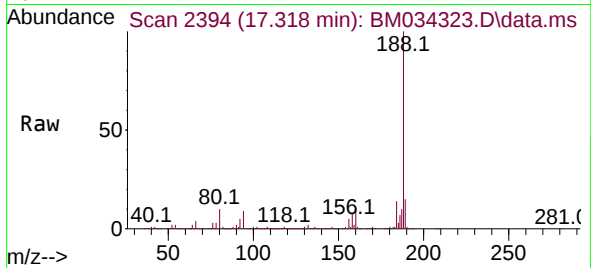

#76
Chrysene-d12
Concen: 20.000 ng
RT: 21.489 min Scan# 3103
Delta R.T. -0.012 min
Lab File: BM034323.D
Acq: 22 Mar 2022 23:04

Tgt Ion:240 Resp: 717682
Ion Ratio Lower Upper
240 100
120 9.7 7.3 10.9
236 24.4 20.2 30.2


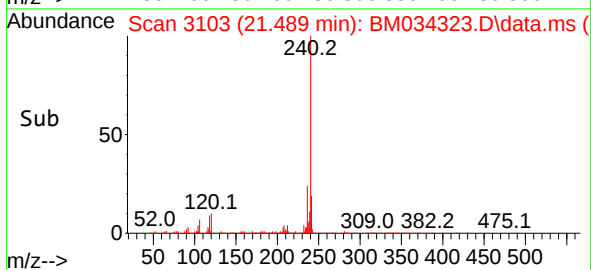
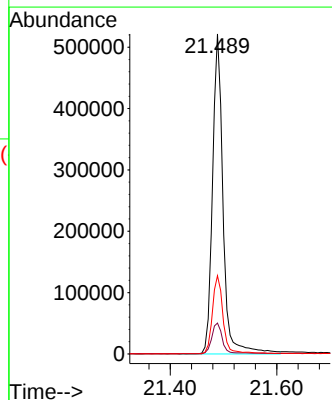
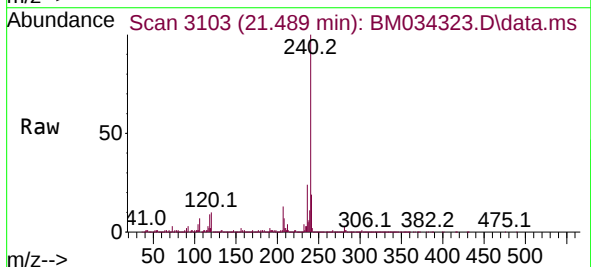


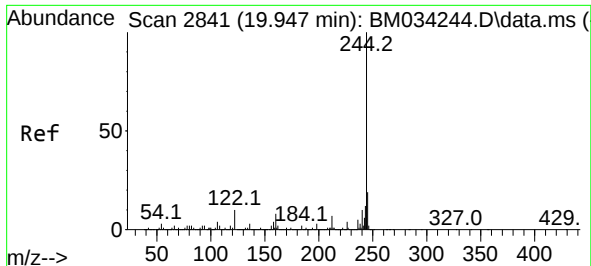

#79
 Terphenyl-d14
 Concen: 48.725 ng
 RT: 19.936 min Scan# 21
 Delta R.T. -0.012 min
 Lab File: BM034323.D
 Acq: 22 Mar 2022 23:04

Instrument :
 BNA_M
 ClientSampleId :
 CP-BH2-031422-0-2

Tgt Ion:244 Resp: 2012497
 Ion Ratio Lower Upper
 244 100
 212 7.2 5.9 8.9
 122 9.9 7.8 11.8

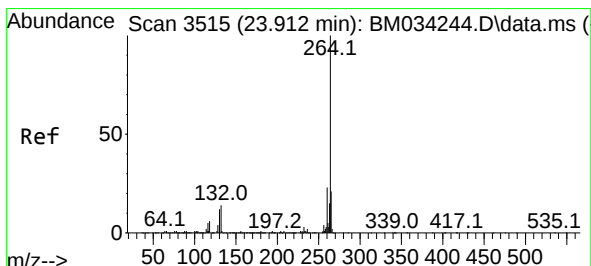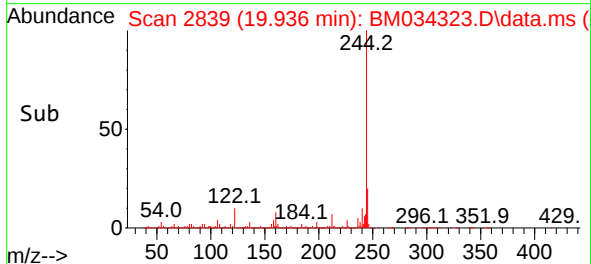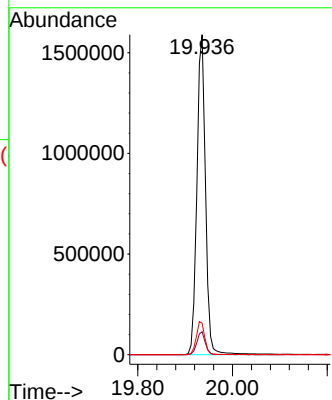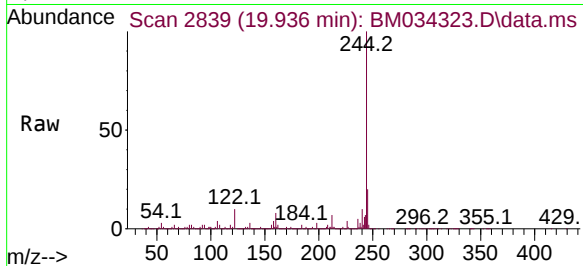

#86
 Perylene-d12
 Concen: 20.000 ng
 RT: 23.900 min Scan# 3513
 Delta R.T. -0.012 min
 Lab File: BM034323.D
 Acq: 22 Mar 2022 23:04

Tgt Ion:264 Resp: 788368
 Ion Ratio Lower Upper
 264 100
 260 23.6 18.6 28.0
 265 22.5 17.6 26.4

