

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM032222\  
 Data File : BM034304.D  
 Acq On : 22 Mar 2022 10:07  
 Operator : CG/JU  
 Sample : PB143451BL  
 Misc :  
 ALS Vial : 3 Sample Multiplier: 1

Instrument :  
 BNA\_M  
 ClientSampleId :  
 PB143451BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034304.D\data.ms

| peak<br># | R.T.<br>min | first<br>scan | max<br>scan | last<br>scan | PK<br>TY | peak<br>height | corr.<br>area | corr.<br>% max. | % of<br>total |
|-----------|-------------|---------------|-------------|--------------|----------|----------------|---------------|-----------------|---------------|
| 1         | 5.496       | 377           | 384         | 395          | rBV      | 3951806        | 5664505       | 43.42%          | 10.179%       |
| 2         | 7.101       | 649           | 657         | 676          | rBV      | 3815016        | 6042287       | 46.32%          | 10.857%       |
| 3         | 7.943       | 792           | 800         | 809          | rBV      | 668194         | 1051652       | 8.06%           | 1.890%        |
| 4         | 9.101       | 986           | 997         | 1019         | rBV      | 2239764        | 3804284       | 29.16%          | 6.836%        |
| 5         | 10.754      | 1270          | 1278        | 1288         | rBV      | 861001         | 1452390       | 11.13%          | 2.610%        |
| 6         | 13.213      | 1688          | 1696        | 1707         | rBV      | 6003284        | 8805786       | 67.50%          | 15.823%       |
| 7         | 14.583      | 1922          | 1929        | 1940         | rBV      | 1321467        | 2008356       | 15.40%          | 3.609%        |
| 8         | 16.066      | 2174          | 2181        | 2211         | rBV      | 4717166        | 6838932       | 52.43%          | 12.289%       |
| 9         | 17.318      | 2387          | 2394        | 2409         | rBV      | 1567427        | 2339709       | 17.94%          | 4.204%        |
| 10        | 19.936      | 2833          | 2839        | 2851         | rBV      | 9927912        | 13044767      | 100.00%         | 23.440%       |
| 11        | 21.489      | 3098          | 3103        | 3118         | rBV      | 1617782        | 2378884       | 18.24%          | 4.275%        |
| 12        | 23.900      | 3506          | 3513        | 3531         | rBV2     | 994905         | 2219637       | 17.02%          | 3.988%        |




Sum of corrected areas: 55651189

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM032222\  
Data File : BM034304.D  
Acq On : 22 Mar 2022 10:07  
Operator : CG/JU  
Sample : PB143451BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB143451BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

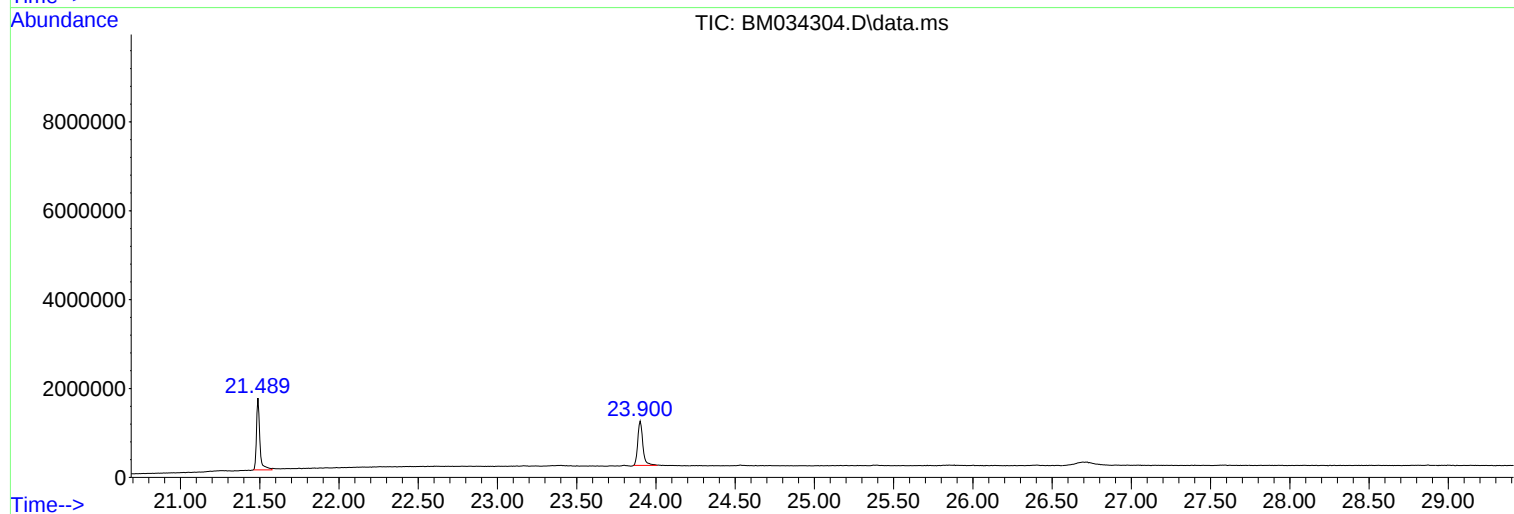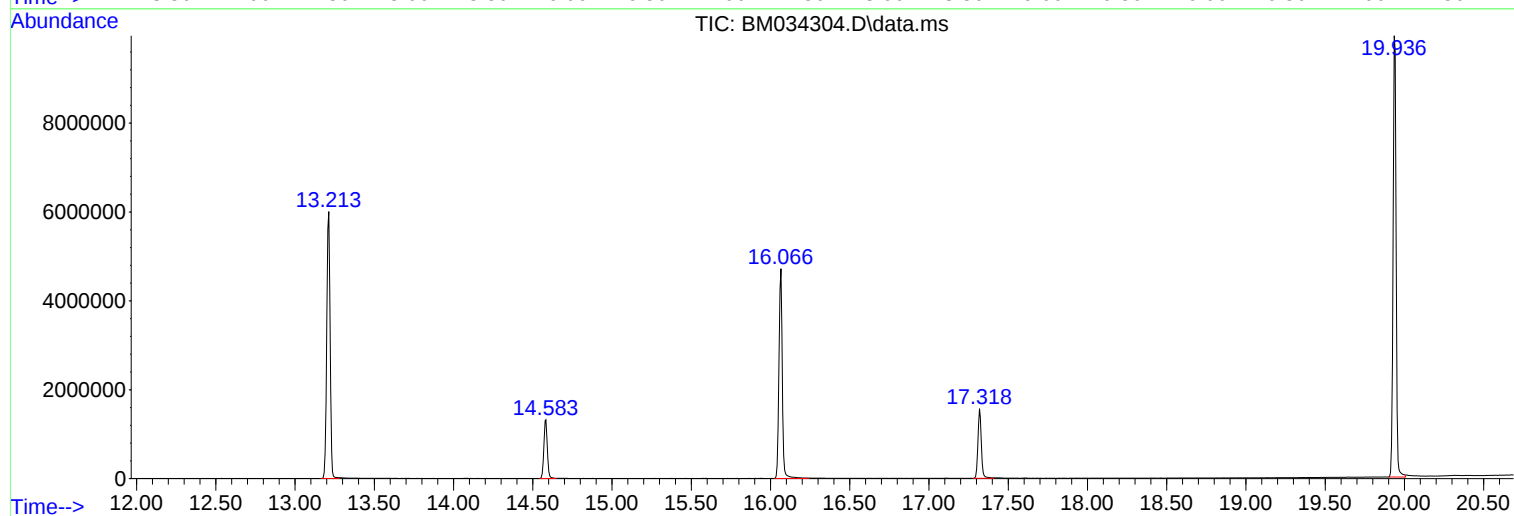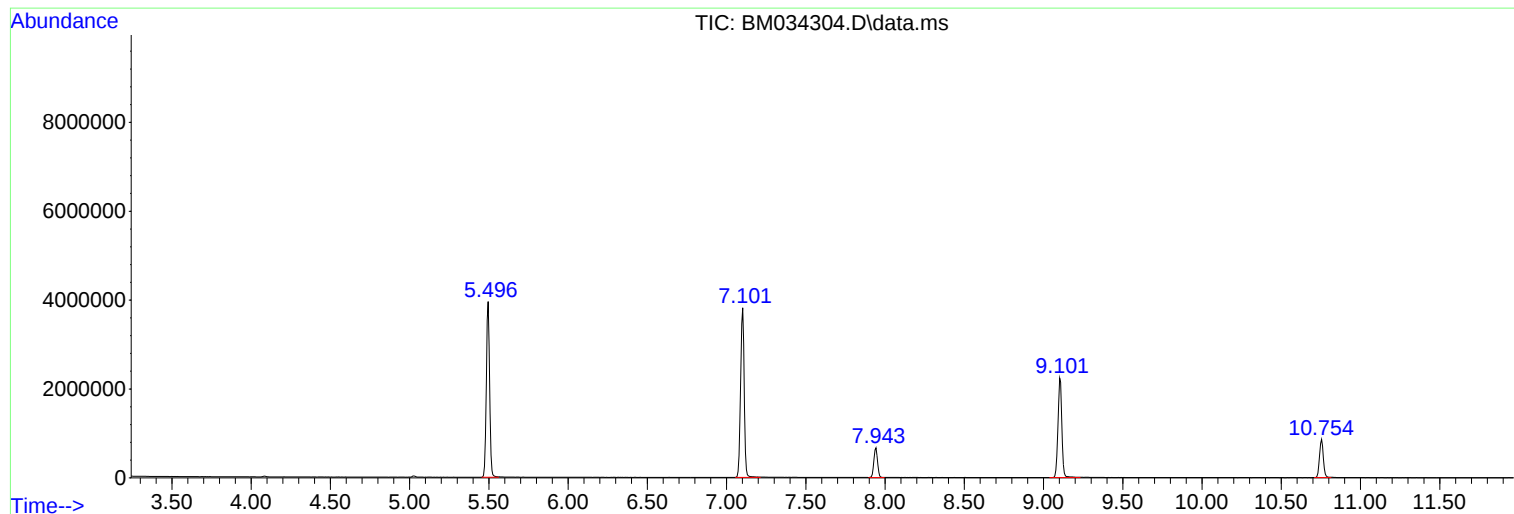

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM032222\  
Data File : BM034304.D  
Acq On : 22 Mar 2022 10:07  
Operator : CG/JU  
Sample : PB143451BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB143451BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

\*\*\*\*\*

Data Path : Z:\svoasrv\HPCHEM1\BNA\_M\Data\BM032222\  
Data File : BM034304.D  
Acq On : 22 Mar 2022 10:07  
Operator : CG/JU  
Sample : PB143451BL  
Misc :  
ALS Vial : 3 Sample Multiplier: 1

Instrument :  
BNA\_M  
ClientSampleId :  
PB143451BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA\_M\Methods\8270-BM031522.M  
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L  
TIC Integration Parameters: LSCINT.P

| TIC Top Hit name | RT | EstConc | Units | Response | # | RT | Resp | Conc |
|------------------|----|---------|-------|----------|---|----|------|------|
|------------------|----|---------|-------|----------|---|----|------|------|