

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034306.D
 Acq On : 22 Mar 2022 12:10
 Operator : CG/JU
 Sample : PB143452BL
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143452BL

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.2 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034306.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.496	377	384	395	rBV	3567941	5129072	41.20%	10.002%
2	7.101	649	657	674	rBV	3452030	5463041	43.88%	10.654%
3	7.943	792	800	813	rBV	586843	947239	7.61%	1.847%
4	9.101	989	997	1008	rBV	2025118	3381899	27.17%	6.595%
5	10.754	1270	1278	1289	rBV	757096	1307836	10.51%	2.550%
6	13.213	1688	1696	1707	rBV	5294039	7928340	63.69%	15.461%
7	14.583	1922	1929	1941	rBV	1184938	1790535	14.38%	3.492%
8	16.066	2174	2181	2205	rBV	4198901	6245120	50.17%	12.179%
9	17.318	2388	2394	2409	rBV	1419085	2121090	17.04%	4.136%
10	19.936	2833	2839	2867	rBV	9433227	12448755	100.00%	24.277%
11	21.489	3098	3103	3119	rBV	1532804	2299265	18.47%	4.484%
12	23.900	3506	3513	3526	rBV2	969193	2216339	17.80%	4.322%




Sum of corrected areas: 51278531

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034306.D
Acq On : 22 Mar 2022 12:10
Operator : CG/JU
Sample : PB143452BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143452BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

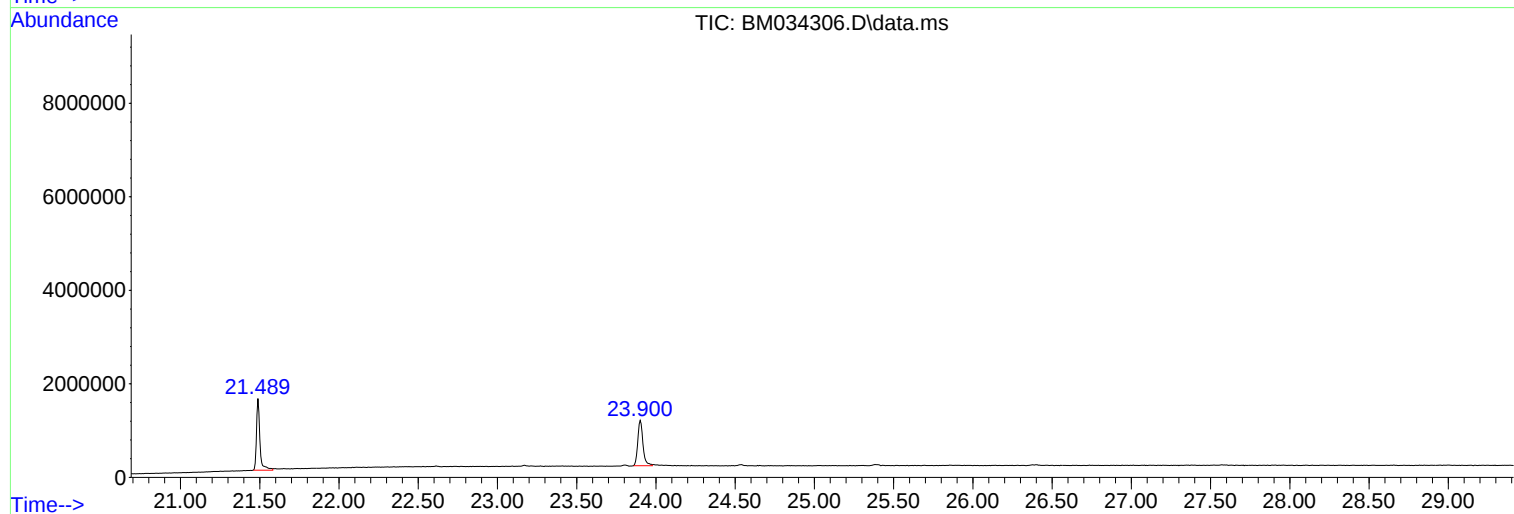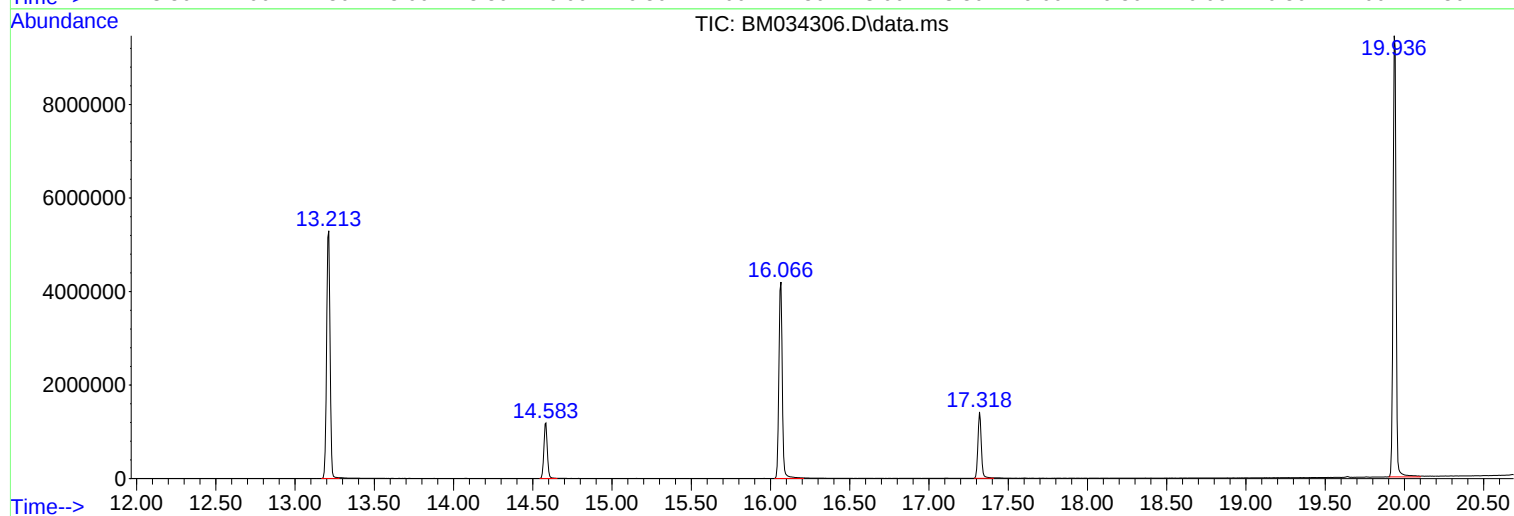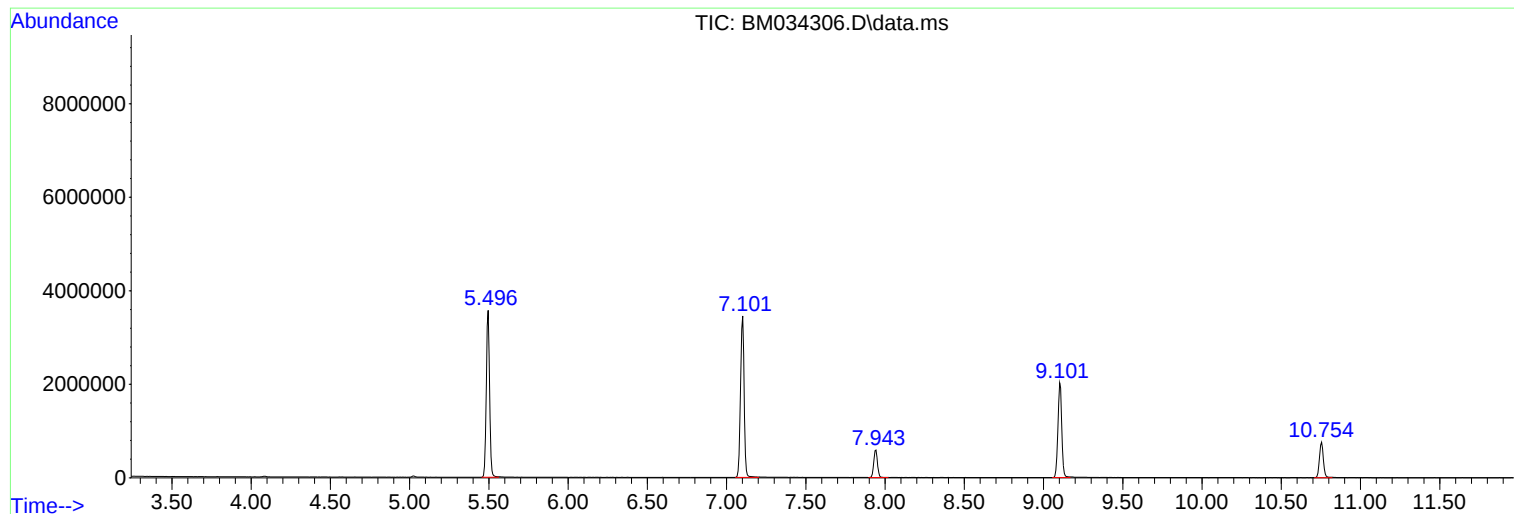

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034306.D
Acq On : 22 Mar 2022 12:10
Operator : CG/JU
Sample : PB143452BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143452BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034306.D
Acq On : 22 Mar 2022 12:10
Operator : CG/JU
Sample : PB143452BL
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143452BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------