

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034313.D
 Acq On : 22 Mar 2022 16:56
 Operator : CG/JU
 Sample : PB143457BL
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 PB143457BL

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034313.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.496	377	384	394	rBV	4000554	5709988	43.33%	10.267%
2	7.101	649	657	669	rBV	3742154	5905128	44.81%	10.617%
3	7.942	793	800	808	rBV	691403	1080131	8.20%	1.942%
4	9.107	989	998	1009	rBV	2183493	3758329	28.52%	6.758%
5	10.754	1271	1278	1288	rBV	856063	1457466	11.06%	2.621%
6	13.213	1688	1696	1706	rBV	6064065	8724660	66.20%	15.687%
7	14.583	1921	1929	1945	rBV	1324995	2003776	15.20%	3.603%
8	16.065	2174	2181	2205	rBV	4788097	6899485	52.35%	12.405%
9	17.318	2388	2394	2408	rBV	1616467	2357299	17.89%	4.238%
10	19.942	2833	2840	2860	rBV	10249041	13178517	100.00%	23.695%
11	21.489	3098	3103	3118	rBV	1573161	2400361	18.21%	4.316%
12	23.906	3507	3514	3535	rVB	945905	2141847	16.25%	3.851%




Sum of corrected areas: 55616987

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034313.D
Acq On : 22 Mar 2022 16:56
Operator : CG/JU
Sample : PB143457BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143457BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

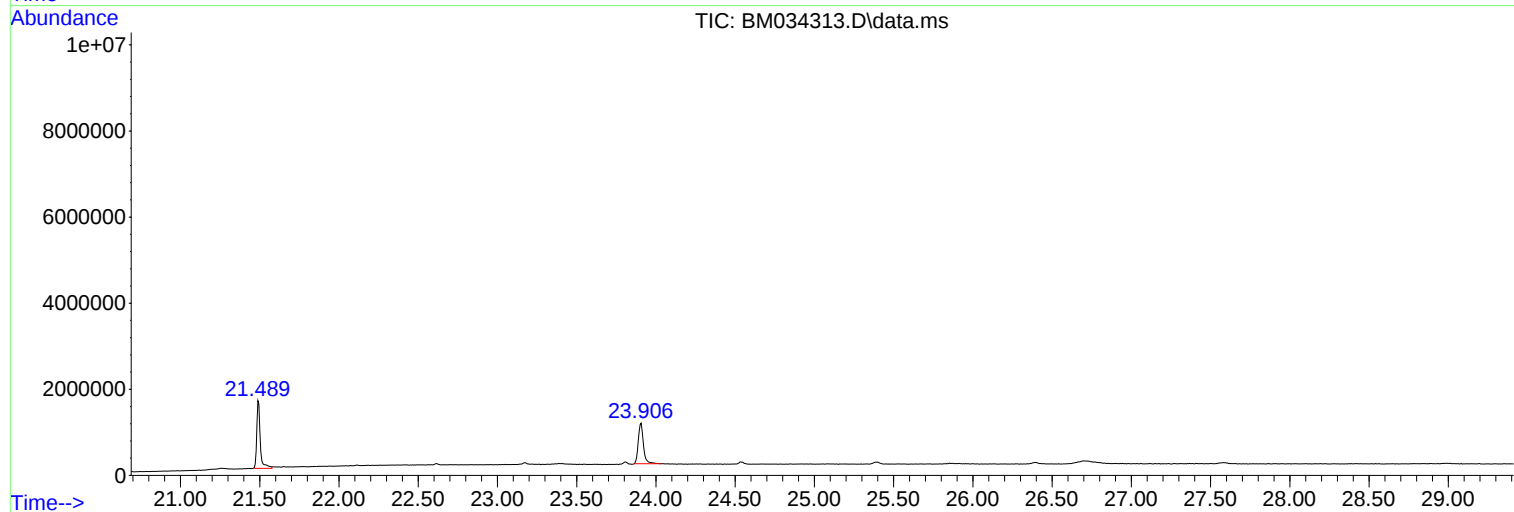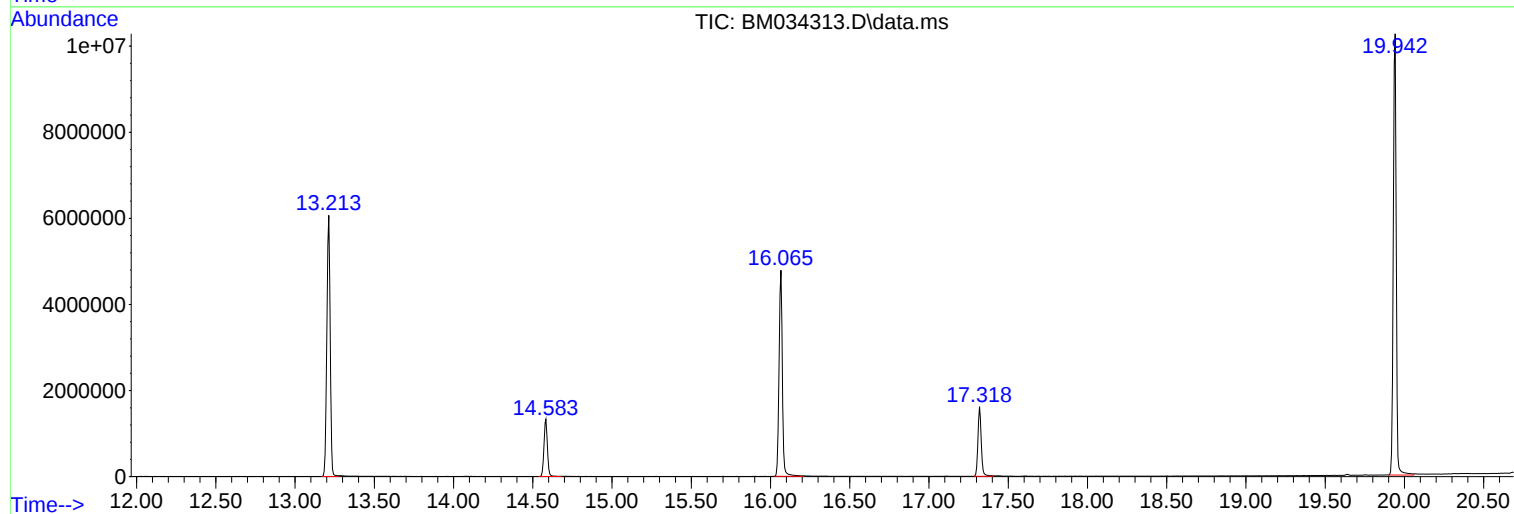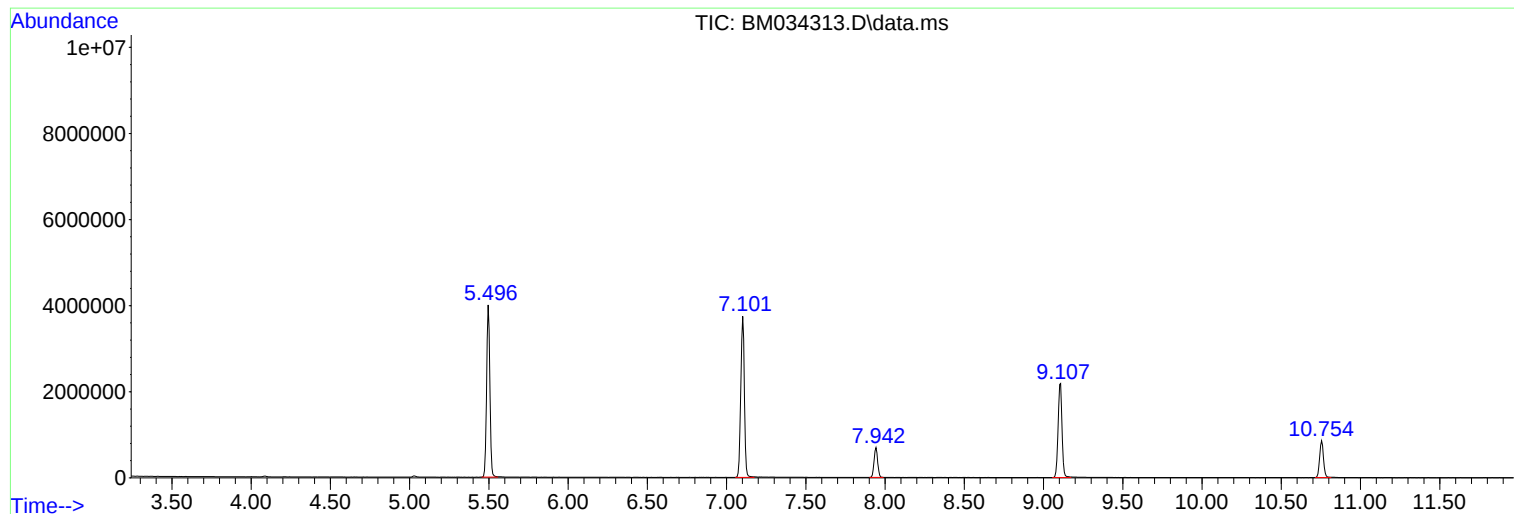

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034313.D
Acq On : 22 Mar 2022 16:56
Operator : CG/JU
Sample : PB143457BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143457BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034313.D
Acq On : 22 Mar 2022 16:56
Operator : CG/JU
Sample : PB143457BL
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
PB143457BL

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------