

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034315.D
 Acq On : 22 Mar 2022 18:13
 Operator : CG/JU
 Sample : N1977-08
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 EB-20220315

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034315.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.019	297	303	309	rBV	330428	438596	4.67%	1.195%
2	5.490	376	383	395	rBV	1248263	1844662	19.63%	5.024%
3	7.095	648	656	673	rBV	697685	1117661	11.89%	3.044%
4	7.937	792	799	807	rBV	588952	931962	9.92%	2.538%
5	9.101	989	997	1008	rBV	1891986	3099881	32.98%	8.443%
6	10.748	1269	1277	1288	rBV	717871	1239839	13.19%	3.377%
7	13.207	1688	1695	1705	rBV	4672090	6655715	70.81%	18.127%
8	14.577	1922	1928	1939	rVB	1058884	1571382	16.72%	4.280%
9	16.060	2173	2180	2190	rBV	3384400	4746170	50.50%	12.926%
10	17.318	2388	2394	2405	rBV	1267086	1789405	19.04%	4.874%
11	19.936	2833	2839	2853	rBV	7844717	9398995	100.00%	25.598%
12	21.489	3098	3103	3117	rBV	1401781	1994218	21.22%	5.431%
13	23.900	3507	3513	3524	rVB2	910763	1888499	20.09%	5.143%




Sum of corrected areas: 36716985

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034315.D
Acq On : 22 Mar 2022 18:13
Operator : CG/JU
Sample : N1977-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EB-20220315

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

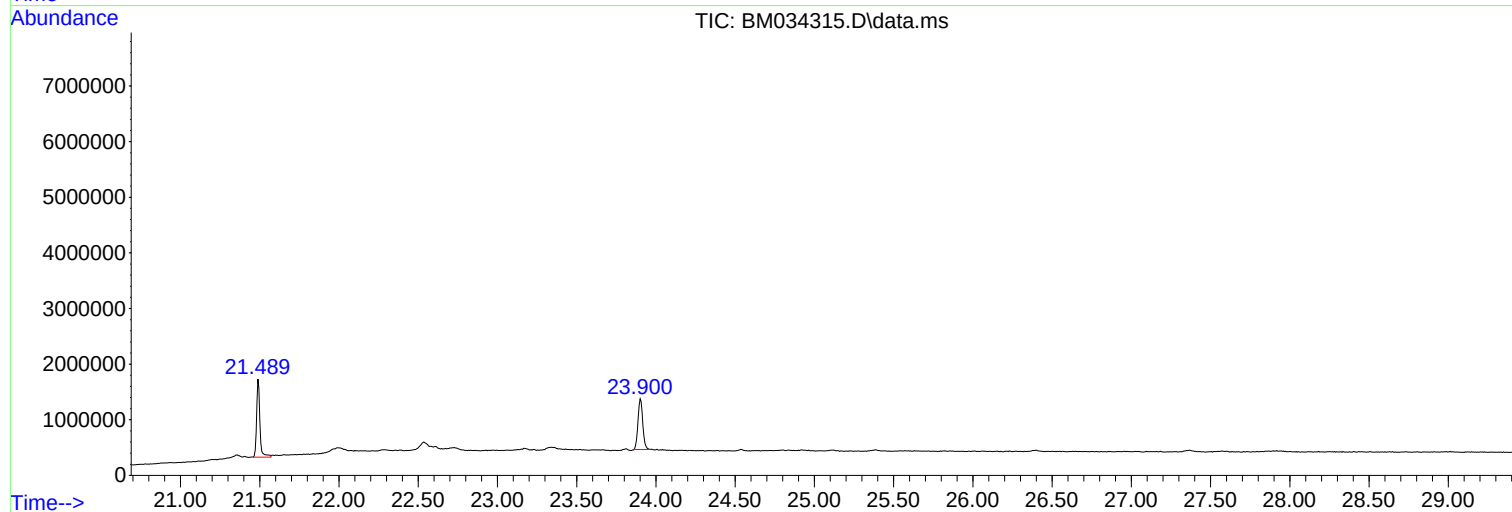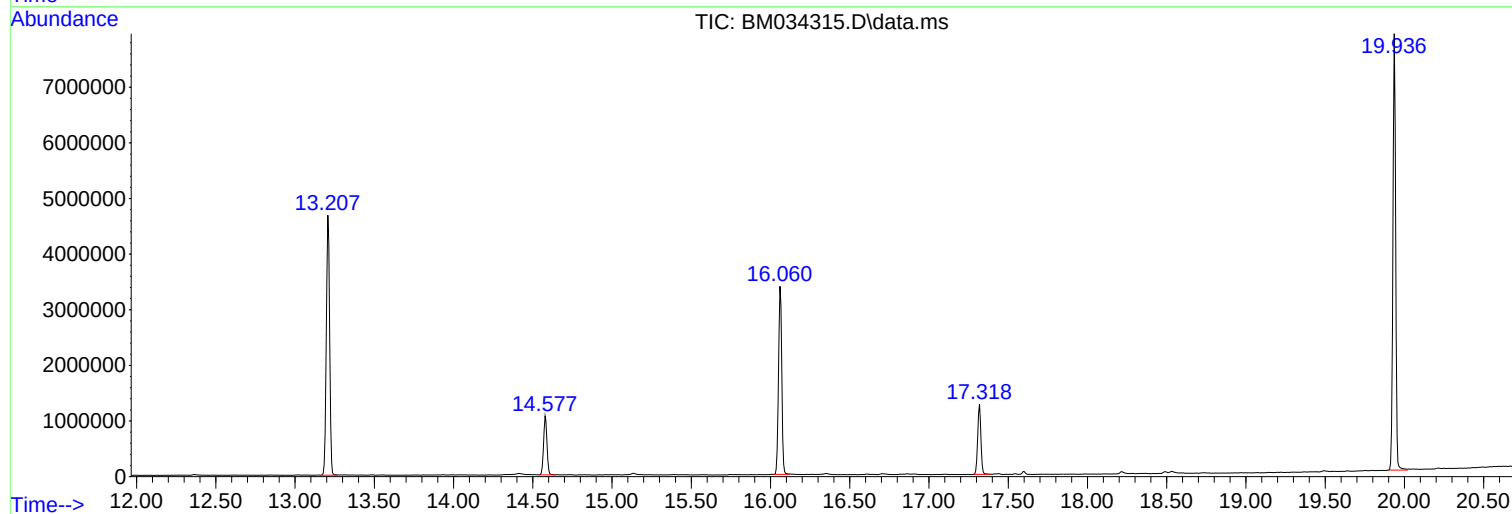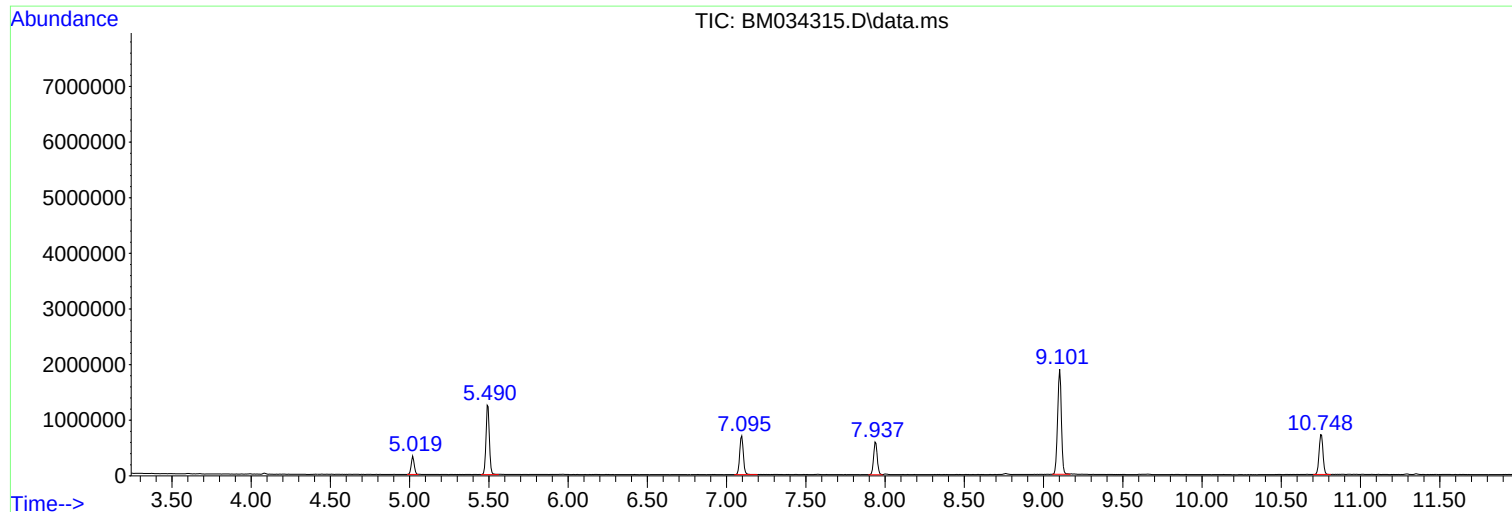

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034315.D
Acq On : 22 Mar 2022 18:13
Operator : CG/JU
Sample : N1977-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EB-20220315










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 2-Pentanone, 4-hydroxy-4-me... Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
5.019	9.41 ng	438596	1,4-Dichlorobenzene-d4	7.937

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	2-Pentanone, 4-hydroxy-4-methyl-	116	C6H12O2	000123-42-2	64		
2	1,3-Dioxolane-2-methanol, 2,4-di...	132	C6H12O3	053951-43-2	25		
3	2,3-Butanedione, monooxime	101	C4H7NO2	000057-71-6	25		
4	Acetic acid, cyano-, 1,1-dimethy...	141	C7H11NO2	001116-98-9	25		
5	Tetraglyme	222	C10H22O5	000143-24-8	25		

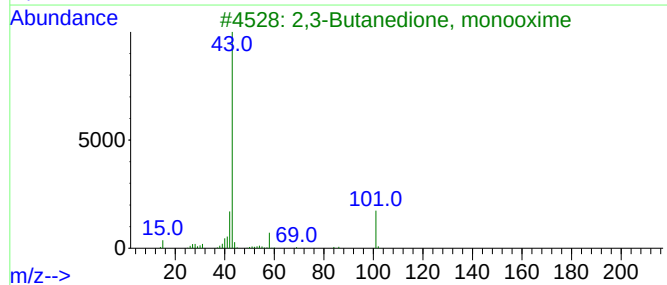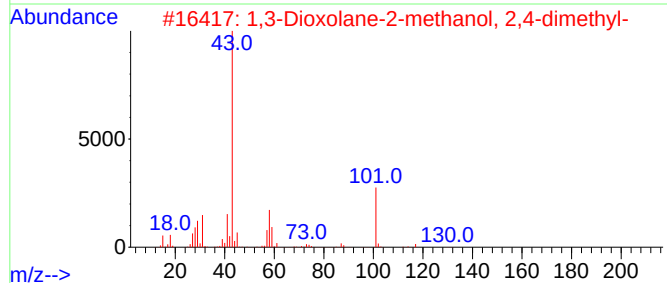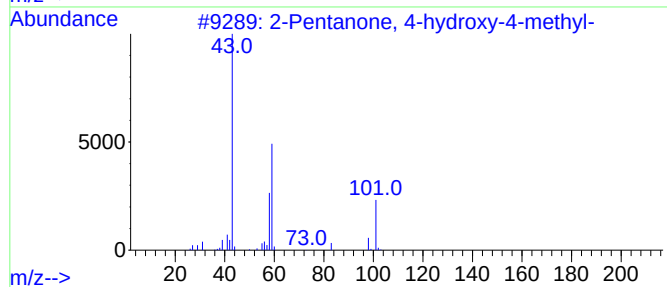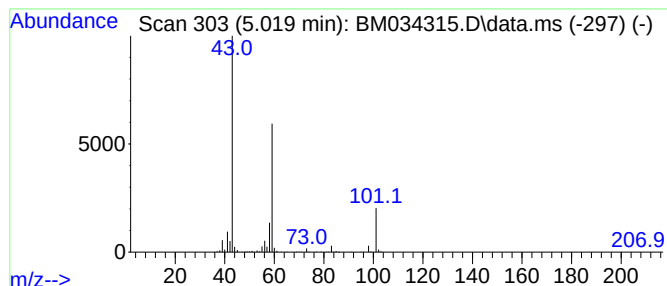

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034315.D
Acq On : 22 Mar 2022 18:13
Operator : CG/JU
Sample : N1977-08
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
EB-20220315

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
2-Pentanone, 4-...	5.019	9.4	ng	438596	1	7.937	931962	20.0