

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034320.D
 Acq On : 22 Mar 2022 21:15
 Operator : CG/JU
 Sample : N1962-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C-23-25-28

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034320.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	4.084	139	144	148	rBV	138563	190523	1.84%	0.141%
2	5.431	365	373	378	rBV	614504	885976	8.54%	0.653%
3	5.490	378	383	390	rBV	2654897	3896411	37.57%	2.874%
4	5.560	390	395	397	rBV	379434	535135	5.16%	0.395%
5	5.931	444	458	471	rBV4	248542	697436	6.72%	0.514%
6	6.419	536	541	549	rBV	109988	169775	1.64%	0.125%
7	6.919	618	626	634	rVB	78854	148687	1.43%	0.110%
8	7.025	639	644	649	rVV	132620	194940	1.88%	0.144%
9	7.095	649	656	663	rVV	2692546	4300108	41.46%	3.171%
10	7.160	663	667	674	rVB	68675	110397	1.06%	0.081%
11	7.331	690	696	700	rBV	82665	123325	1.19%	0.091%
12	7.589	732	740	750	rBV2	356927	681788	6.57%	0.503%
13	7.936	792	799	806	rBV	643427	1013032	9.77%	0.747%
14	8.060	814	820	827	rBV2	144524	270677	2.61%	0.200%
15	8.319	857	864	871	rBV	1714582	2646796	25.52%	1.952%
16	8.478	886	891	900	rVB	345662	590998	5.70%	0.436%
17	9.101	991	997	1007	rVB	1508500	2477001	23.88%	1.827%
18	10.001	1145	1150	1155	rVB	75859	115006	1.11%	0.085%
19	10.154	1170	1176	1185	rBV4	126324	346531	3.34%	0.256%
20	10.254	1185	1193	1204	rVB3	59781	199121	1.92%	0.147%
21	10.748	1268	1277	1281	rBV	809627	1452124	14.00%	1.071%
22	10.801	1281	1286	1295	rVB	2178401	3563565	34.36%	2.628%
23	10.919	1301	1306	1312	rVB2	70817	123198	1.19%	0.091%
24	12.413	1553	1560	1569	rVB	467670	760425	7.33%	0.561%
25	12.630	1591	1597	1605	rVB	389735	616977	5.95%	0.455%
26	13.207	1688	1695	1706	rVB	3535928	5060998	48.79%	3.732%
27	13.418	1726	1731	1736	rVB	123244	178559	1.72%	0.132%
28	13.742	1779	1786	1788	rBV2	104754	171877	1.66%	0.127%
29	13.901	1808	1813	1818	rBV	212443	353031	3.40%	0.260%
30	13.954	1818	1822	1828	rVB	135598	197019	1.90%	0.145%
31	14.136	1846	1853	1857	rBV2	110887	201450	1.94%	0.149%
32	14.301	1875	1881	1892	rVB2	172272	295574	2.85%	0.218%
33	14.577	1920	1928	1934	rBV	1160419	1754251	16.91%	1.294%
34	14.642	1934	1939	1945	rVV	562705	855382	8.25%	0.631%
35	14.977	1990	1996	2003	rVB	495933	771099	7.43%	0.569%
36	15.054	2004	2009	2014	rVB	90113	129954	1.25%	0.096%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034320.D
 Acq On : 22 Mar 2022 21:15
 Operator : CG/JU
 Sample : N1962-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C-23-25-28

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

37	15.195	2027	2033	2038	rBV	86054	157698	1.52%	0.116%
38	15.248	2038	2042	2046	rVB	76975	109990	1.06%	0.081%
39	15.365	2055	2062	2065	rBV5	93747	194432	1.87%	0.143%
40	15.618	2099	2105	2111	rBV	825413	1243606	11.99%	0.917%
41	15.783	2130	2133	2138	rVB3	102761	139681	1.35%	0.103%
42	15.836	2138	2142	2145	rBV4	78118	115562	1.11%	0.085%
43	15.918	2151	2156	2163	rVB	192829	346533	3.34%	0.256%
44	16.059	2174	2180	2188	rBV	3243794	4626070	44.60%	3.412%
45	16.295	2216	2220	2233	rVB5	122919	294679	2.84%	0.217%
46	16.624	2269	2276	2281	rVB3	148692	296341	2.86%	0.219%
47	16.671	2281	2284	2291	rBV2	83085	119349	1.15%	0.088%
48	16.777	2299	2302	2307	rVB2	84683	119373	1.15%	0.088%
49	16.854	2312	2315	2318	rVV2	84216	127025	1.22%	0.094%
50	16.971	2330	2335	2342	rVB	248375	381885	3.68%	0.282%
51	17.048	2345	2348	2350	rBV2	86213	115683	1.12%	0.085%
52	17.136	2359	2363	2372	rVB	396880	579768	5.59%	0.428%
53	17.318	2389	2394	2397	rBV	1302229	1893598	18.26%	1.396%
54	17.365	2397	2402	2408	rVV	6637353	9425473	90.87%	6.951%
55	17.454	2408	2417	2422	rVB	1076764	1686465	16.26%	1.244%
56	17.506	2422	2426	2432	rBV3	156558	274028	2.64%	0.202%
57	17.718	2454	2462	2467	rBV2	563579	964067	9.29%	0.711%
58	17.901	2490	2493	2501	rVB2	99616	146628	1.41%	0.108%
59	18.195	2539	2543	2548	rBV	562229	1113373	10.73%	0.821%
60	18.242	2548	2551	2559	rVB	859915	1238152	11.94%	0.913%
61	18.324	2561	2565	2570	rVV	235890	332017	3.20%	0.245%
62	18.395	2571	2577	2580	rVV3	971092	1743186	16.81%	1.286%
63	18.424	2580	2582	2588	rVB2	408981	521311	5.03%	0.384%
64	18.606	2610	2613	2616	rVB2	97572	110090	1.06%	0.081%
65	18.695	2624	2628	2631	rBV	433339	558051	5.38%	0.412%
66	18.730	2631	2634	2642	rVB	485846	637731	6.15%	0.470%
67	18.942	2667	2670	2674	rVB	157772	167646	1.62%	0.124%
68	19.071	2689	2692	2695	rBV	200381	255776	2.47%	0.189%
69	19.112	2695	2699	2703	rVV	296223	442101	4.26%	0.326%
70	19.248	2719	2722	2730	rBV2	201608	348136	3.36%	0.257%
71	19.377	2738	2744	2749	rBV	7757119	10221272	98.55%	7.538%
72	19.436	2749	2754	2758	rBV	1617559	1999035	19.27%	1.474%
73	19.618	2781	2785	2788	rBV	231968	290113	2.80%	0.214%
74	19.736	2795	2805	2813	rBV	6447972	10372007	100.00%	7.649%
75	19.806	2814	2817	2824	rVB2	295530	453051	4.37%	0.334%
76	19.936	2831	2839	2843	rBV	5204057	6458463	62.27%	4.763%

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034320.D
 Acq On : 22 Mar 2022 21:15
 Operator : CG/JU
 Sample : N1962-10
 Misc :
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 C-23-25-28

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
 Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

77	19.971	2843	2845	2850	rVB	359127	464737	4.48%	0.343%
78	20.059	2855	2860	2866	rBV3	299510	702719	6.78%	0.518%
79	20.153	2872	2876	2879	rBV	597031	767028	7.40%	0.566%
80	20.230	2885	2889	2895	rVB	812921	1126456	10.86%	0.831%
81	20.330	2902	2906	2909	rBV	629603	771298	7.44%	0.569%
82	20.383	2912	2915	2920	rVB2	442034	650476	6.27%	0.480%
83	20.524	2936	2939	2943	rBV	263586	329675	3.18%	0.243%
84	20.571	2944	2947	2951	rVB	314323	401799	3.87%	0.296%
85	20.971	3012	3015	3022	rVB	243096	405157	3.91%	0.299%
86	21.136	3041	3043	3047	rVB	273366	295628	2.85%	0.218%
87	21.177	3047	3050	3052	rBV	424364	487034	4.70%	0.359%
88	21.206	3052	3055	3061	rVB3	414828	839470	8.09%	0.619%
89	21.265	3061	3065	3067	rBV2	412464	611048	5.89%	0.451%
90	21.477	3097	3101	3107	rBV3	3601610	6621022	63.84%	4.883%
91	21.530	3107	3110	3120	rVB	2839075	3720348	35.87%	2.744%
92	21.653	3127	3131	3137	rVB	461518	661935	6.38%	0.488%
93	21.812	3155	3158	3164	rVB2	365153	526828	5.08%	0.389%
94	23.171	3383	3389	3395	rBV	2033878	5228051	50.41%	3.856%
95	23.353	3417	3420	3429	rVB	361817	622951	6.01%	0.459%
96	23.694	3472	3478	3487	rVB	1320901	2765474	26.66%	2.039%
97	23.800	3489	3496	3504	rBV	1868724	3916648	37.76%	2.888%
98	23.906	3508	3514	3519	rBV2	985652	1886927	18.19%	1.392%
99	26.418	3933	3941	3954	rVB2	910925	2902462	27.98%	2.141%
100	27.188	4065	4072	4085	rVB	692676	2193479	21.15%	1.618%




Sum of corrected areas: 135597241

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034320.D
Acq On : 22 Mar 2022 21:15
Operator : CG/JU
Sample : N1962-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-23-25-28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

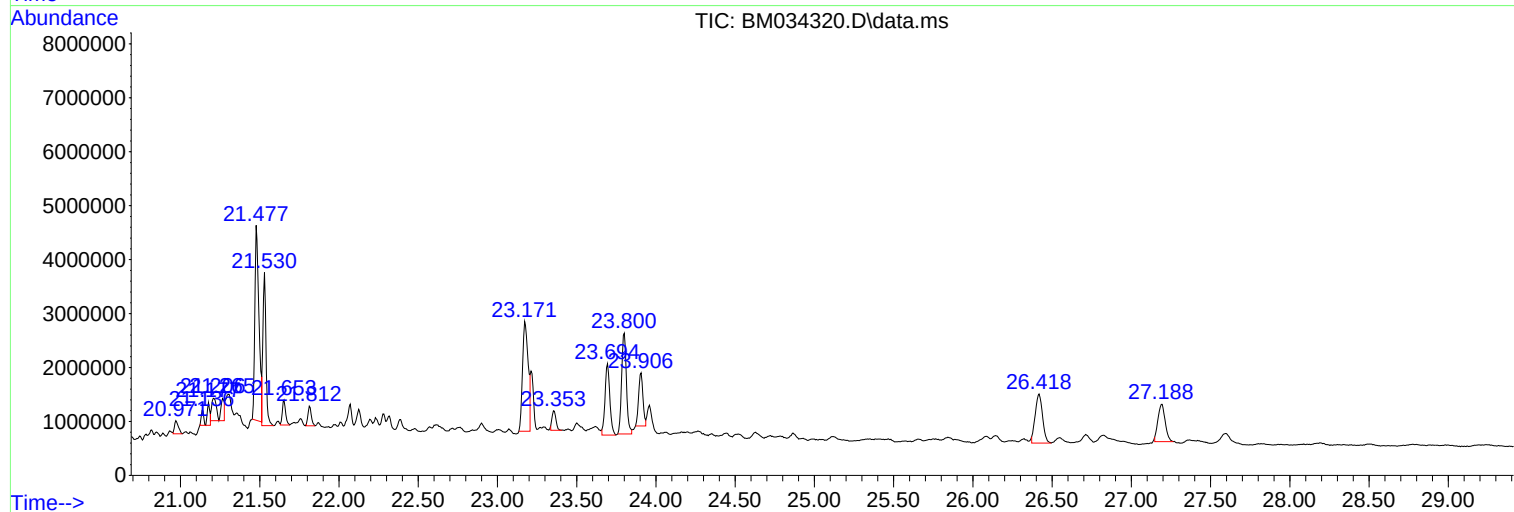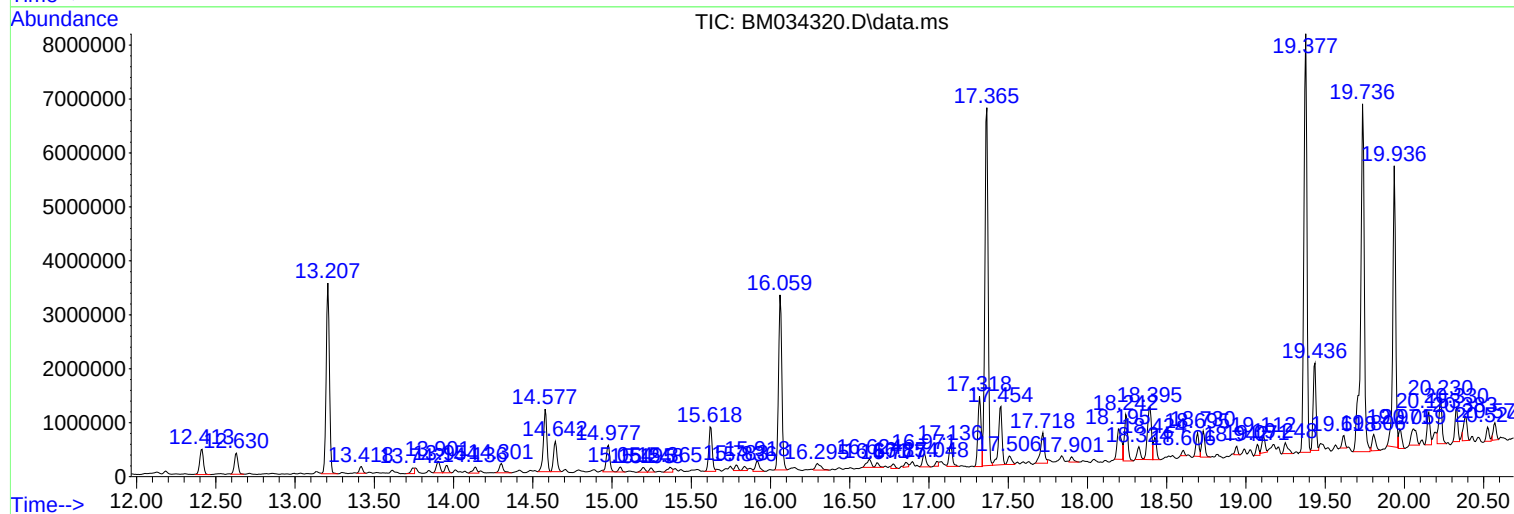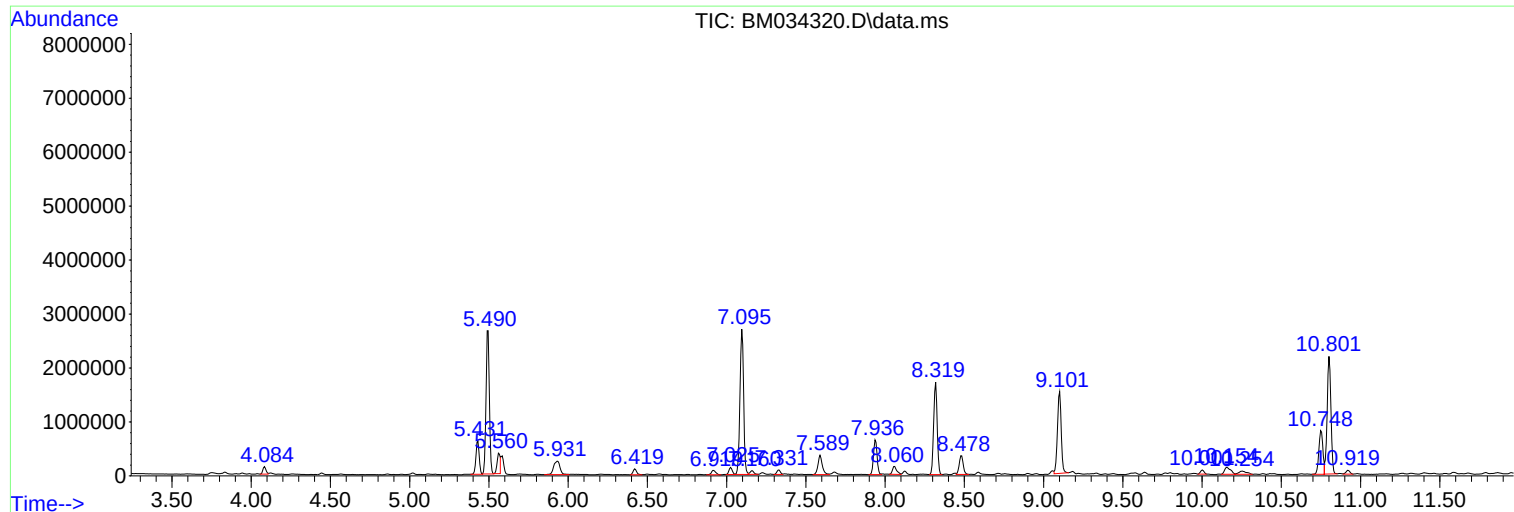

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034320.D
Acq On : 22 Mar 2022 21:15
Operator : CG/JU
Sample : N1962-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-23-25-28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

No Library Search Compounds Detected

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034320.D
Acq On : 22 Mar 2022 21:15
Operator : CG/JU
Sample : N1962-10
Misc :
ALS Vial : 10 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
C-23-25-28

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library :
TIC Integration Parameters: rteint.p

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------