

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
 Data File : BM034325.D
 Acq On : 23 Mar 2022 00:16
 Operator : CG/JU
 Sample : N1949-12
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 BNA_M
 ClientSampleId :
 CP-BH1-031422-0-2

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M

Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

Signal : TIC: BM034325.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	5.496	377	384	395	rBV	2262403	3341359	54.40%	9.620%
2	7.095	648	656	672	rBV	2280377	3591077	58.46%	10.339%
3	7.937	792	799	807	rBV	670970	1067631	17.38%	3.074%
4	9.101	987	997	1014	rBV	1341409	2273098	37.01%	6.545%
5	10.748	1270	1277	1286	rBV	820870	1426974	23.23%	4.108%
6	13.207	1688	1695	1707	rBV	3280106	4739224	77.16%	13.645%
7	14.407	1890	1899	1908	rBV3	24883	66462	1.08%	0.191%
8	14.577	1922	1928	1940	rVB	1193948	1782036	29.01%	5.131%
9	16.060	2174	2180	2193	rBV	2545405	3714872	60.48%	10.696%
10	17.318	2388	2394	2405	rBV	1361366	1947779	31.71%	5.608%
11	18.212	2541	2546	2555	rBV	109708	190053	3.09%	0.547%
12	19.371	2739	2743	2752	rBV	56276	96700	1.57%	0.278%
13	19.936	2833	2839	2849	rBV	5052801	6142304	100.00%	17.685%
14	21.195	3050	3053	3060	rBV	302201	368365	6.00%	1.061%
15	21.489	3098	3103	3115	rBV	1437818	1988435	32.37%	5.725%
16	23.900	3507	3513	3524	rVB2	969107	1996026	32.50%	5.747%




Sum of corrected areas: 34732395

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034325.D
Acq On : 23 Mar 2022 00:16
Operator : CG/JU
Sample : N1949-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CP-BH1-031422-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

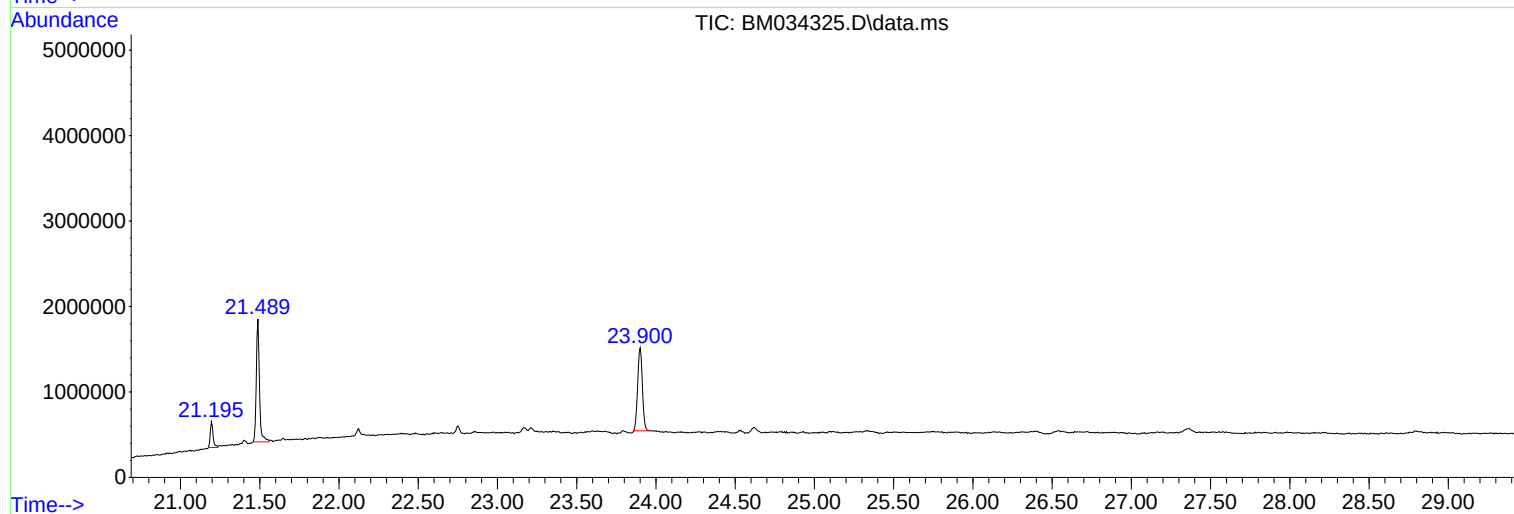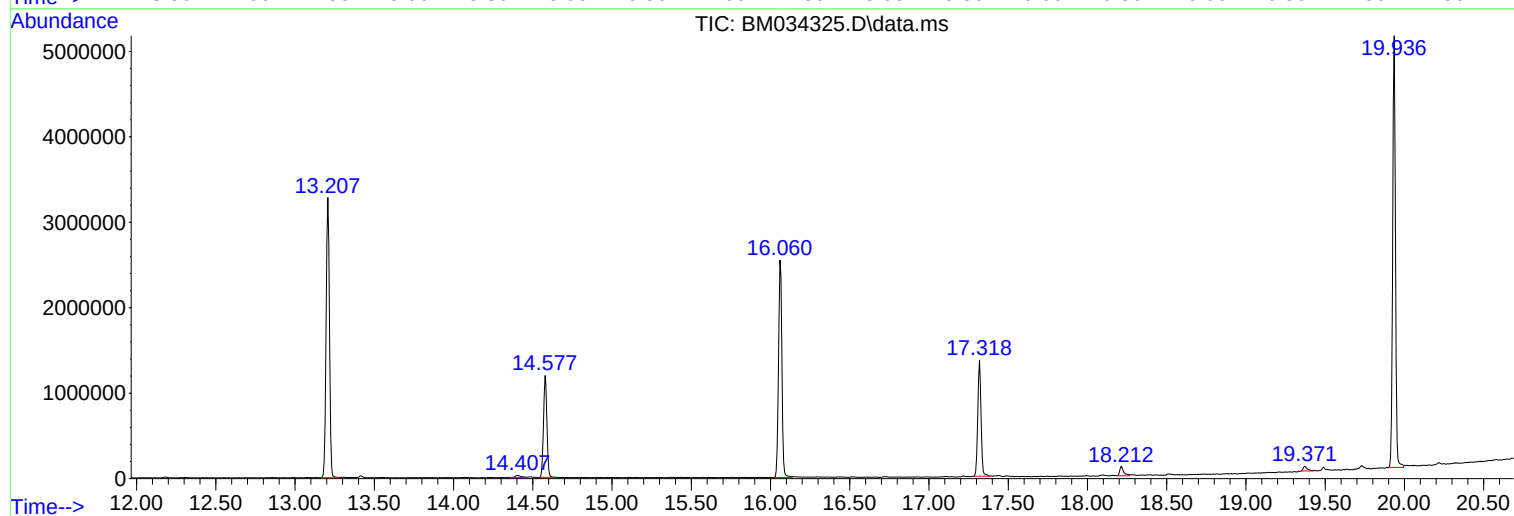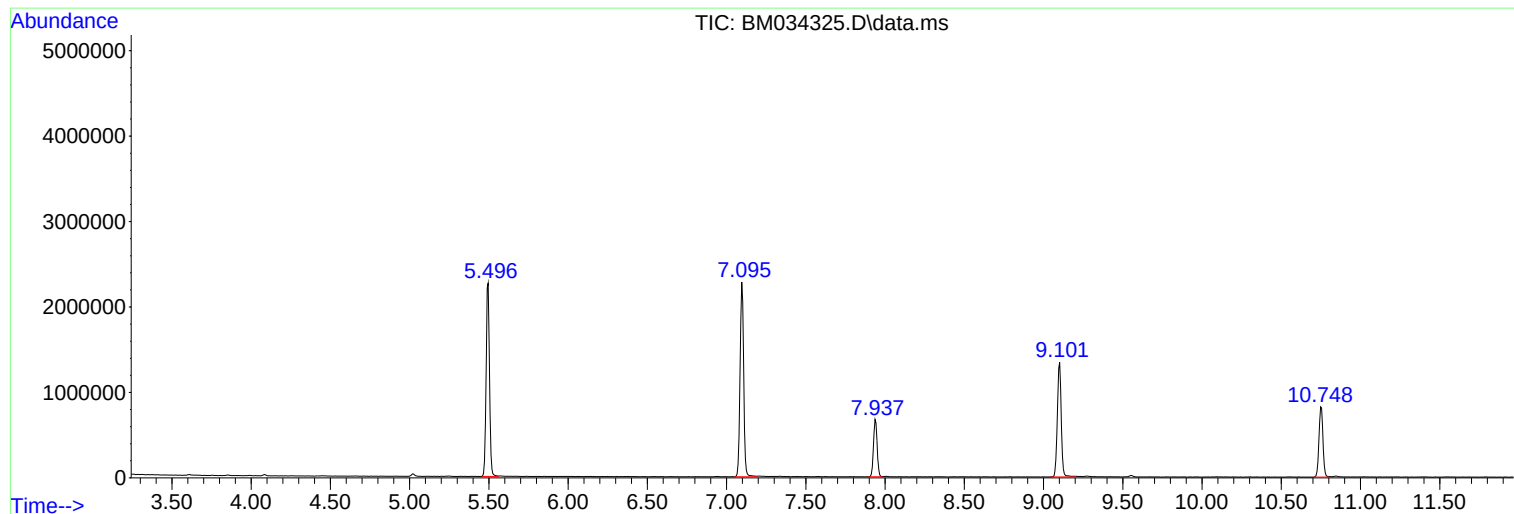

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034325.D
Acq On : 23 Mar 2022 00:16
Operator : CG/JU
Sample : N1949-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CP-BH1-031422-0-2










Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 1-Hexacosene Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
21.195	3.71 ng	368365	Chrysene-d12	21.489

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1	1-Hexacosene			364	C26H52	018835-33-1	99
2	9-Tricosene, (Z)-			322	C23H46	027519-02-4	99
3	5-Eicosene, (E)-			280	C20H40	074685-30-6	99
4	Heptacos-1-ene			378	C27H54	015306-27-1	96
5	Pentacos-1-ene			350	C25H50	016980-85-1	96

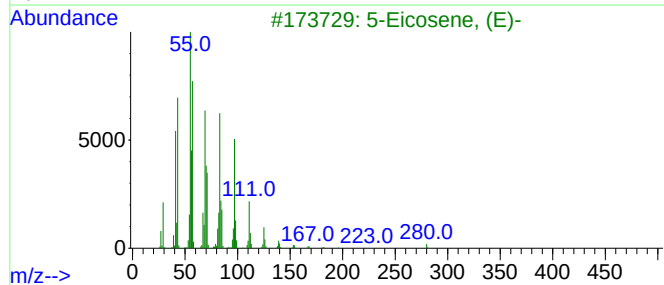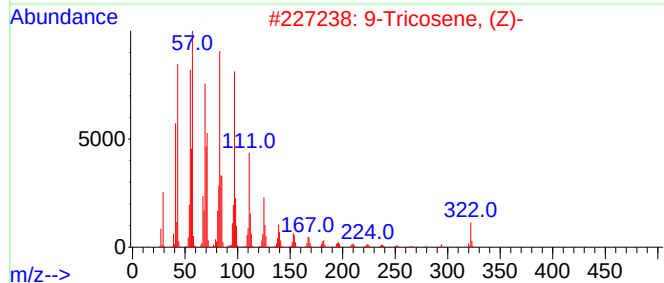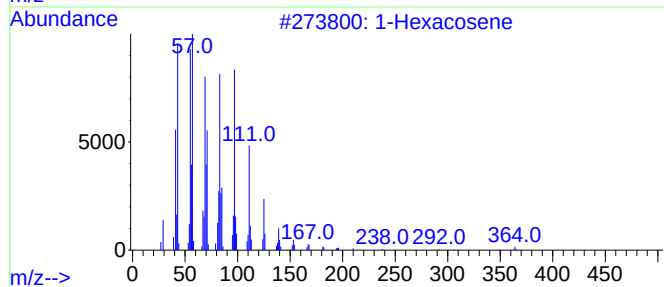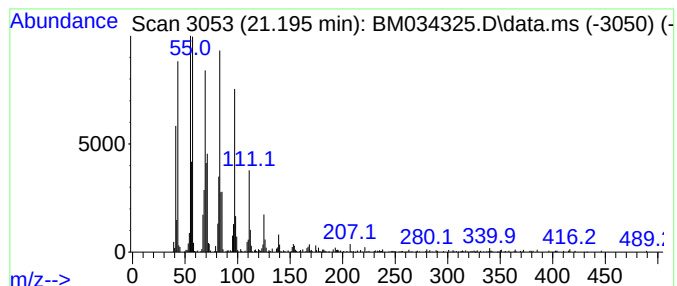

Data Path : Z:\svoasrv\HPCHEM1\BNA_M\Data\BM032222\
Data File : BM034325.D
Acq On : 23 Mar 2022 00:16
Operator : CG/JU
Sample : N1949-12
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
BNA_M
ClientSampleId :
CP-BH1-031422-0-2

Quant Method : Z:\svoasrv\HPCHEM1\BNA_M\Methods\8270-BM031522.M
Quant Title : ASP BNA STANDARDS FOR 5 POINT CALIBRATION

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
1-Hexacosene	21.195	3.7	ng	368365	5	21.489	1988440	20.0